




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079025.D
Acq On : 24 May 2024 18:52
Operator : RP/MD
Sample : P2577-16
Misc : 4.71G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BHBP9

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

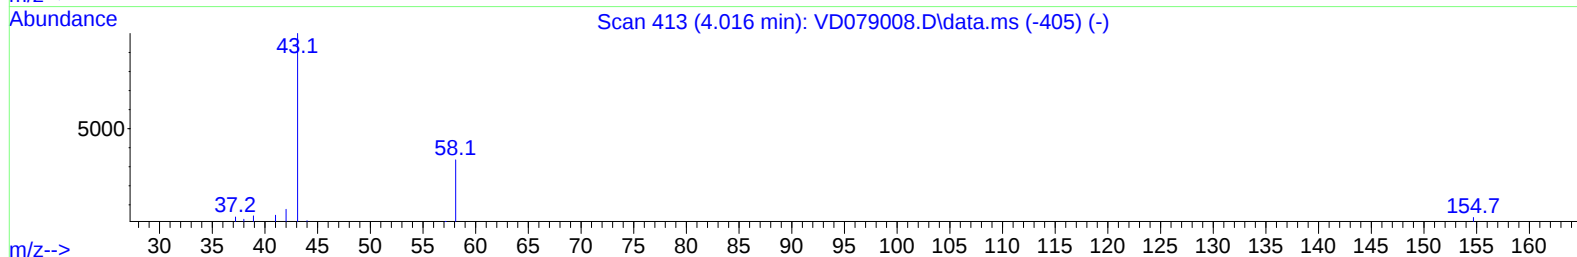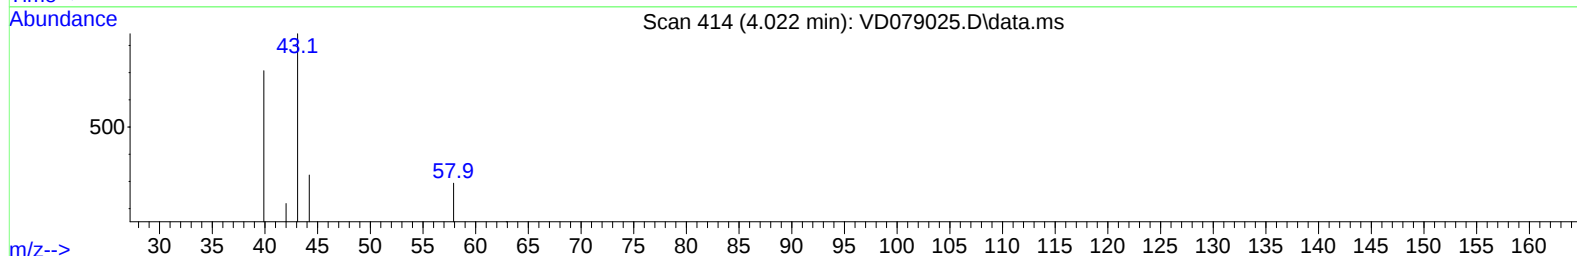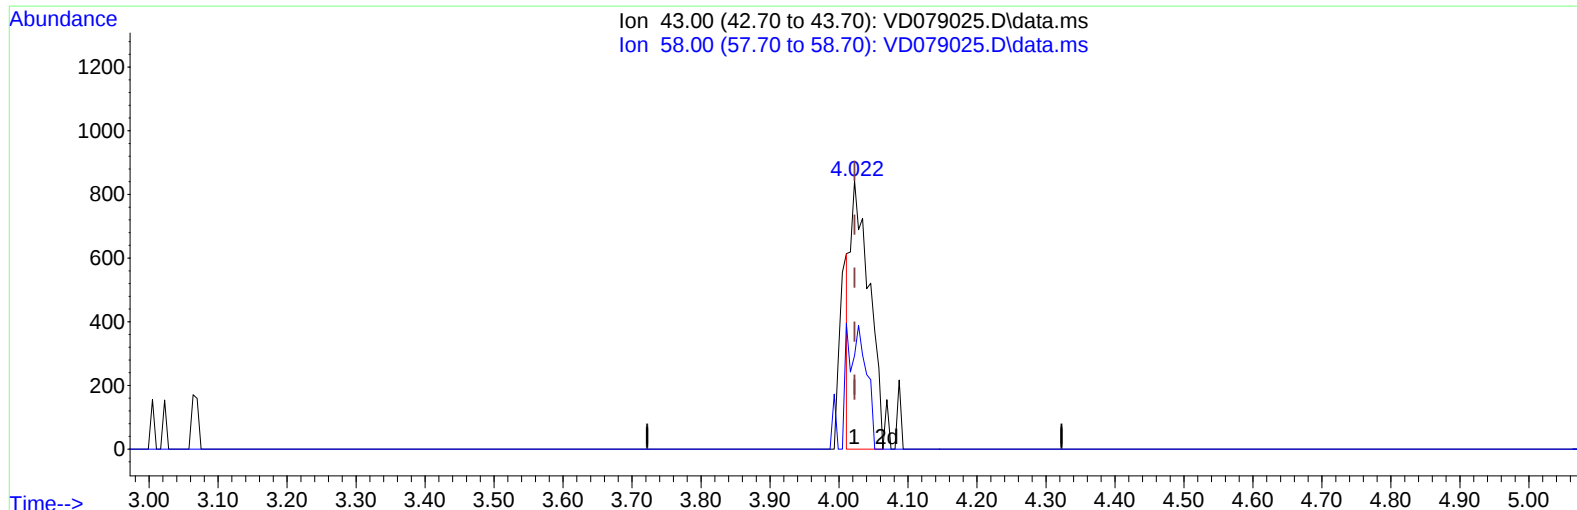

TIC: VD079025.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 4.40 ug/L

response	1598	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.50	31.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079025.D
Acq On : 24 May 2024 18:52
Operator : RP/MD
Sample : P2577-16
Misc : 4.71G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BHBP9

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

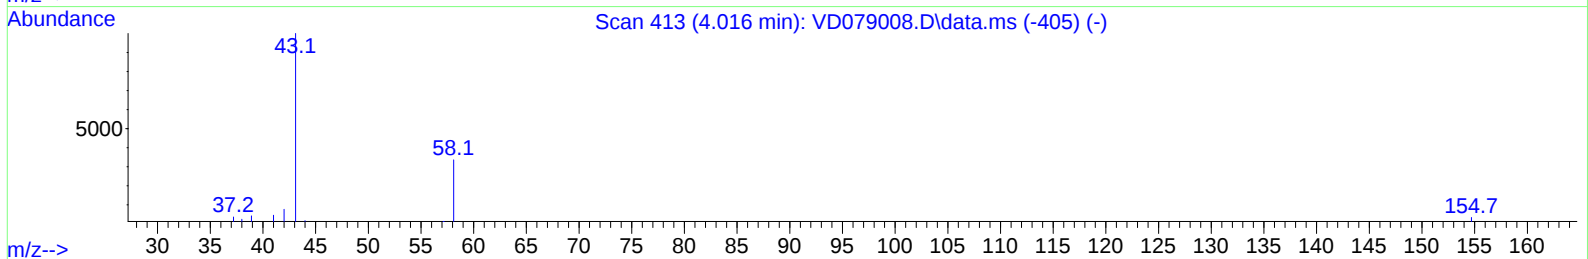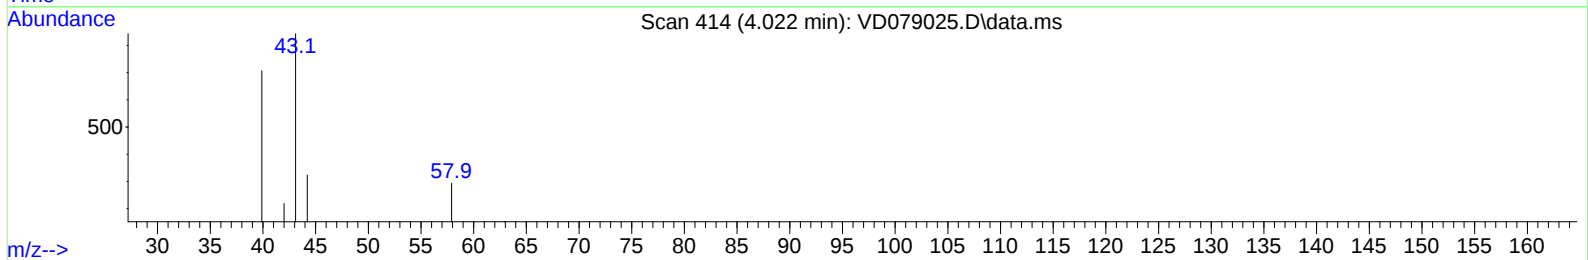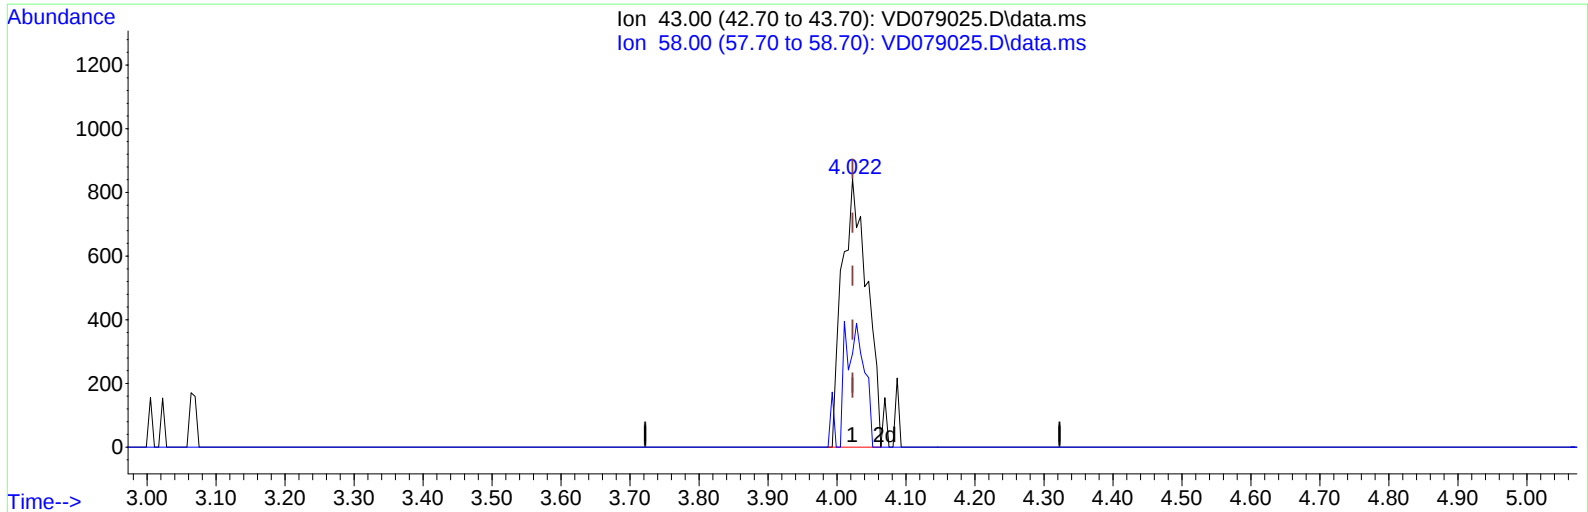

TIC: VD079025.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 5.81 ug/L m

response 2110

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.50	23.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
 Data File : VD079025.D
 Acq On : 24 May 2024 18:52
 Operator : RP/MD
 Sample : P2577-16
 Misc : 4.71G/10ml/MSVOA_D/SOIL/VIAL A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BHBP9

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 02:12:30 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
 Supervised By :Semsettin Yesilyurt 05/30/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	86571	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	78593	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	22415	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.270	65	48262	22.741	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.960%		
7) Chloroethane-d5	2.799	69	47284	20.814	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.240%		
11) 1,1-Dichloroethene-d2	3.917	65	6261	15.124	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.480%		
21) 2-Butanone-d5	6.981	46	14226	47.359	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.720%		
24) Chloroform-d	7.569	84	41394	16.062	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	64.240%		
26) 1,2-Dichloroethane-d4	8.234	65	26927	22.001	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.000%		
32) Benzene-d6	8.205	84	76434	19.060	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.240%		
36) 1,2-Dichloropropane-d6	9.205	67	26576	21.750	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	87.000%		
41) Toluene-d8	10.269	98	55431	14.996	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	60.000%		
43) trans-1,3-Dichloroprop...	10.522	79	9950	17.678	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	70.720%		
47) 2-Hexanone-d5	10.875	63	9549	38.993	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.980%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	30620	22.029	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.120%		
66) 1,2-Dichlorobenzene-d4	13.816	152	12960	17.035	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	68.120%#		
Target Compounds					Qvalue	
13) Acetone	4.022	43	2110m	5.815	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079025.D
Acq On : 24 May 2024 18:52
Operator : RP/MD
Sample : P2577-16
Misc : 4.71G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BHBP9

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

Quant Time: May 24 23:27:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

