




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079029.D
Acq On : 24 May 2024 20:43
Operator : RP/MD
Sample : P2577-01
Misc : 5.24G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH639

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

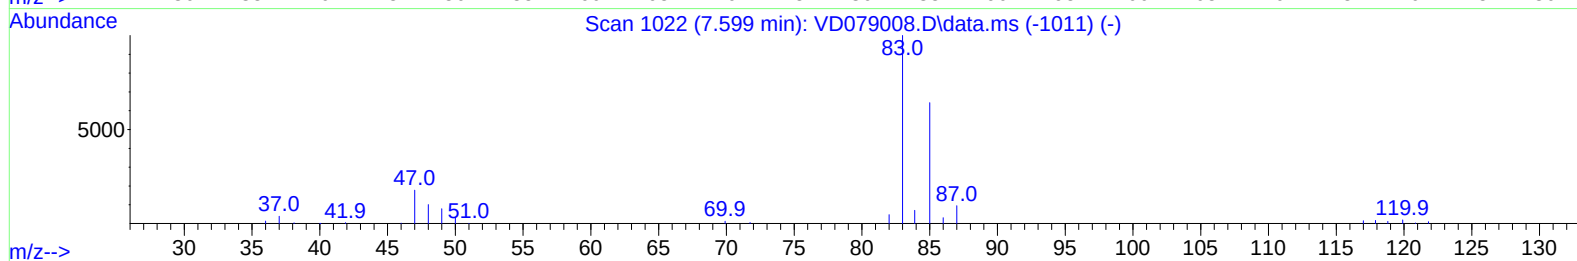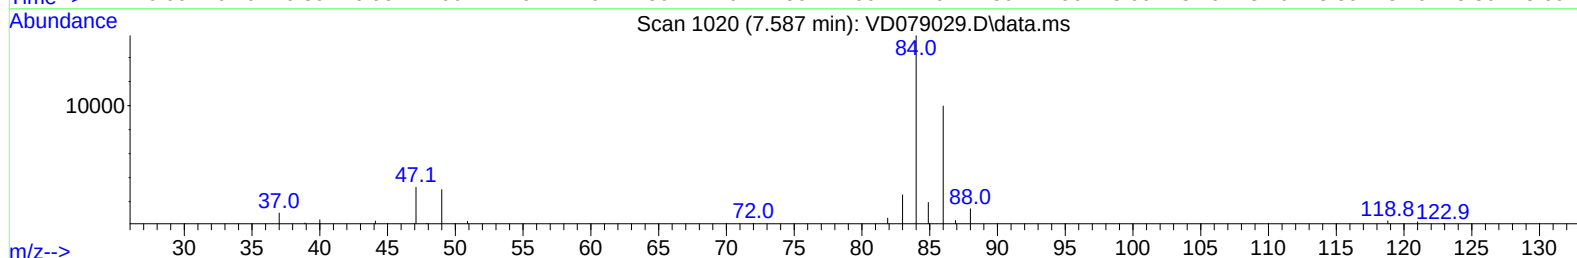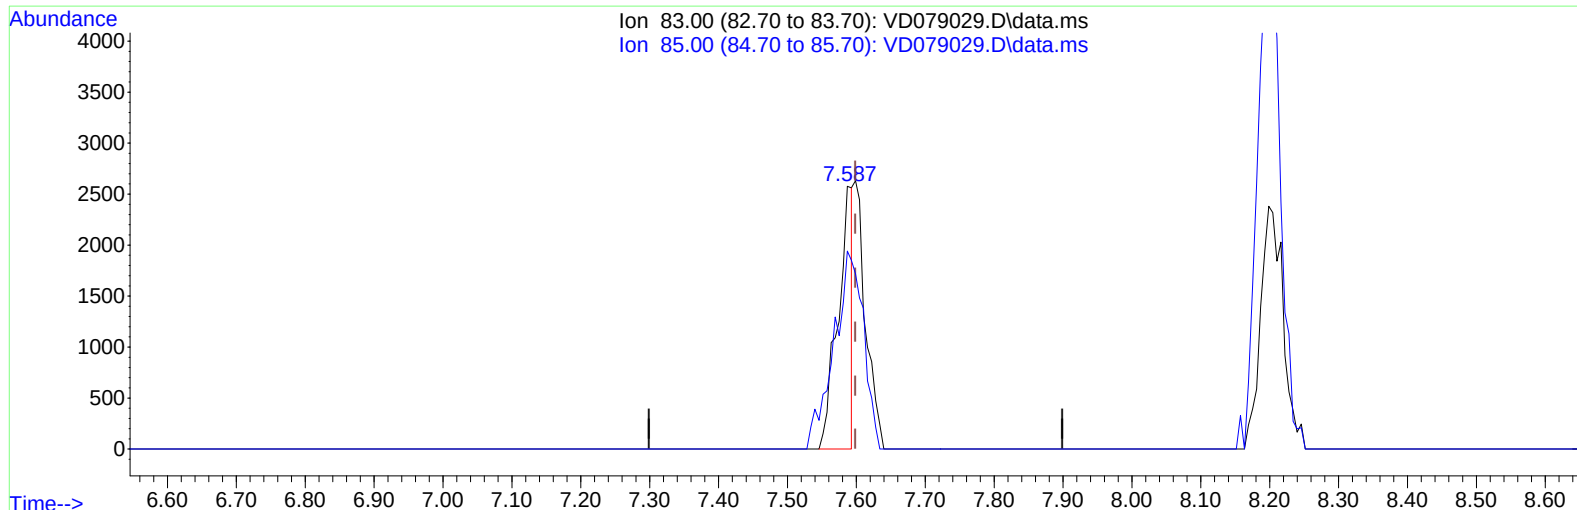

TIC: VD079029.D\data.ms

(25) Chloroform (T)

7.587min (-0.012) 0.57 ug/L

response 3825

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	59.70	75.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079029.D
Acq On : 24 May 2024 20:43
Operator : RP/MD
Sample : P2577-01
Misc : 5.24G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH639

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

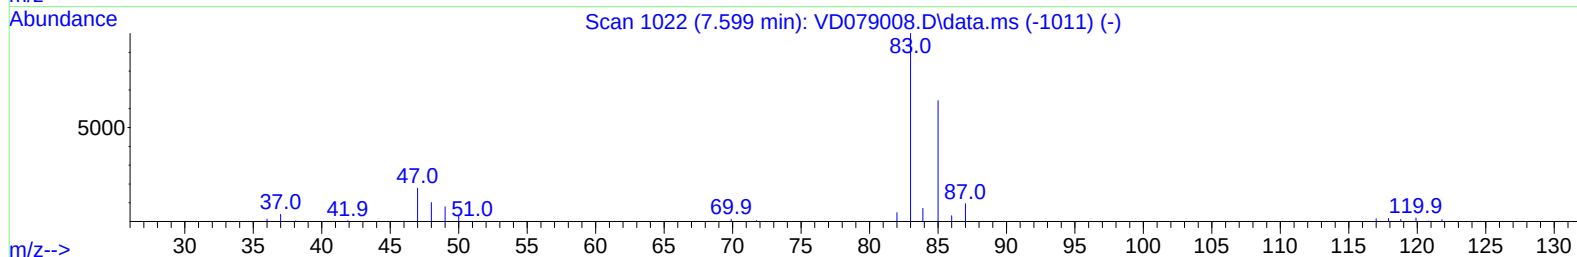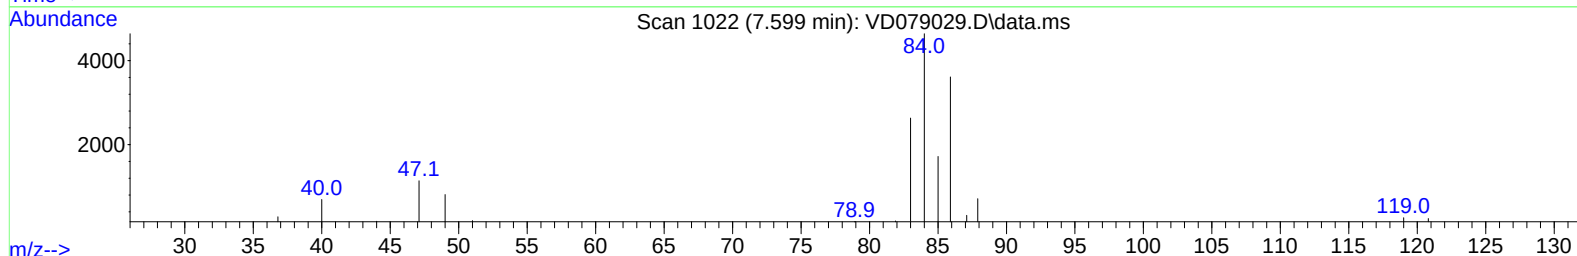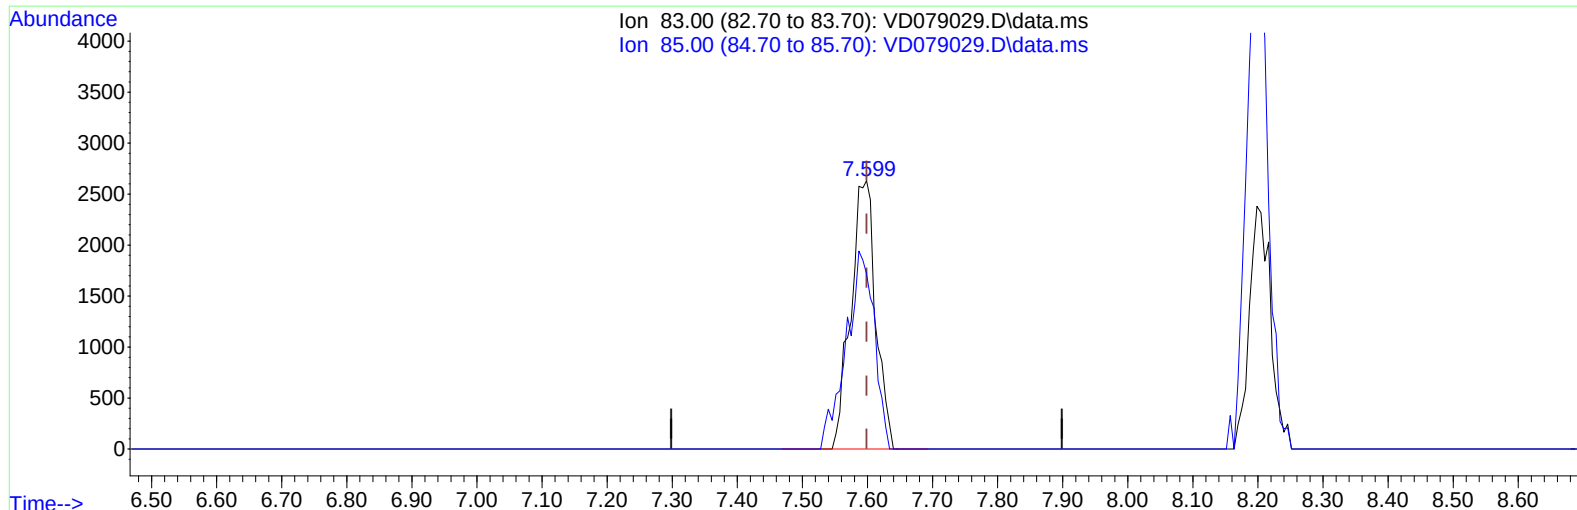

TIC: VD079029.D\data.ms

(25) Chloroform (T)

7.599min (-0.000) 1.05 ug/L m

response 6987

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	59.70	65.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
 Data File : VD079029.D
 Acq On : 24 May 2024 20:43
 Operator : RP/MD
 Sample : P2577-01
 Misc : 5.24G/10ml/MSVOA_D/SOIL/VIAL A
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH639

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/30/2024
 Supervised By :Semsettin Yesilyurt 05/30/2024

Quant Time: May 24 23:27:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 02:12:30 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene		8.775	114	187789	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.581	117	169202	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.516	152	54472	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.269	65	118658	25.775	ug/L	0.00
Spiked Amount	25.000	Range 30	- 150	Recovery	=	103.120%	
7) Chloroethane-d5		2.799	69	114413	23.218	ug/L	0.00
Spiked Amount	25.000	Range 30	- 150	Recovery	=	92.880%	
11) 1,1-Dichloroethene-d2		3.905	65	16811	18.721	ug/L	-0.01
Spiked Amount	25.000	Range 45	- 110	Recovery	=	74.880%	
21) 2-Butanone-d5		6.987	46	15547	23.860	ug/L	0.00
Spiked Amount	50.000	Range 20	- 135	Recovery	=	47.720%	
24) Chloroform-d		7.563	84	88498	15.830	ug/L	0.00
Spiked Amount	25.000	Range 40	- 150	Recovery	=	63.320%	
26) 1,2-Dichloroethane-d4		8.228	65	48302	18.194	ug/L	0.00
Spiked Amount	25.000	Range 70	- 130	Recovery	=	72.760%	
32) Benzene-d6		8.199	84	178777	20.707	ug/L	0.00
Spiked Amount	25.000	Range 20	- 135	Recovery	=	82.840%	
36) 1,2-Dichloropropane-d6		9.204	67	54467	20.705	ug/L	0.00
Spiked Amount	25.000	Range 70	- 120	Recovery	=	82.840%	
41) Toluene-d8		10.269	98	144867	18.204	ug/L	0.00
Spiked Amount	25.000	Range 30	- 130	Recovery	=	72.800%	
43) trans-1,3-Dichloroprop...		10.528	79	20670	17.058	ug/L	0.00
Spiked Amount	25.000	Range 30	- 135	Recovery	=	68.240%	
47) 2-Hexanone-d5		10.875	63	10983	20.832	ug/L	0.00
Spiked Amount	50.000	Range 20	- 135	Recovery	=	41.660%	
56) 1,1,2,2-Tetrachloroeth...		12.645	84	47222	15.780	ug/L	0.00
Spiked Amount	25.000	Range 45	- 120	Recovery	=	63.120%	
66) 1,2-Dichlorobenzene-d4		13.810	152	32944	17.819	ug/L	0.00
Spiked Amount	25.000	Range 75	- 120	Recovery	=	71.280%#	
Target Compounds							Qvalue
16) Methylene chloride		4.793	84	11728	2.637	ug/L	96
25) Chloroform		7.599	83	6987m	1.047	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079029.D
Acq On : 24 May 2024 20:43
Operator : RP/MD
Sample : P2577-01
Misc : 5.24G/10ml/MSVOA_D/SOIL/VIAL A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH639

Manual IntegrationsAPPROVED

Quant Time: May 24 23:27:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/30/2024
Supervised By :Semsettin Yesilyurt 05/30/2024

