
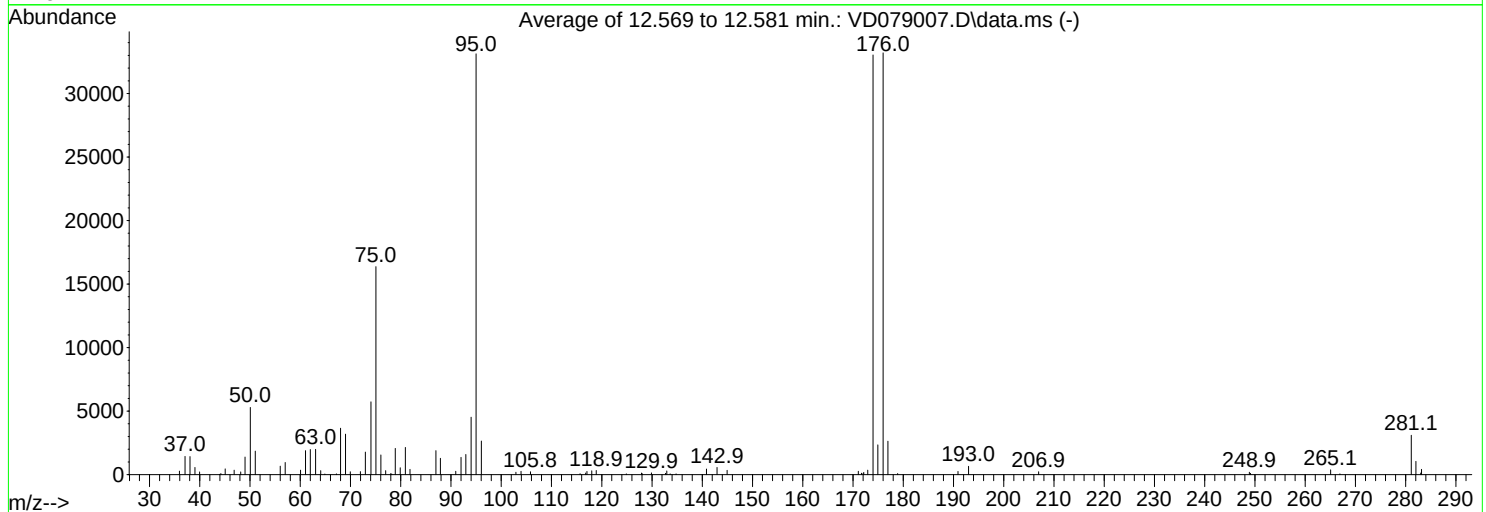


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052424\
Data File : VD079007.D
Acq On : 24 May 2024 08:12
Operator : RP/MD
Sample : BFB215
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB215

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Title : SFAM01.0
Last Update : Fri May 24 02:12:30 2024

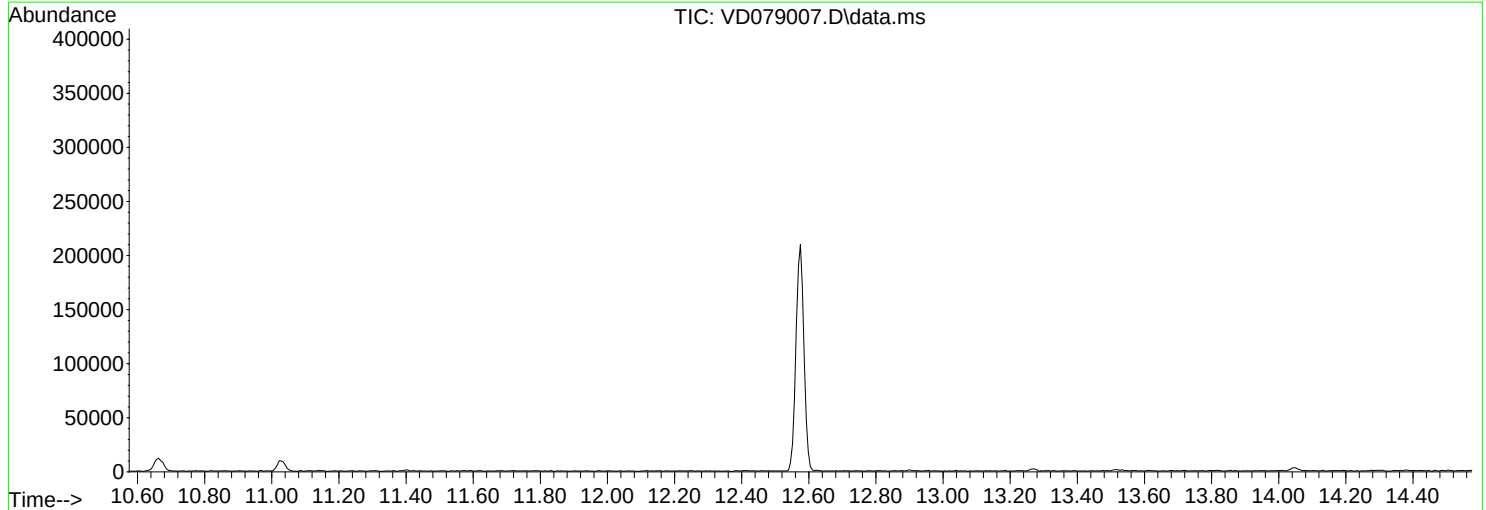

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	5290	PASS
75	95	30	80	49.4	16369	PASS
95	95	100	100	100.0	33123	PASS
96	95	5	9	8.0	2641	PASS
173	174	0.00	2	1.1	348	PASS
174	95	50	120	99.7	33040	PASS
175	174	5	9	7.1	2346	PASS
176	174	95	105	100.5	33203	PASS
177	176	5	10	7.9	2633	PASS

m/z	Abundance
40.00	529.0
44.00	317.0

Instrument :
MSVOA_D
ClientSampleId :
BFB215

m/z	Abundance
36.00	235.0
37.10	1492.0
38.00	1472.0
39.00	517.0
40.10	891.0
43.90	397.0
45.10	367.0
46.80	241.0
48.20	261.0
49.00	1341.0
50.10	5905.0
51.00	1706.0
55.90	849.0
57.00	1401.0
60.10	205.0
61.10	1851.0
62.00	2342.0
63.00	1742.0
64.00	349.0
67.20	179.0
68.00	3842.0
69.00	2838.0
69.90	295.0
72.00	317.0
73.00	1576.0
74.10	5986.0
75.10	16512.0
76.10	1571.0
77.00	408.0
78.90	2078.0
79.90	418.0
80.90	2385.0
81.90	521.0
87.00	1814.0
87.90	1543.0
90.90	208.0
92.00	1540.0
93.00	1516.0
94.00	4236.0
95.00	34888.0
96.10	2954.0
102.80	161.0
103.90	252.0
105.80	296.0
115.70	233.0
117.10	476.0
118.10	395.0
118.90	363.0
128.00	191.0
129.90	217.0
132.70	308.0
133.60	201.0
140.80	370.0
143.00	618.0
145.00	400.0
171.10	252.0
172.00	306.0
173.10	472.0
174.00	32304.0
175.00	2065.0
176.00	32016.0
177.00	3016.0
190.90	189.0
193.10	615.0
248.90	347.0
265.00	314.0
281.10	1802.0
282.00	506.0
283.00	393.0

Instrument :
MSVOA_D
ClientSampleId :
BFB215

m/z	Abundance
35.80	232.0
37.00	1204.0
38.10	1565.0
39.10	613.0
39.90	631.0
43.80	264.0
44.20	276.0
45.00	604.0
46.90	383.0
48.10	198.0
49.00	1434.0
50.10	5415.0
51.00	1989.0
56.00	752.0
57.00	917.0
60.00	376.0
61.00	2078.0
62.00	1600.0
63.10	2655.0
64.10	313.0
68.00	4513.0
69.00	4004.0
70.00	402.0
71.80	207.0
73.00	2272.0
74.10	6429.0
75.00	17776.0
76.00	1703.0
77.00	193.0
78.00	263.0
78.90	2584.0
79.90	586.0
80.90	2111.0
81.90	368.0
87.00	2087.0
87.90	1340.0
91.00	240.0
92.00	1336.0
92.90	1779.0
94.00	4730.0
95.00	36376.0
96.00	3078.0
102.90	201.0
104.00	328.0
105.80	375.0
116.80	365.0
118.00	275.0
118.90	347.0
127.80	189.0
132.90	527.0
140.80	512.0
142.90	639.0
144.90	278.0
171.10	257.0
172.20	182.0
172.90	379.0
174.00	36640.0
174.90	2813.0
176.00	36848.0
177.00	2907.0
190.80	391.0
193.00	895.0
207.00	494.0
248.90	233.0
265.10	430.0
266.90	183.0
281.10	3765.0
282.10	1185.0
283.20	608.0

Instrument :
MSVOA_D
ClientSampleId :
BFB215

m/z	Abundance
36.00	379.0
37.00	1614.0
38.00	1221.0
39.00	579.0
39.90	720.0
43.90	361.0
45.10	383.0
46.90	454.0
48.10	205.0
49.00	1400.0
50.00	4551.0
51.10	1858.0
56.10	388.0
57.10	570.0
60.10	484.0
61.00	1744.0
62.00	1973.0
63.00	1577.0
64.10	273.0
64.90	157.0
68.00	2617.0
69.00	2727.0
72.00	206.0
72.90	1463.0
74.00	4774.0
75.00	14819.0
76.00	1362.0
76.90	178.0
77.10	174.0
78.20	162.0
79.00	1523.0
79.90	636.0
80.90	1919.0
81.80	352.0
87.00	1764.0
87.90	979.0
90.90	345.0
92.00	1215.0
93.00	1477.0
94.00	4583.0
95.00	28104.0
96.00	1892.0
103.00	194.0
104.00	216.0
117.00	271.0
117.90	235.0
118.90	292.0
124.90	193.0
128.10	186.0
129.90	188.0
133.00	349.0
134.80	198.0
140.90	450.0
142.90	445.0
145.00	348.0
171.00	273.0
171.70	351.0
172.10	337.0
172.80	193.0
174.00	30176.0
174.90	2159.0
176.00	30744.0
176.90	1977.0
178.90	279.0
191.00	191.0
192.90	467.0
206.90	189.0
249.10	320.0
265.10	395.0
281.10	3722.0
282.10	1435.0
283.10	639.0

Instrument :
MSVOA_D
ClientSampleId :
BFB215