


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD052819\
Data File : VD062534.D
Acq On : 28 May 2019 10:33
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D052019S.M
Title : SW846 8260
Last Update : Tue May 21 03:32:39 2019

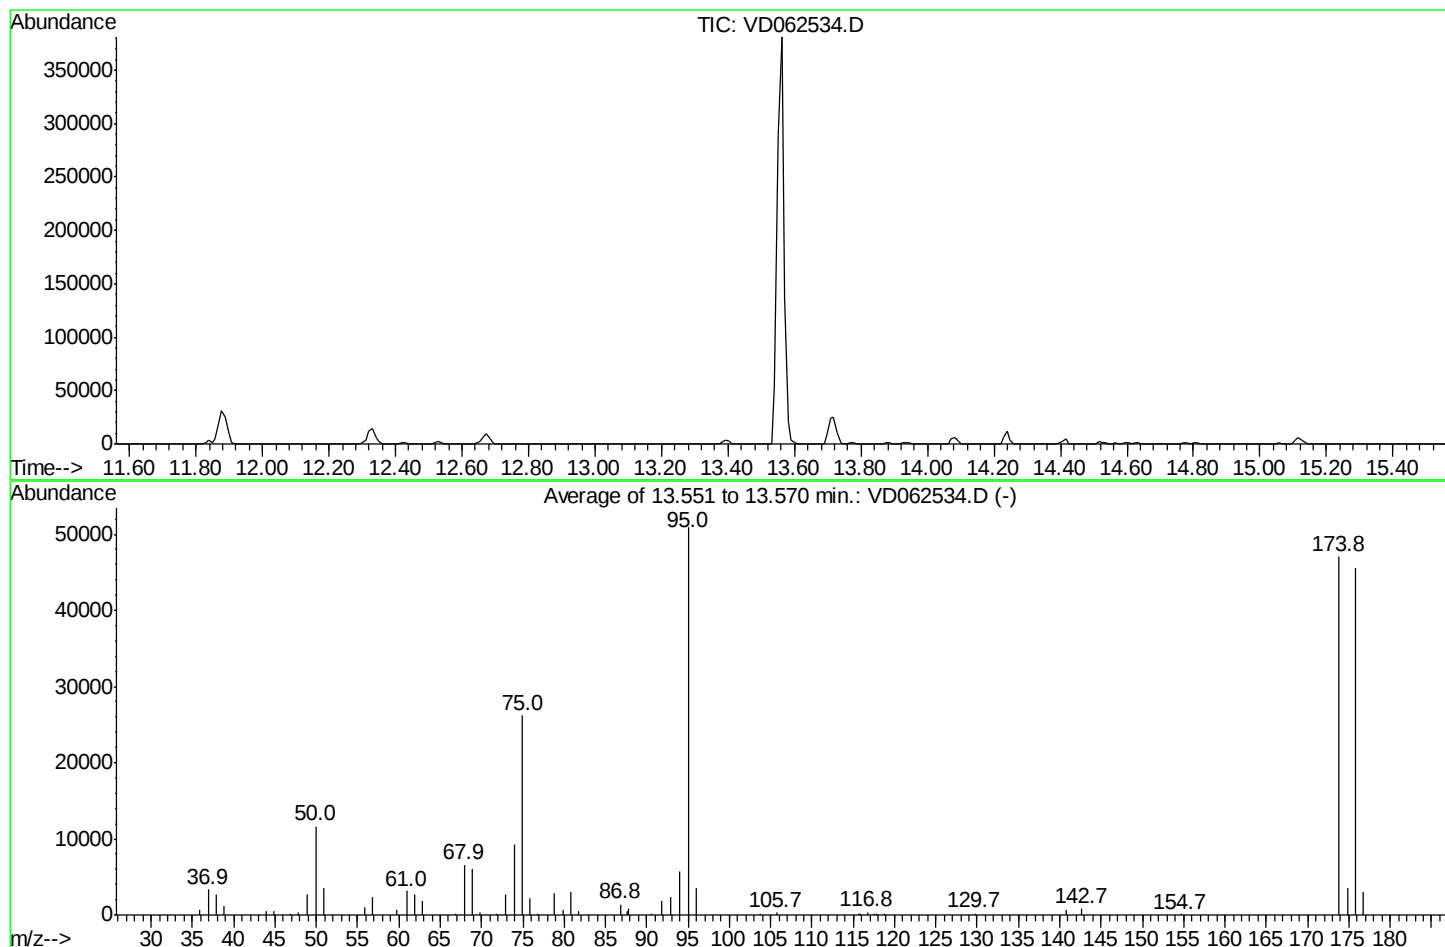

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	11604	PASS
75	95	30	60	51.5	26218	PASS
95	95	100	100	100.0	50906	PASS
96	95	5	9	7.1	3594	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.3	46986	PASS
175	174	5	9	7.4	3480	PASS
176	174	95	101	97.1	45632	PASS
177	176	5	9	6.6	3032	PASS