
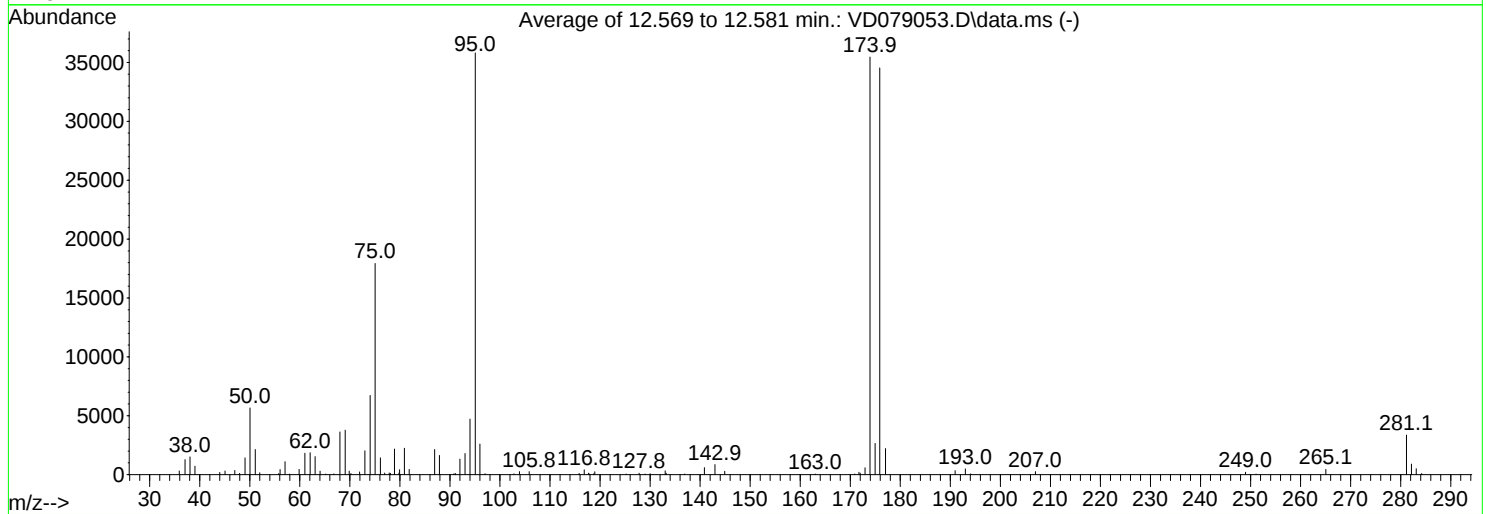


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052924\
Data File : VD079053.D
Acq On : 29 May 2024 08:25
Operator : RP/MD
Sample : BFB801
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB801

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Fri May 31 01:52:18 2024

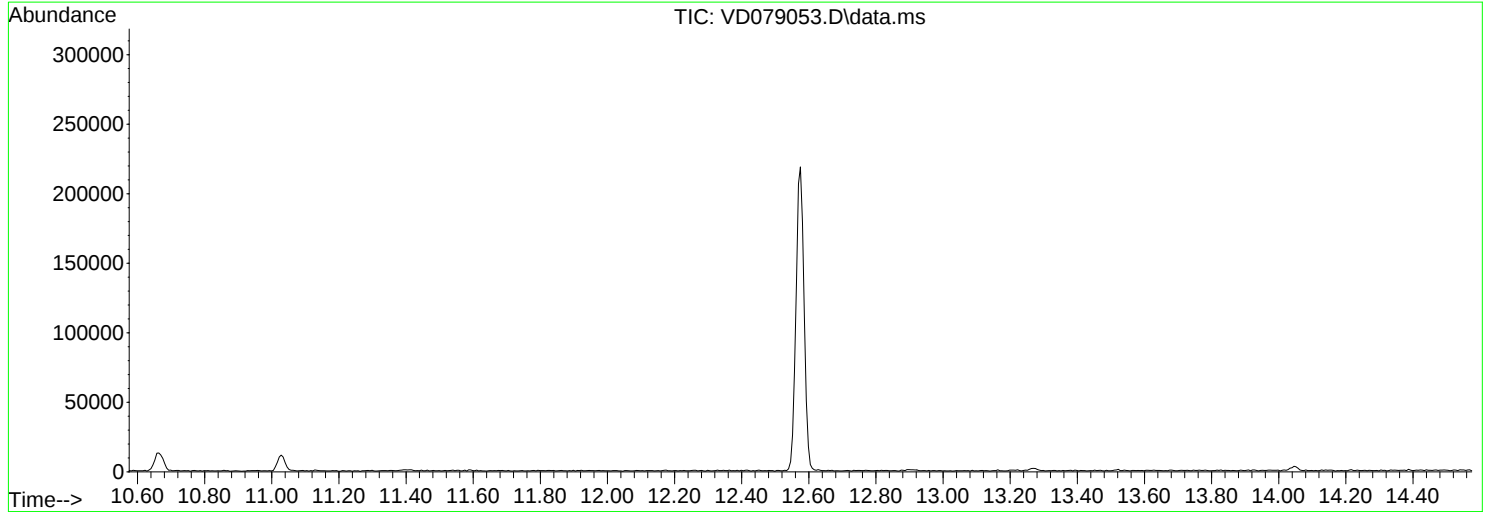

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	5669	PASS
75	95	30	80	50.1	17937	PASS
95	95	100	100	100.0	35816	PASS
96	95	5	9	7.3	2598	PASS
173	174	0.00	2	1.6	579	PASS
174	95	50	120	99.0	35464	PASS
175	174	5	9	7.5	2652	PASS
176	174	95	105	97.4	34536	PASS
177	176	5	10	6.4	2213	PASS

m/z	Abundance
40.00	803.0
44.00	327.0

Instrument :
MSVOA_D
ClientSampleId :
BFB801

m/z	Abundance
36.00	161.0
37.00	1267.0
38.00	1826.0
39.00	651.0
40.10	466.0
44.10	519.0
45.00	243.0
47.00	261.0
49.00	1254.0
50.00	6024.0
51.10	2226.0
52.00	324.0
56.00	657.0
57.10	1140.0
57.90	152.0
59.80	473.0
61.00	1917.0
62.10	1706.0
63.00	1686.0
64.00	310.0
68.00	3789.0
69.00	4503.0
69.90	411.0
72.00	184.0
73.00	1899.0
74.10	6999.0
75.00	19096.0
76.10	1600.0
77.00	269.0
77.90	236.0
78.90	2772.0
79.80	394.0
80.90	2416.0
82.00	365.0
87.00	2282.0
87.90	1610.0
90.80	249.0
92.00	1303.0
93.00	1724.0
94.00	5215.0
95.10	37848.0
96.00	2648.0
102.80	223.0
103.90	185.0
105.90	394.0
115.80	170.0
116.90	572.0
119.00	309.0
125.20	162.0
127.80	151.0
133.00	470.0
140.80	620.0
143.00	959.0
144.90	259.0
171.70	203.0
172.90	685.0
173.90	36544.0
175.00	3000.0
175.90	33664.0
177.00	2062.0
190.90	344.0
193.00	419.0
194.10	214.0
207.00	231.0
265.00	256.0
281.10	2815.0
282.20	698.0
283.10	362.0

Instrument :
MSVOA_D
ClientSampleId :
BFB801

m/z	Abundance
35.90	506.0
37.10	1515.0
38.00	1432.0
39.00	879.0
40.00	686.0
44.00	603.0
45.10	446.0
47.10	354.0
48.00	151.0
49.10	1693.0
50.10	6750.0
51.10	2496.0
52.00	170.0
56.10	659.0
57.00	1522.0
59.90	454.0
61.00	1844.0
62.10	2088.0
63.10	1856.0
64.00	372.0
66.80	194.0
68.00	4089.0
69.10	3815.0
69.80	174.0
70.20	274.0
71.90	272.0
73.00	2349.0
74.10	7971.0
75.00	19328.0
76.10	1481.0
76.90	160.0
77.80	204.0
78.90	2140.0
80.00	616.0
80.90	2475.0
81.80	461.0
87.00	1858.0
87.90	1706.0
91.10	281.0
92.10	1577.0
93.00	1873.0
94.00	4823.0
95.00	38648.0
96.00	2903.0
103.90	262.0
105.80	220.0
115.80	176.0
116.80	341.0
117.70	356.0
118.90	410.0
133.00	496.0
136.90	167.0
140.90	540.0
142.90	990.0
145.00	390.0
163.00	158.0
170.90	183.0
171.80	422.0
173.00	637.0
174.00	37744.0
174.90	2905.0
175.90	37512.0
177.00	2734.0
191.00	275.0
193.00	469.0
207.00	240.0
249.00	251.0
265.10	511.0
281.10	3182.0
282.10	999.0
283.10	613.0

Instrument :
MSVOA_D
ClientSampleId :
BFB801

m/z	Abundance
35.90	277.0
37.00	1047.0
38.10	1259.0
39.10	652.0
40.10	893.0
43.90	434.0
45.10	257.0
46.90	429.0
47.90	175.0
49.00	1335.0
50.10	4234.0
51.10	1690.0
55.80	290.0
57.00	630.0
59.90	439.0
61.00	1689.0
61.90	1798.0
63.10	1062.0
64.10	234.0
65.20	180.0
68.00	3022.0
69.00	3037.0
69.90	309.0
72.00	240.0
73.00	1845.0
74.00	5226.0
75.10	15386.0
76.10	1198.0
78.10	327.0
78.90	1605.0
79.90	642.0
80.90	1816.0
81.80	534.0
86.90	2246.0
87.90	1581.0
91.90	1093.0
93.00	1785.0
94.00	4095.0
95.00	30952.0
96.00	2243.0
97.00	242.0
103.90	318.0
105.90	152.0
116.90	301.0
117.90	175.0
118.70	197.0
127.80	200.0
129.00	166.0
130.00	230.0
133.20	350.0
140.90	625.0
142.90	609.0
144.80	228.0
172.00	356.0
173.00	414.0
174.00	32104.0
175.00	2052.0
175.90	32432.0
177.10	1844.0
191.00	403.0
193.00	567.0
207.00	294.0
249.00	363.0
251.10	161.0
265.10	591.0
281.20	4054.0
282.10	997.0
283.10	537.0
284.20	269.0

Instrument :
MSVOA_D
ClientSampleId :
BFB801