

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD053122\
 Data File : VD073424.D
 Acq On : 31 May 2022 14:43
 Operator : VA/SY
 Sample : VD0531SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0531SBL01

Quant Time: May 31 17:42:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
 Quant Title : SW846 8260
 QLast Update : Thu May 19 15:13:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	380471	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.856	114	666022	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	681751	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	328276	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	195083	46.396	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.800%
35) Dibromofluoromethane	7.909	113	210338	47.860	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.720%
50) Toluene-d8	10.332	98	772882	47.707	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	95.420%
62) 4-Bromofluorobenzene	12.620	95	316581	55.683	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD053122\
Data File : VD073424.D
Acq On : 31 May 2022 14:43
Operator : VA/SY
Sample : VD0531SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0531SBL01

Quant Time: May 31 17:42:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
Quant Title : SW846 8260
QLast Update : Thu May 19 15:13:42 2022
Response via : Initial Calibration




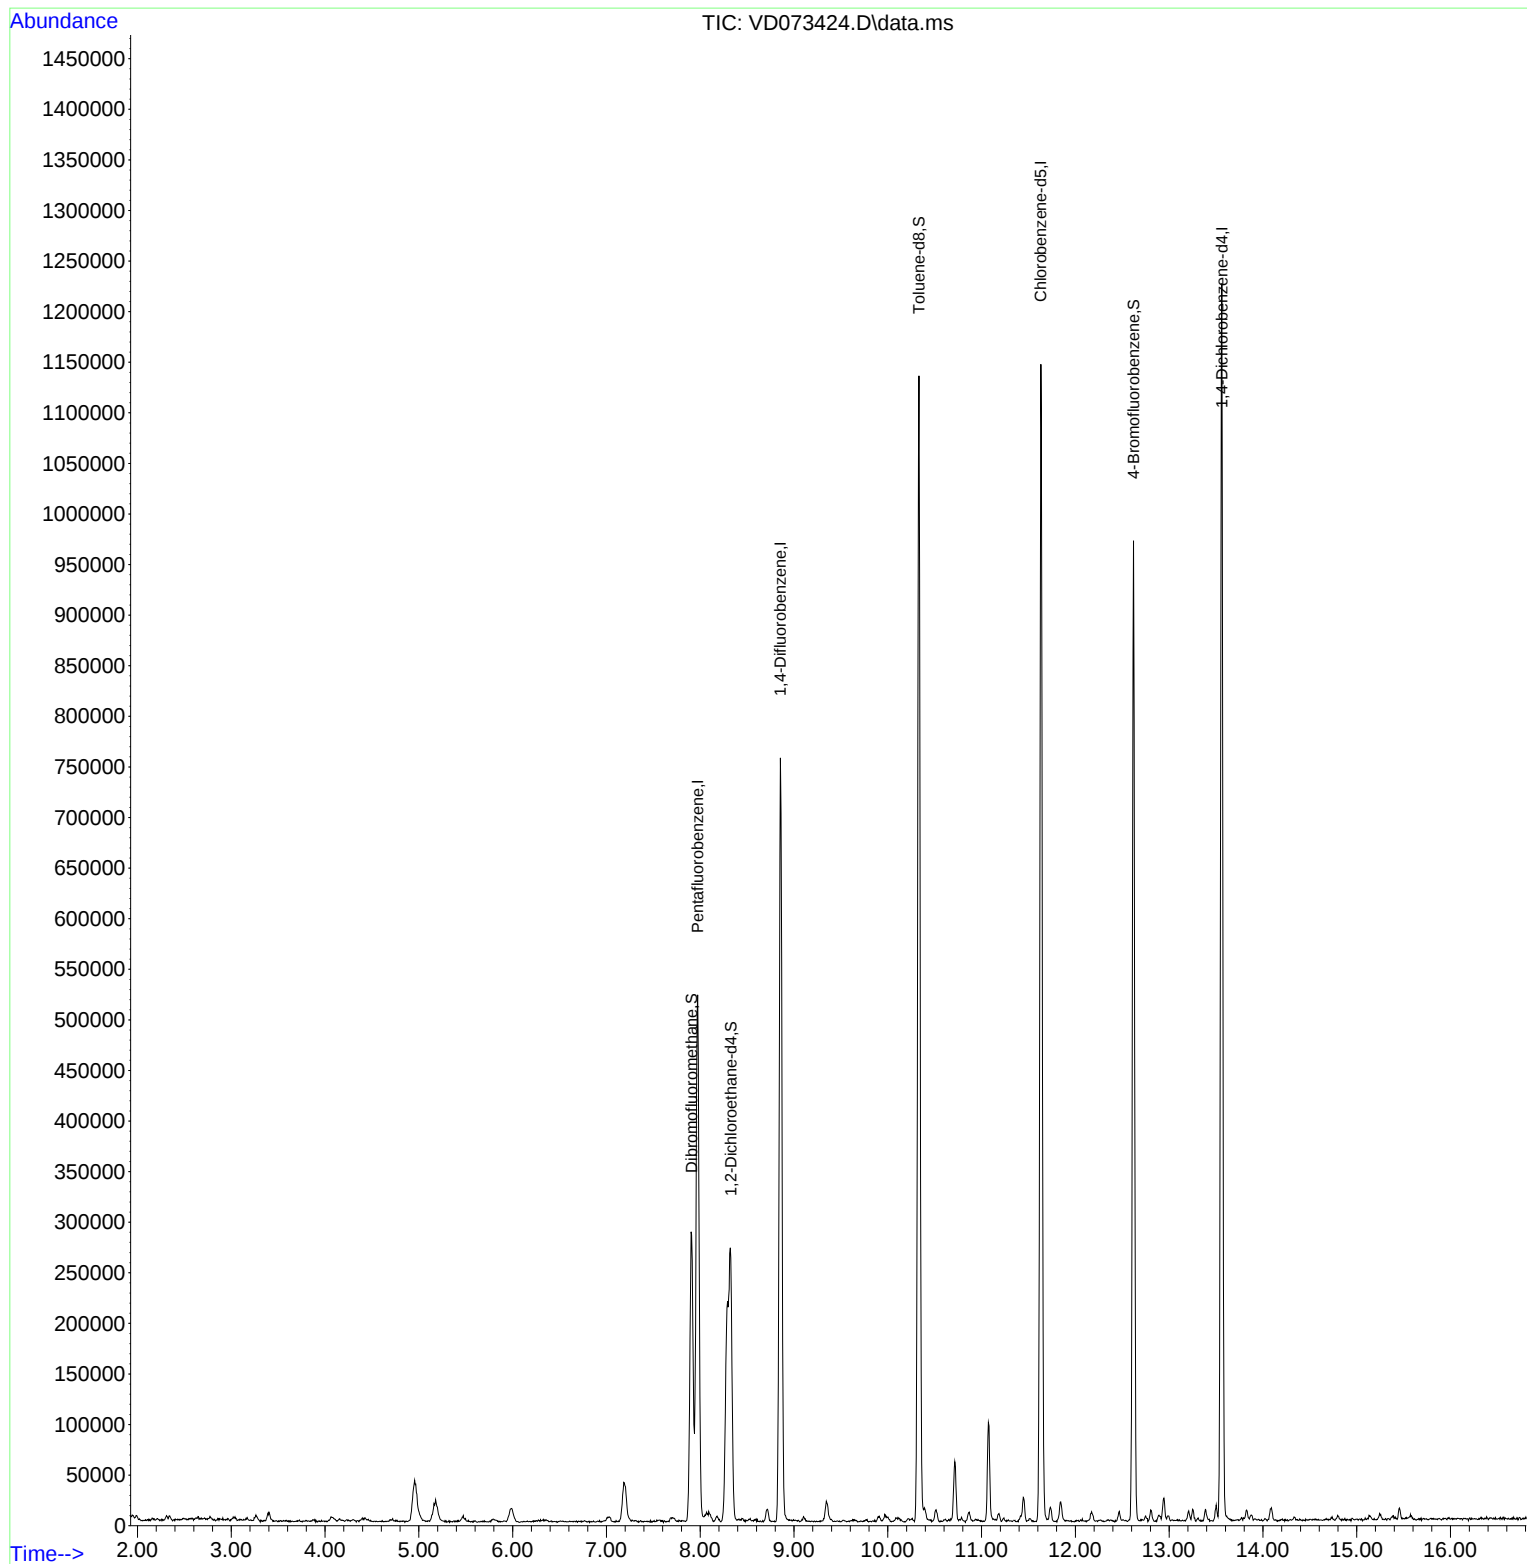


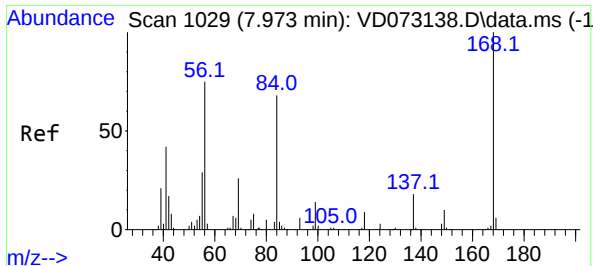

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43




Instrument :
MSVOA_D
ClientSampleId :
VD0531SBL01


Tgt Ion:168 Resp: 380471
Ion Ratio Lower Upper
168 100
99 59.0 49.8 74.6

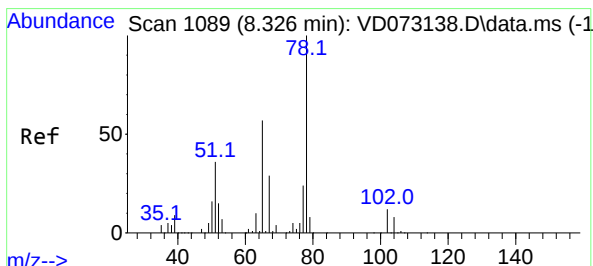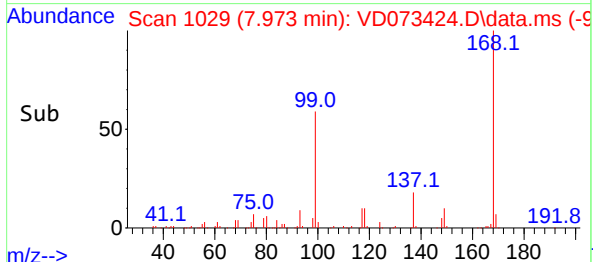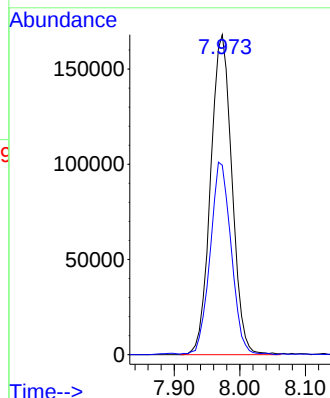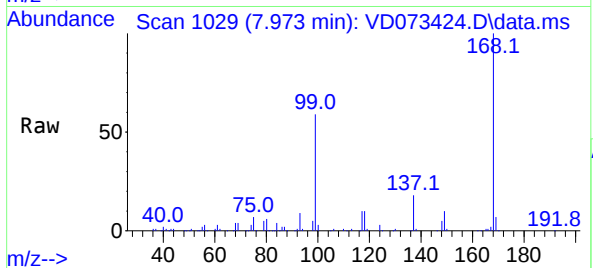

#33
1,2-Dichloroethane-d4
Concen: 46.396 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43

Tgt Ion: 65 Resp: 195083
Ion Ratio Lower Upper
65 100
67 53.4 0.0 101.4

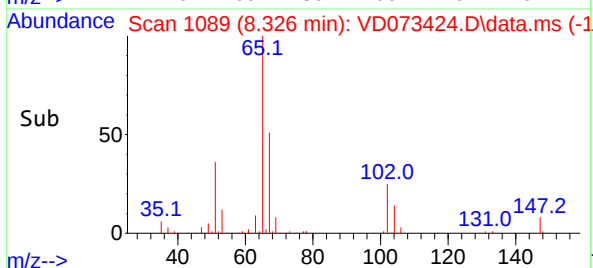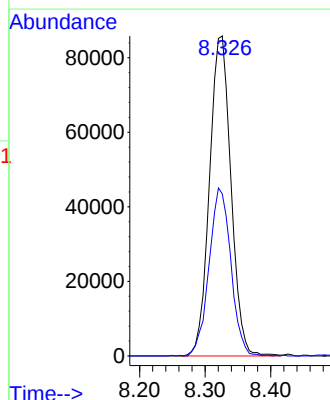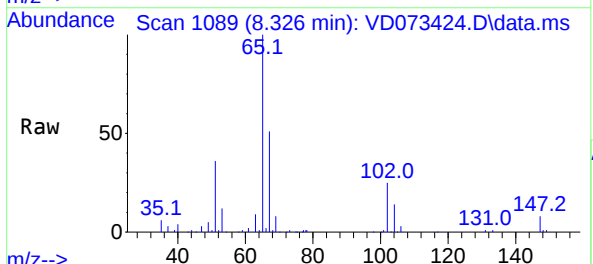

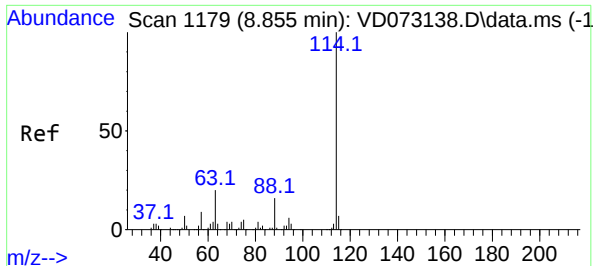

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.856 min Scan# 1179

Delta R.T. 0.001 min

Lab File: VD073424.D

Acq: 31 May 2022 14:43

Instrument :

MSVOA_D

ClientSampleId :

VD0531SBL01





Tgt Ion:114 Resp: 666022

Ion Ratio Lower Upper

114 100

63 19.7 0.0 46.6

88 15.5 0.0 33.2

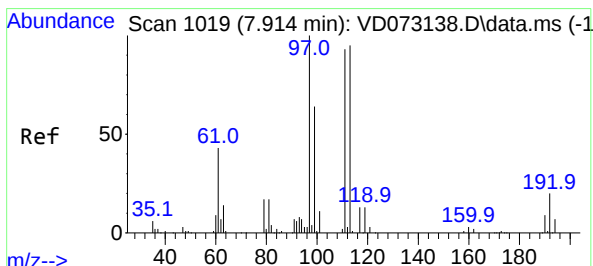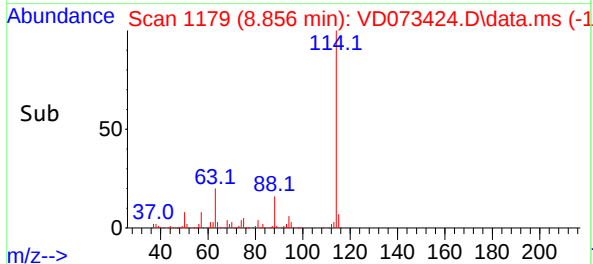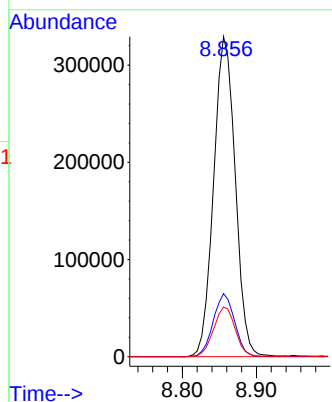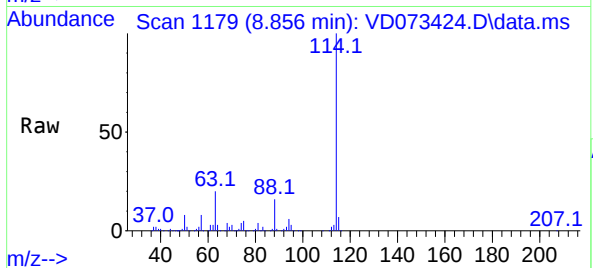

#35

Dibromofluoromethane

Concen: 47.860 ug/l

RT: 7.909 min Scan# 1018

Delta R.T. -0.005 min

Lab File: VD073424.D

Acq: 31 May 2022 14:43




Tgt Ion:113 Resp: 210338

Ion Ratio Lower Upper

113 100

111 103.9 83.8 125.6

192 18.8 14.6 21.8

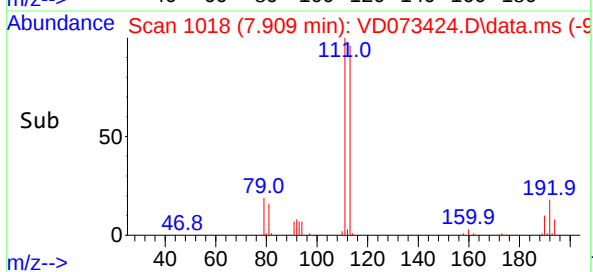
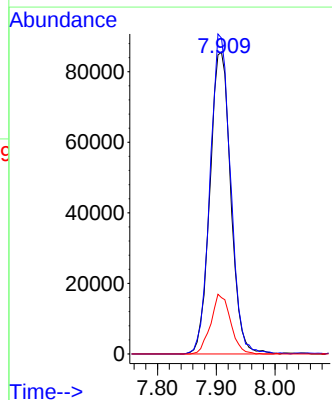
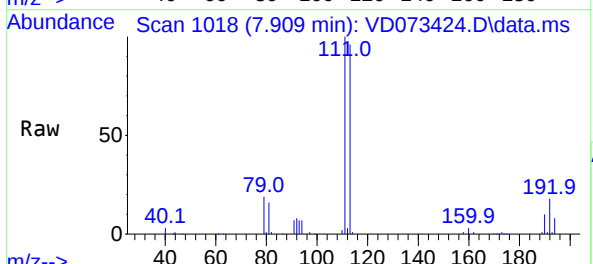




#50
Toluene-d8
Concen: 47.707 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43




Instrument :
MSVOA_D
ClientSampleId :
VD0531SBL01


Tgt Ion: 98 Resp: 772882
Ion Ratio Lower Upper
98 100
100 67.3 52.4 78.6

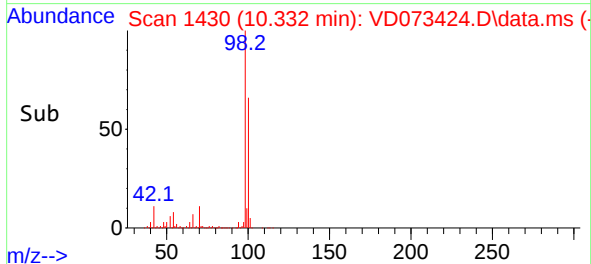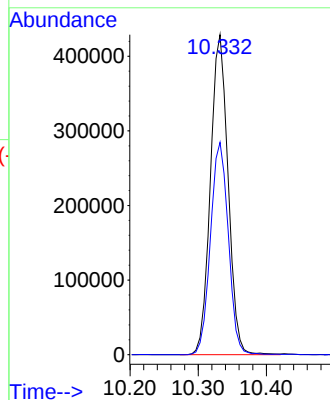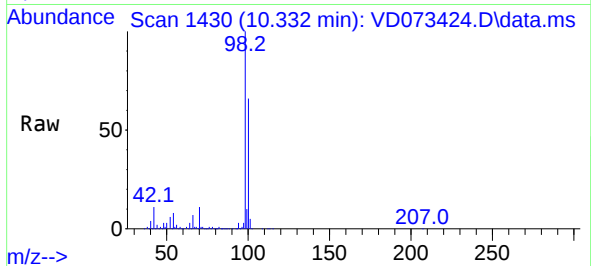

#62
4-Bromofluorobenzene
Concen: 55.683 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43

Tgt Ion: 95 Resp: 316581
Ion Ratio Lower Upper
95 100
174 79.3 0.0 152.8
176 75.0 0.0 145.4


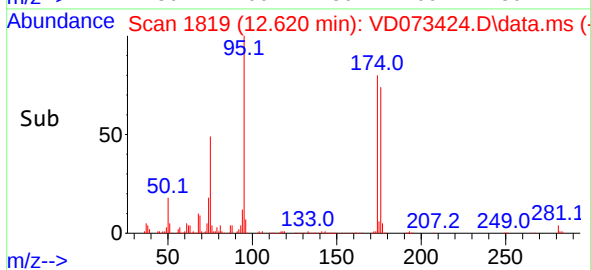
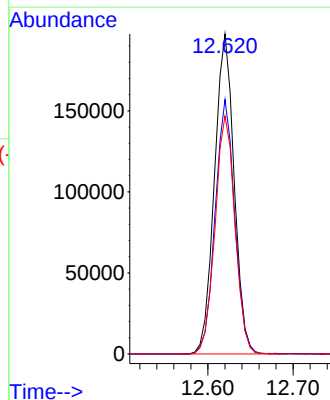
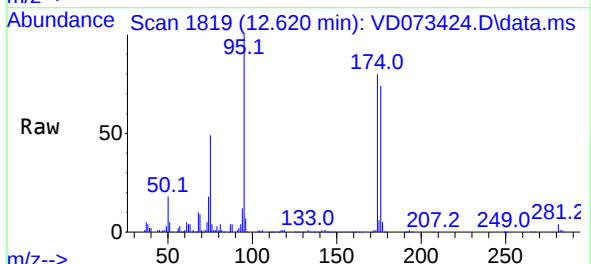


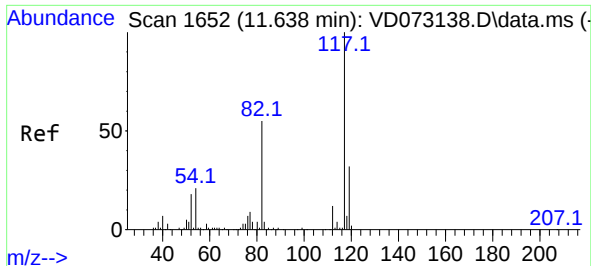

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 1
Delta R.T. -0.006 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43

Instrument :
MSVOA_D
ClientSampleId :
VD0531SBL01

Tgt Ion:117 Resp: 681751
Ion Ratio Lower Upper
117 100
82 54.3 45.3 67.9
119 31.0 26.6 40.0

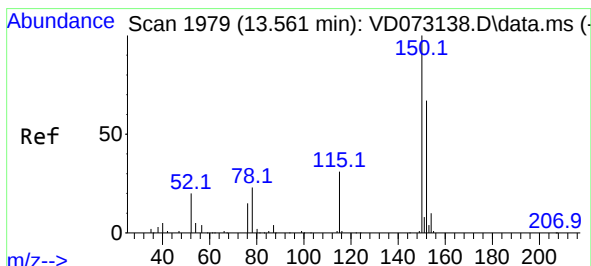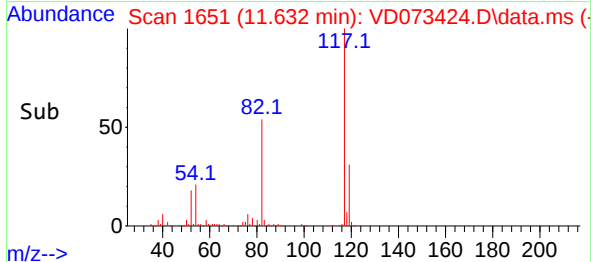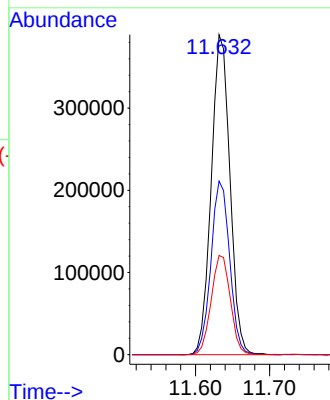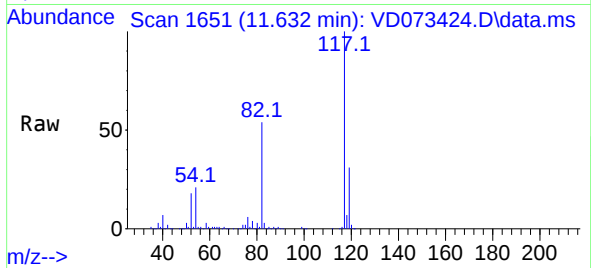

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073424.D
Acq: 31 May 2022 14:43

Tgt Ion:152 Resp: 328276
Ion Ratio Lower Upper
152 100
115 61.5 31.3 93.8
150 159.1 0.0 348.6

