


Methyl Iodide

Response Ratio

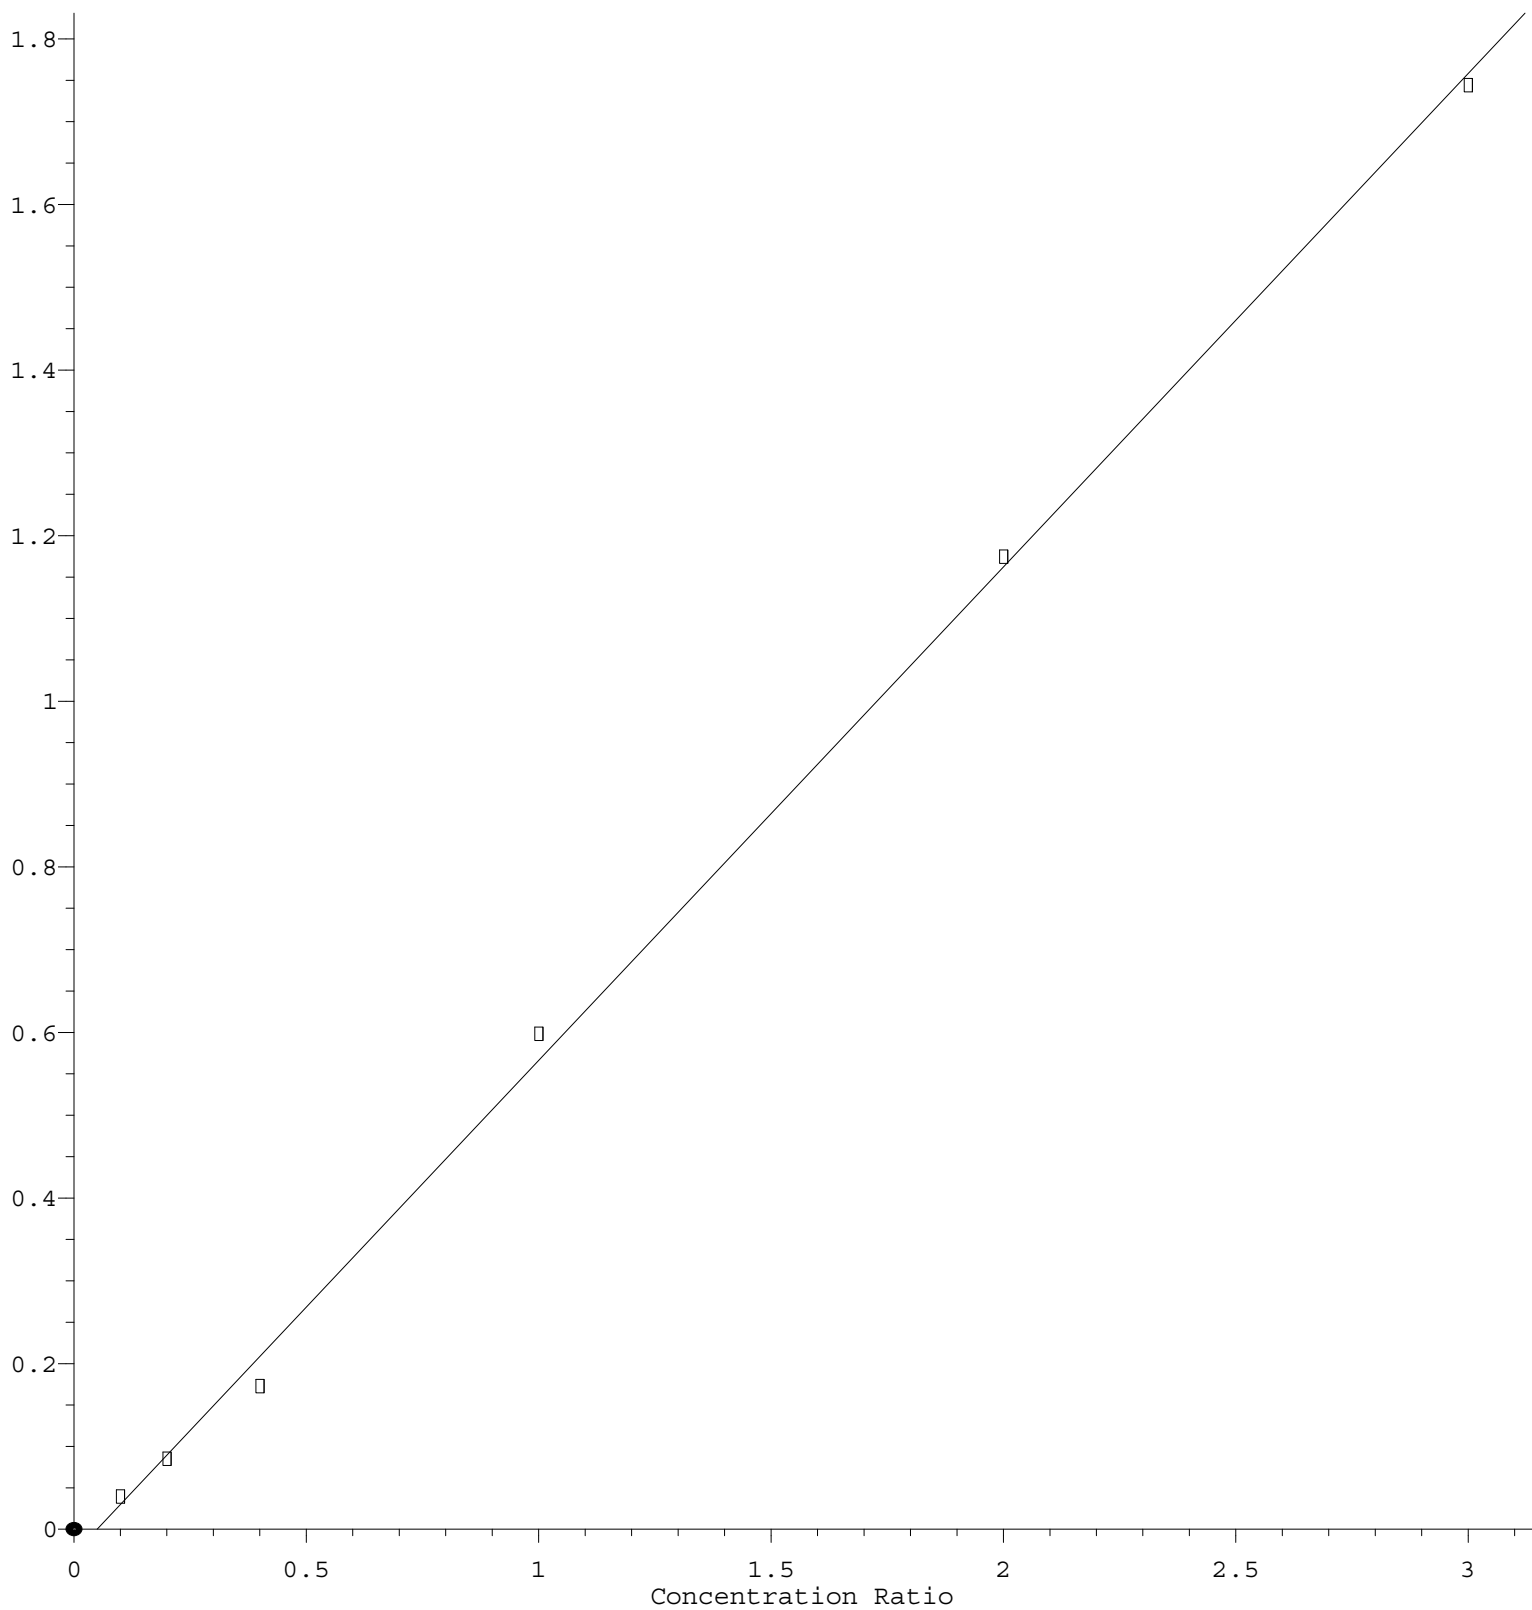

$$\text{Response} = 5.960\text{e-}001 * \text{Amt} - 2.993\text{e-}002$$


Coef of Det (r^2) = 0.998840 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M

Calibration Table Last Updated: Wed Jun 02 02:17:36 2021

Ethyl methacrylate

Response Ratio

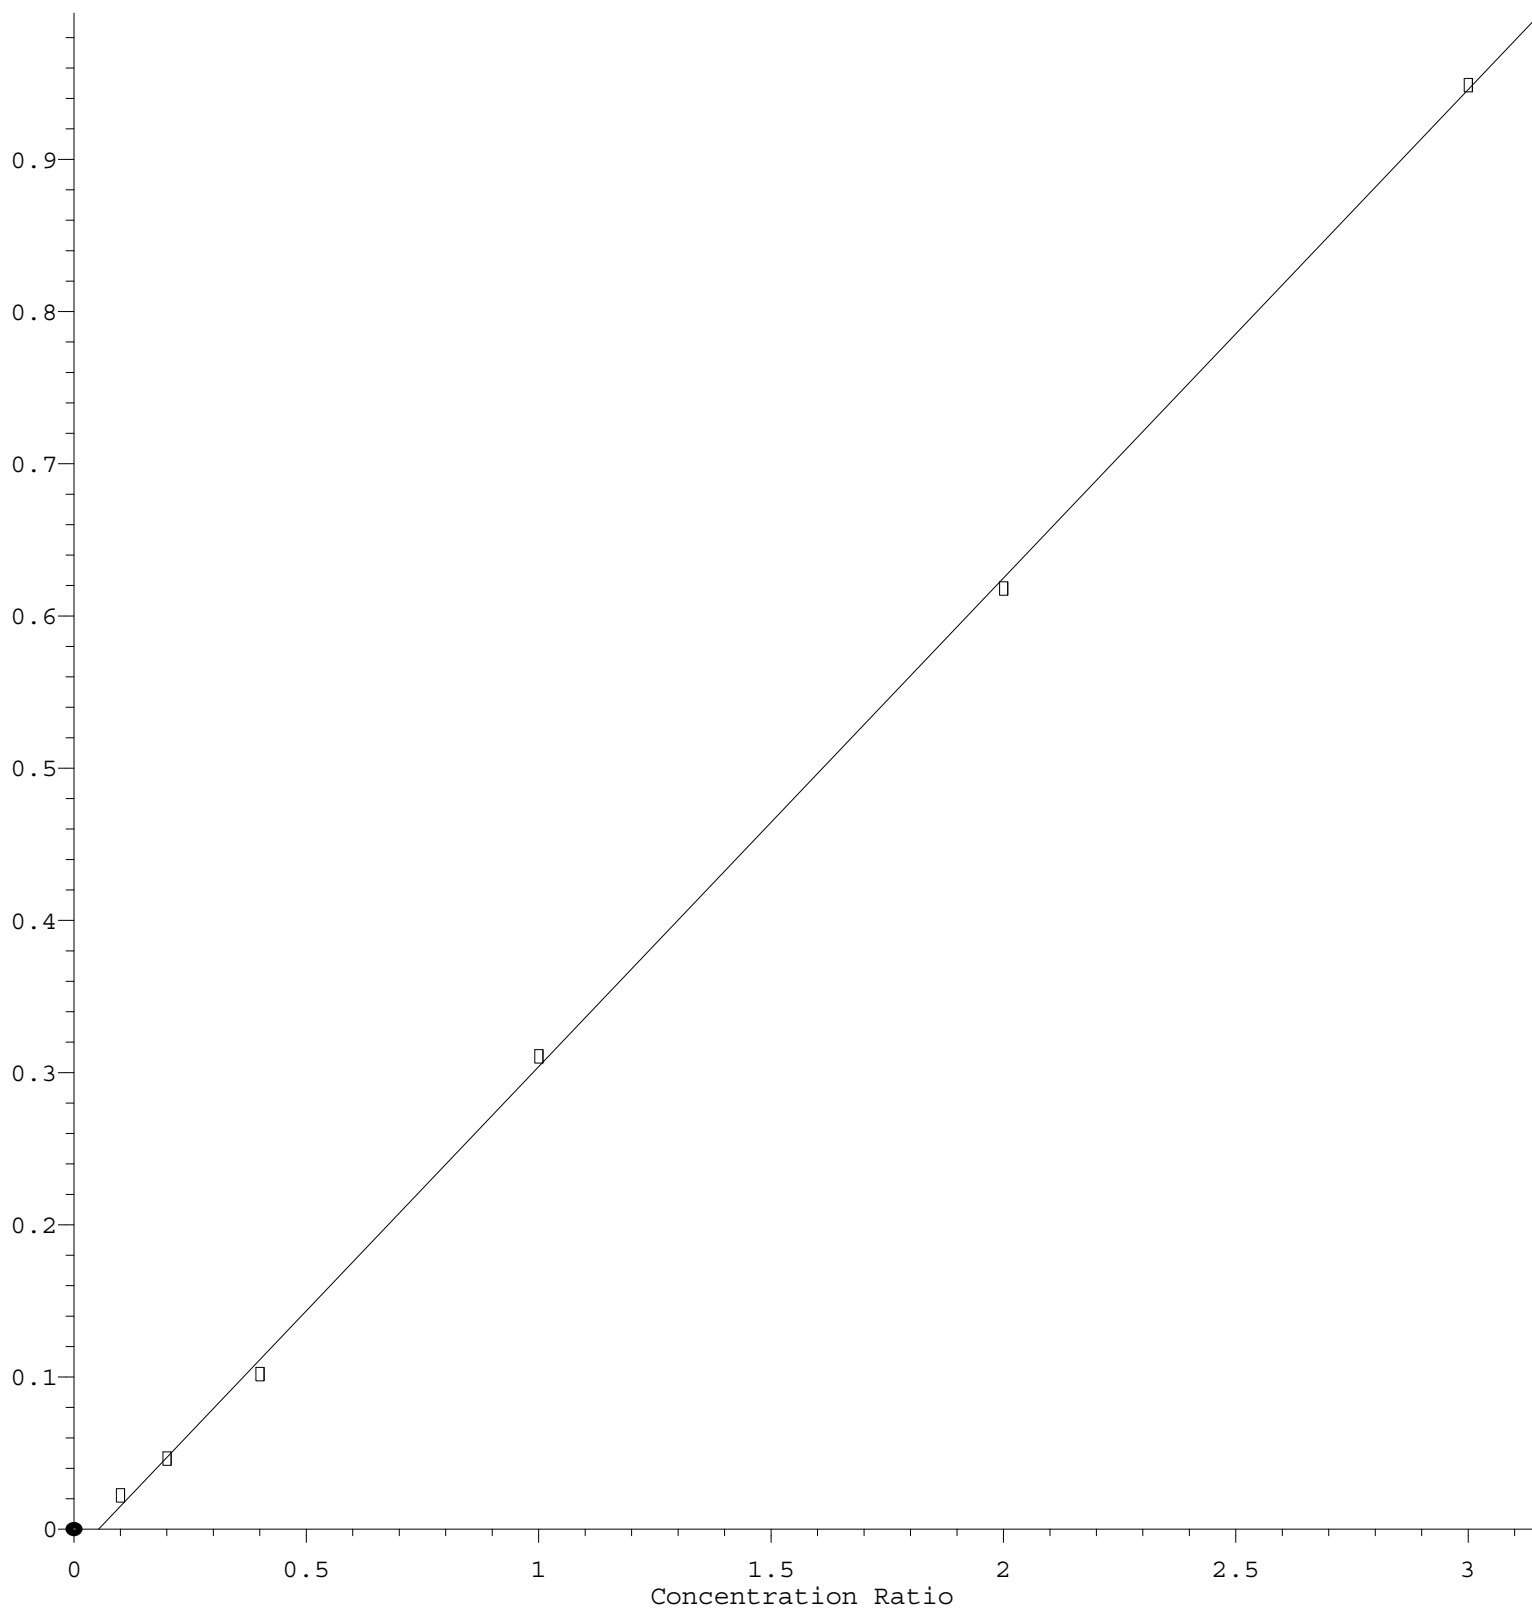

$$\text{Response} = 3.208\text{e-}001 * \text{Amt} - 1.692\text{e-}002$$


Coef of Det (r^2) = 0.999650 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M

Calibration Table Last Updated: Wed Jun 02 02:17:36 2021

Naphthalene

Response Ratio

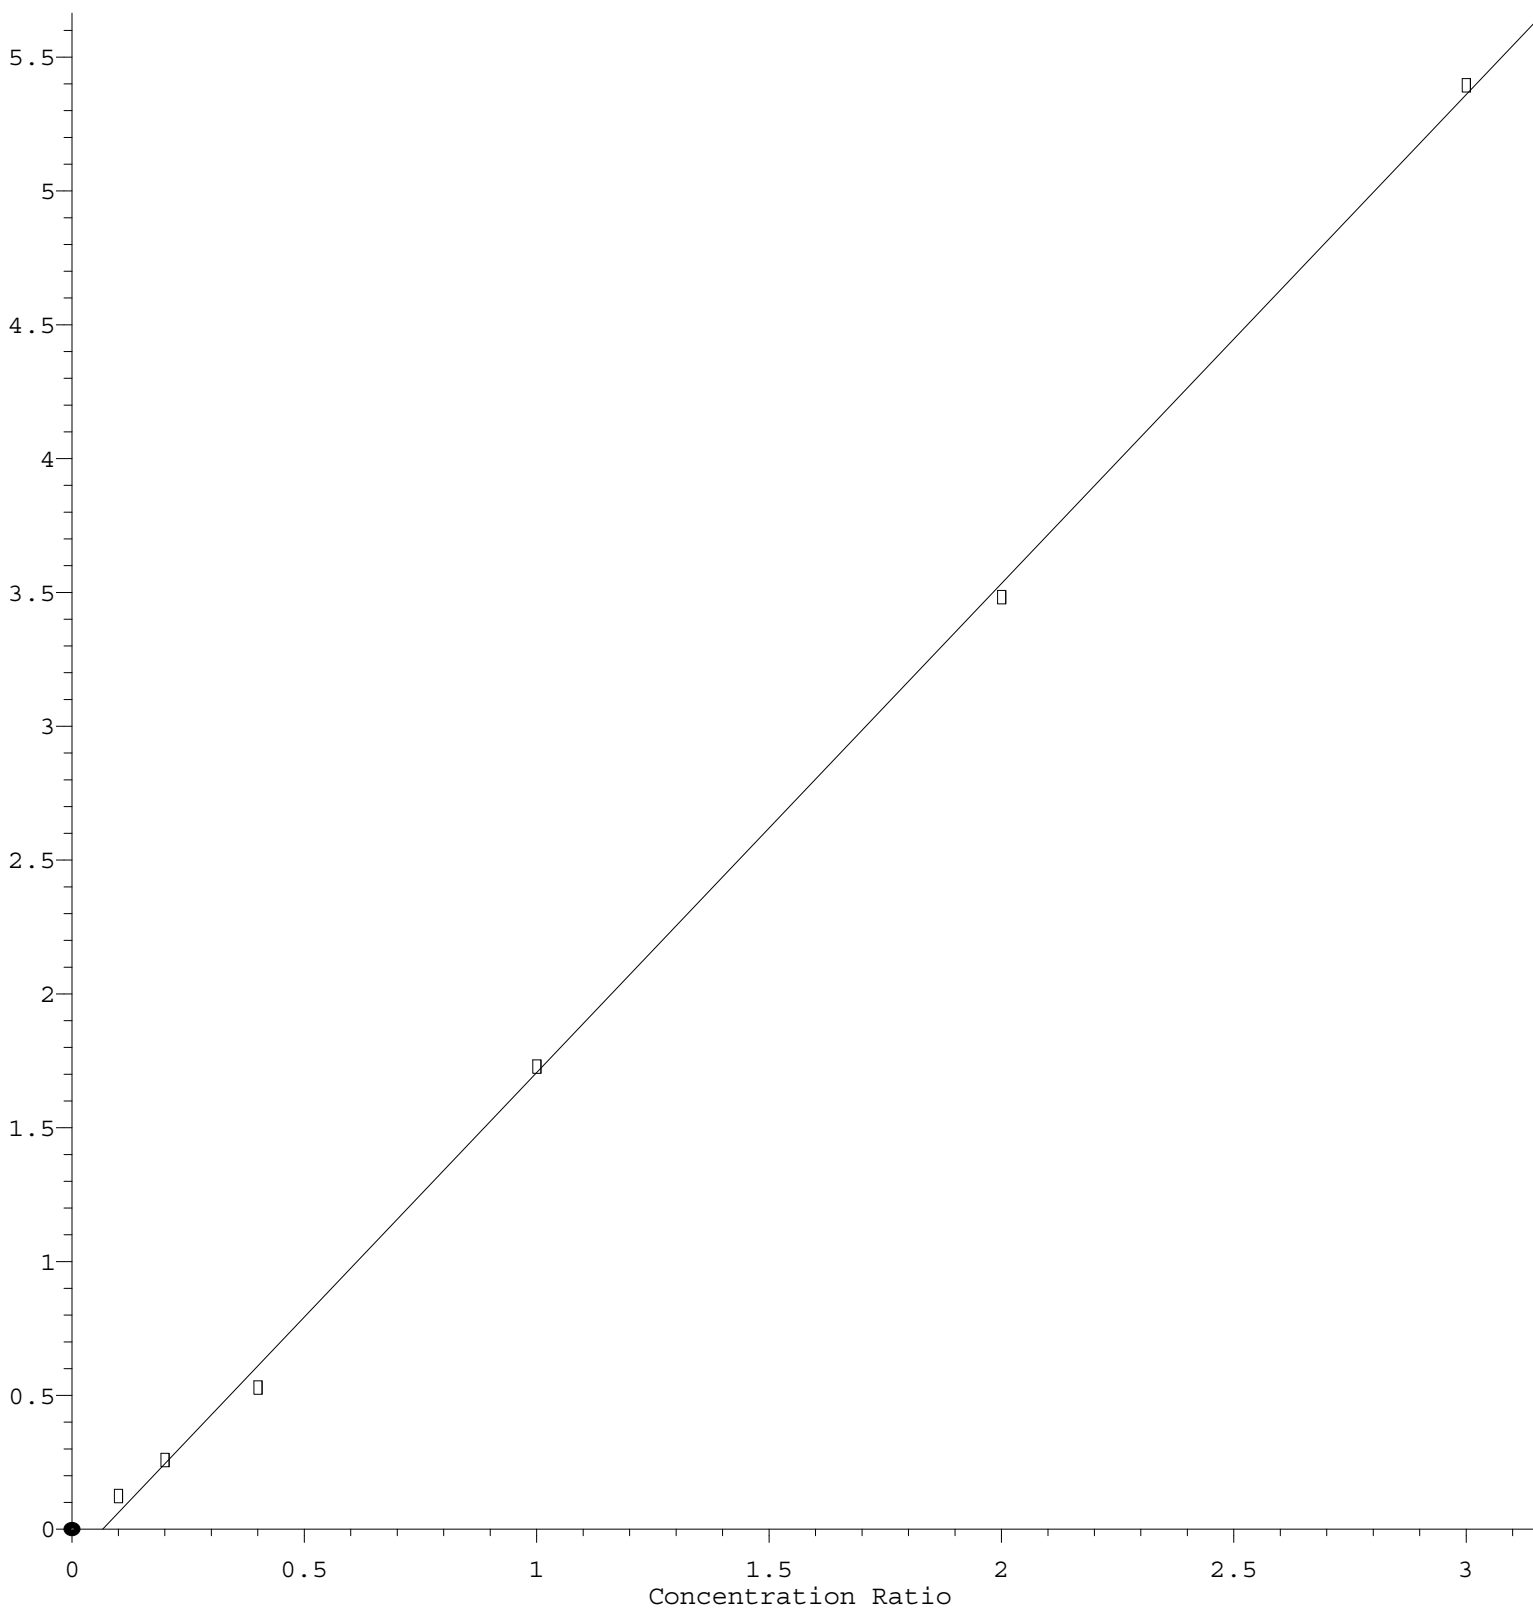


$$\text{Response} = 1.827\text{e}+000 * \text{Amt} - 1.206\text{e}-001$$

Coef of Det (r^2) = 0.999338 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M


Calibration Table Last Updated: Wed Jun 02 02:17:36 2021

Tert butyl alcohol

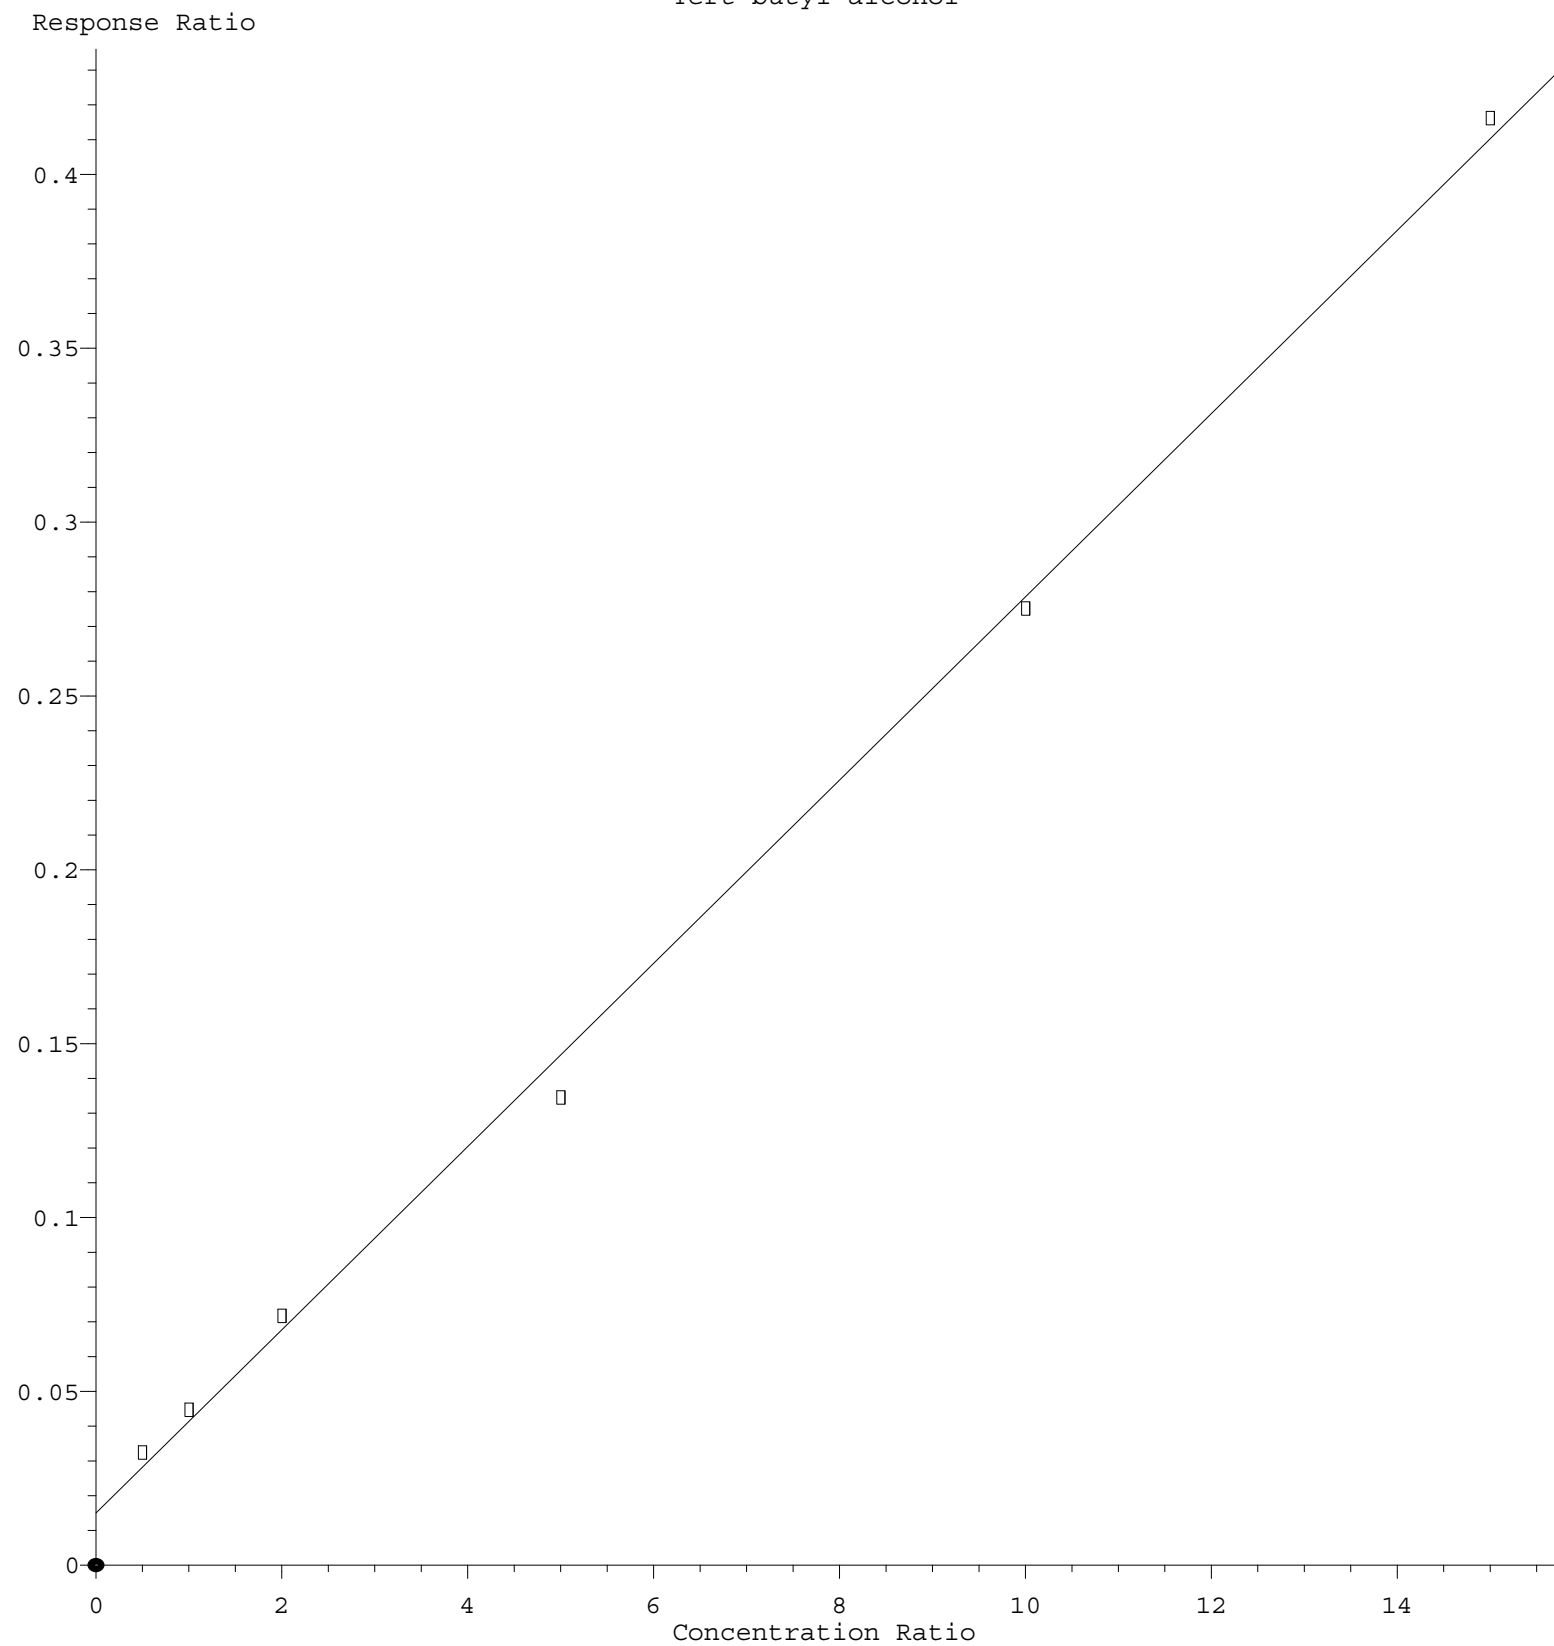

Response = $2.633\text{e-}002 * \text{Amt} + 1.540\text{e-}002$
Coef of Det (r^2) = 0.997946 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M
Calibration Table Last Updated: Wed Jun 02 02:17:36 2021


Acrolein

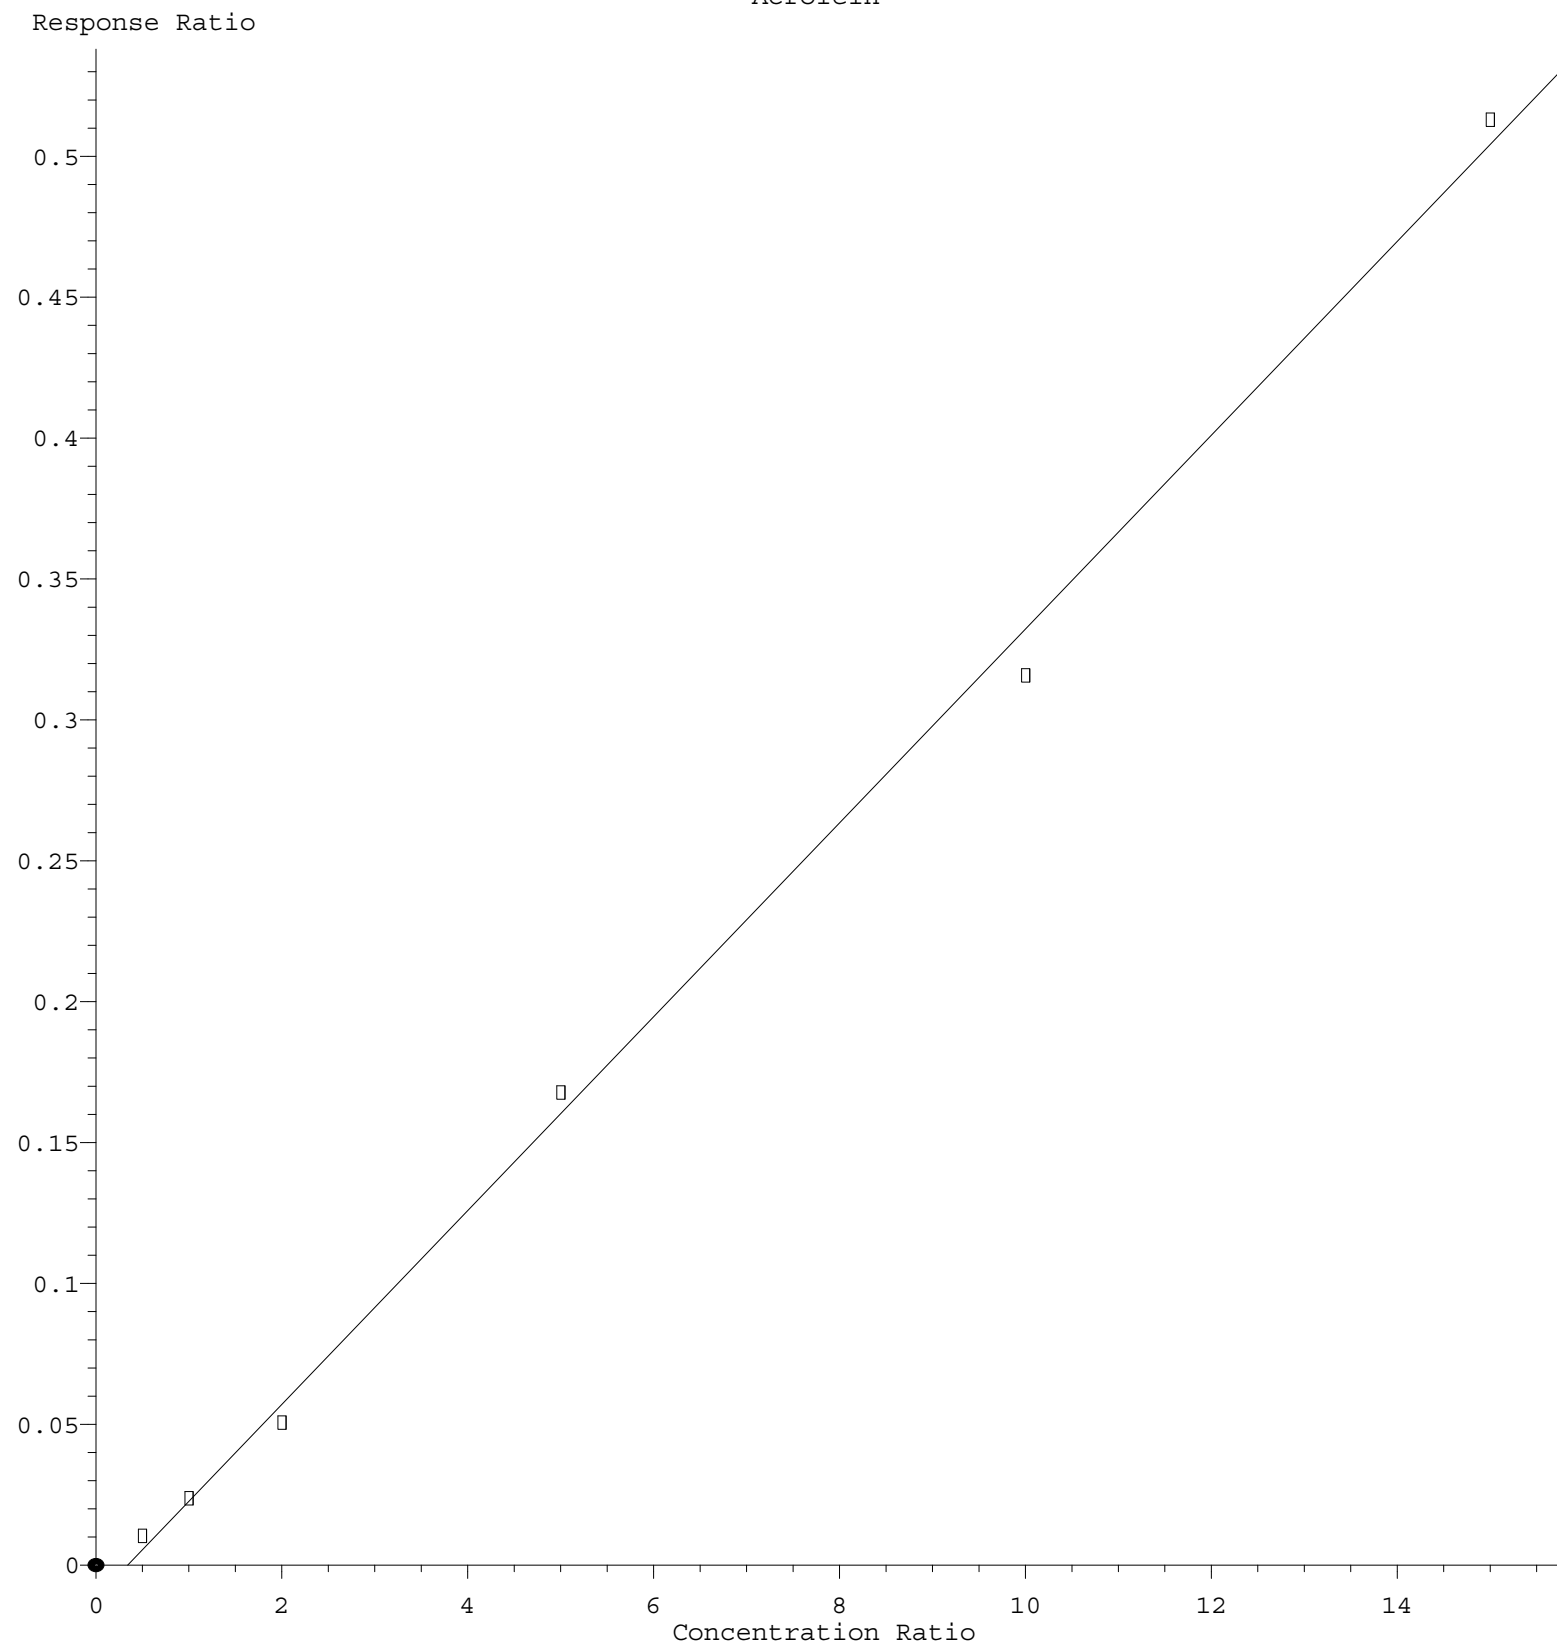

Response = $3.439 \times 10^{-2} \times \text{Amt} - 1.179 \times 10^{-2}$
 Coef of Det (r^2) = 0.997644 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M
 Calibration Table Last Updated: Wed Jun 02 02:17:36 2021

Methylene Chloride

Response Ratio

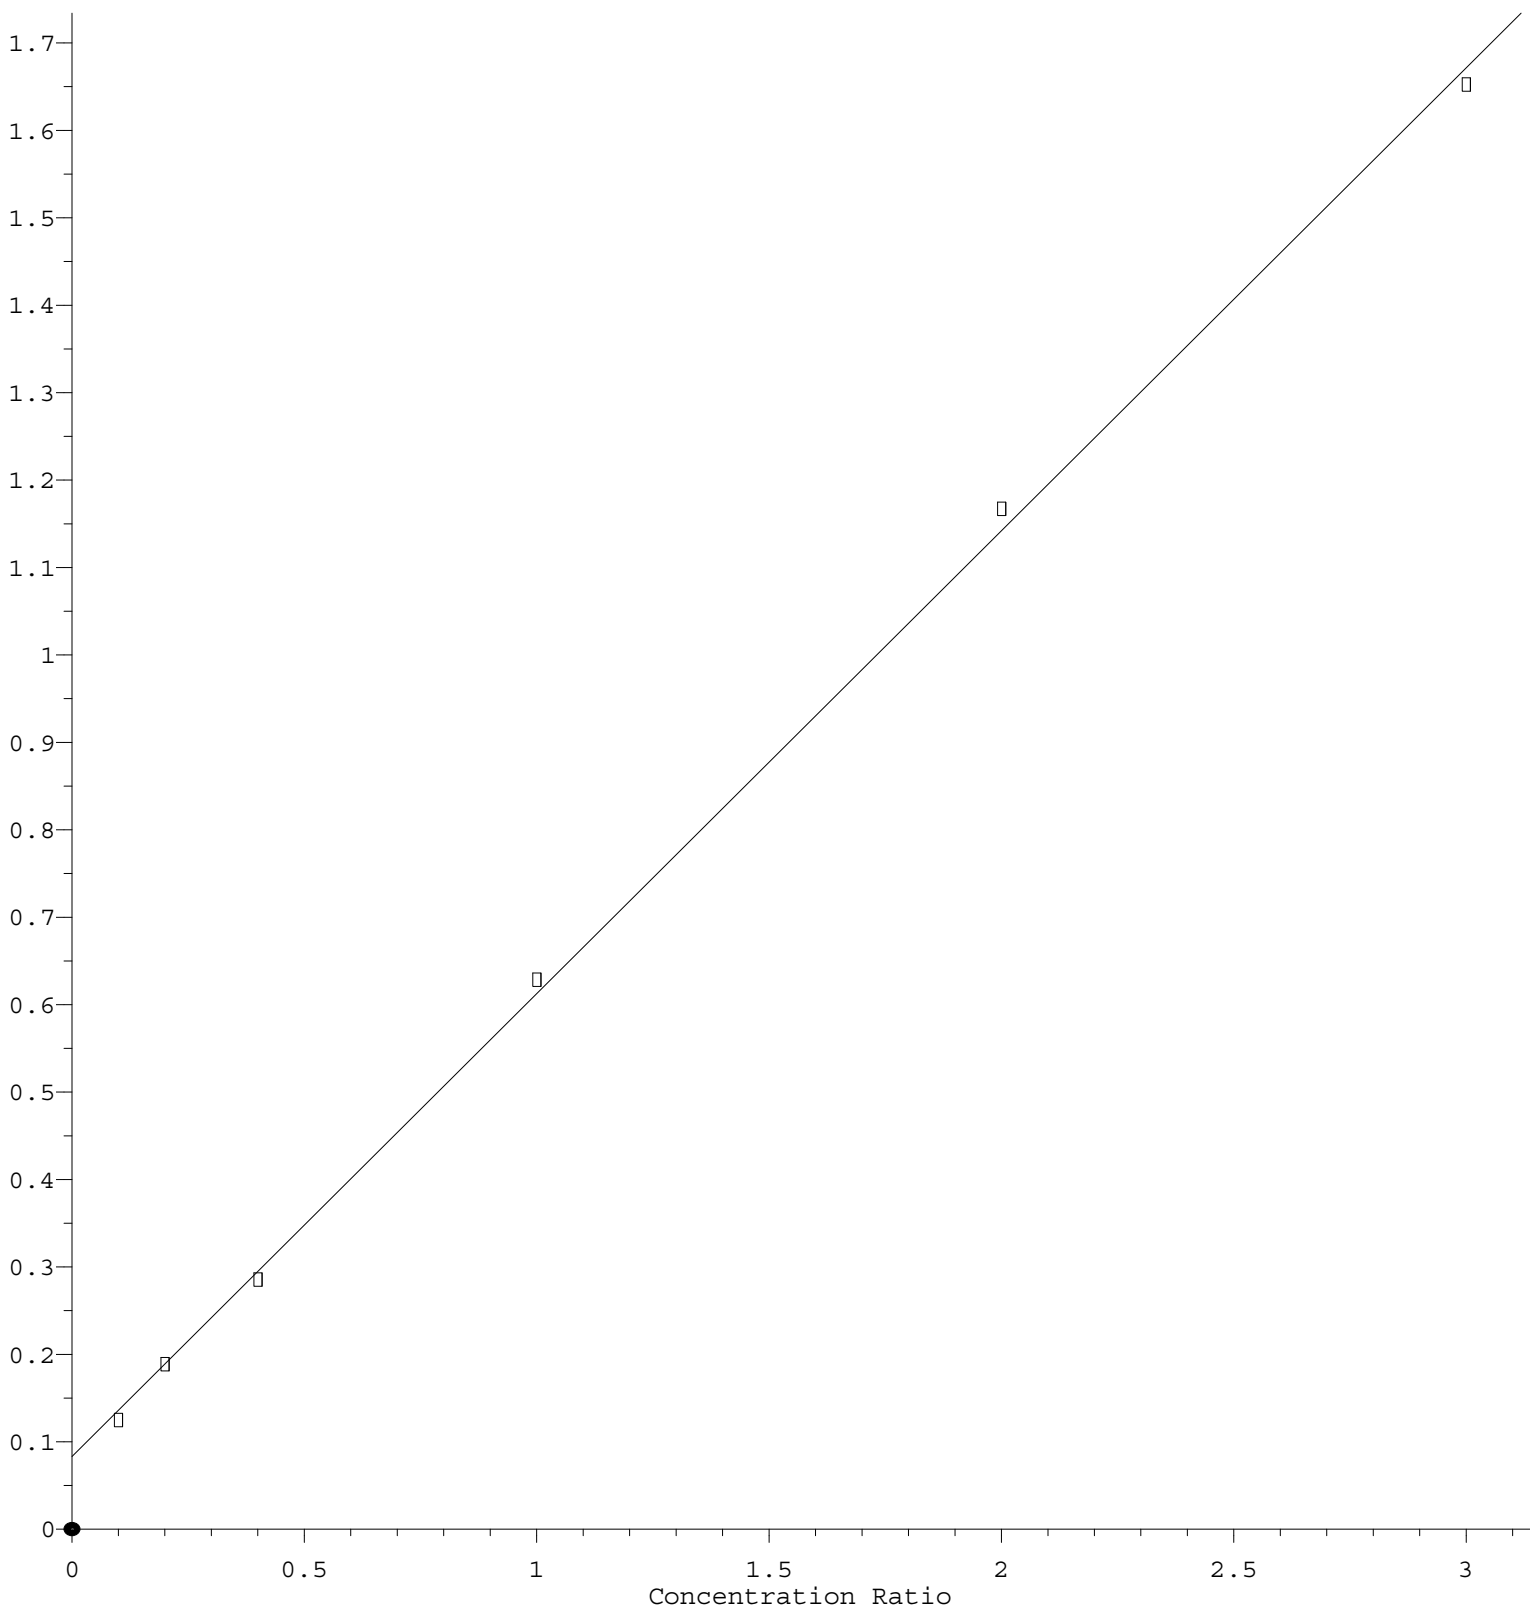

$$\text{Response} = 5.298\text{e-}001 * \text{Amt} + 8.282\text{e-}002$$

Coef of Det (r^2) = 0.999227 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M

Calibration Table Last Updated: Wed Jun 02 02:17:36 2021

Vinyl Acetate

Response Ratio

12
11
10
9
8
7
6
5
4
3
2
1
0

0

2

4

6

8

10

12

14

Concentration Ratio

Response = 7.787e-001 * Amt - 1.808e-001
 Coef of Det (r^2) = 0.999549 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D060121S.M
 Calibration Table Last Updated: Wed Jun 02 02:17:36 2021