

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060122\
 Data File : VD073451.D
 Acq On : 01 Jun 2022 16:46
 Operator : VA/SY
 Sample : VIBLK
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK

Quant Time: Jun 02 08:51:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
 Quant Title : SW846 8260
 QLast Update : Thu May 19 15:13:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	277615	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	512879	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	577499	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	284241	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	149686	48.789	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.580%
35) Dibromofluoromethane	7.908	113	172326	50.919	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.840%
50) Toluene-d8	10.332	98	658037	52.747	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.500%
62) 4-Bromofluorobenzene	12.620	95	264232	60.353	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	120.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060122\
Data File : VD073451.D
Acq On : 01 Jun 2022 16:46
Operator : VA/SY
Sample : VIBLK
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Quant Time: Jun 02 08:51:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
Quant Title : SW846 8260
QLast Update : Thu May 19 15:13:42 2022
Response via : Initial Calibration




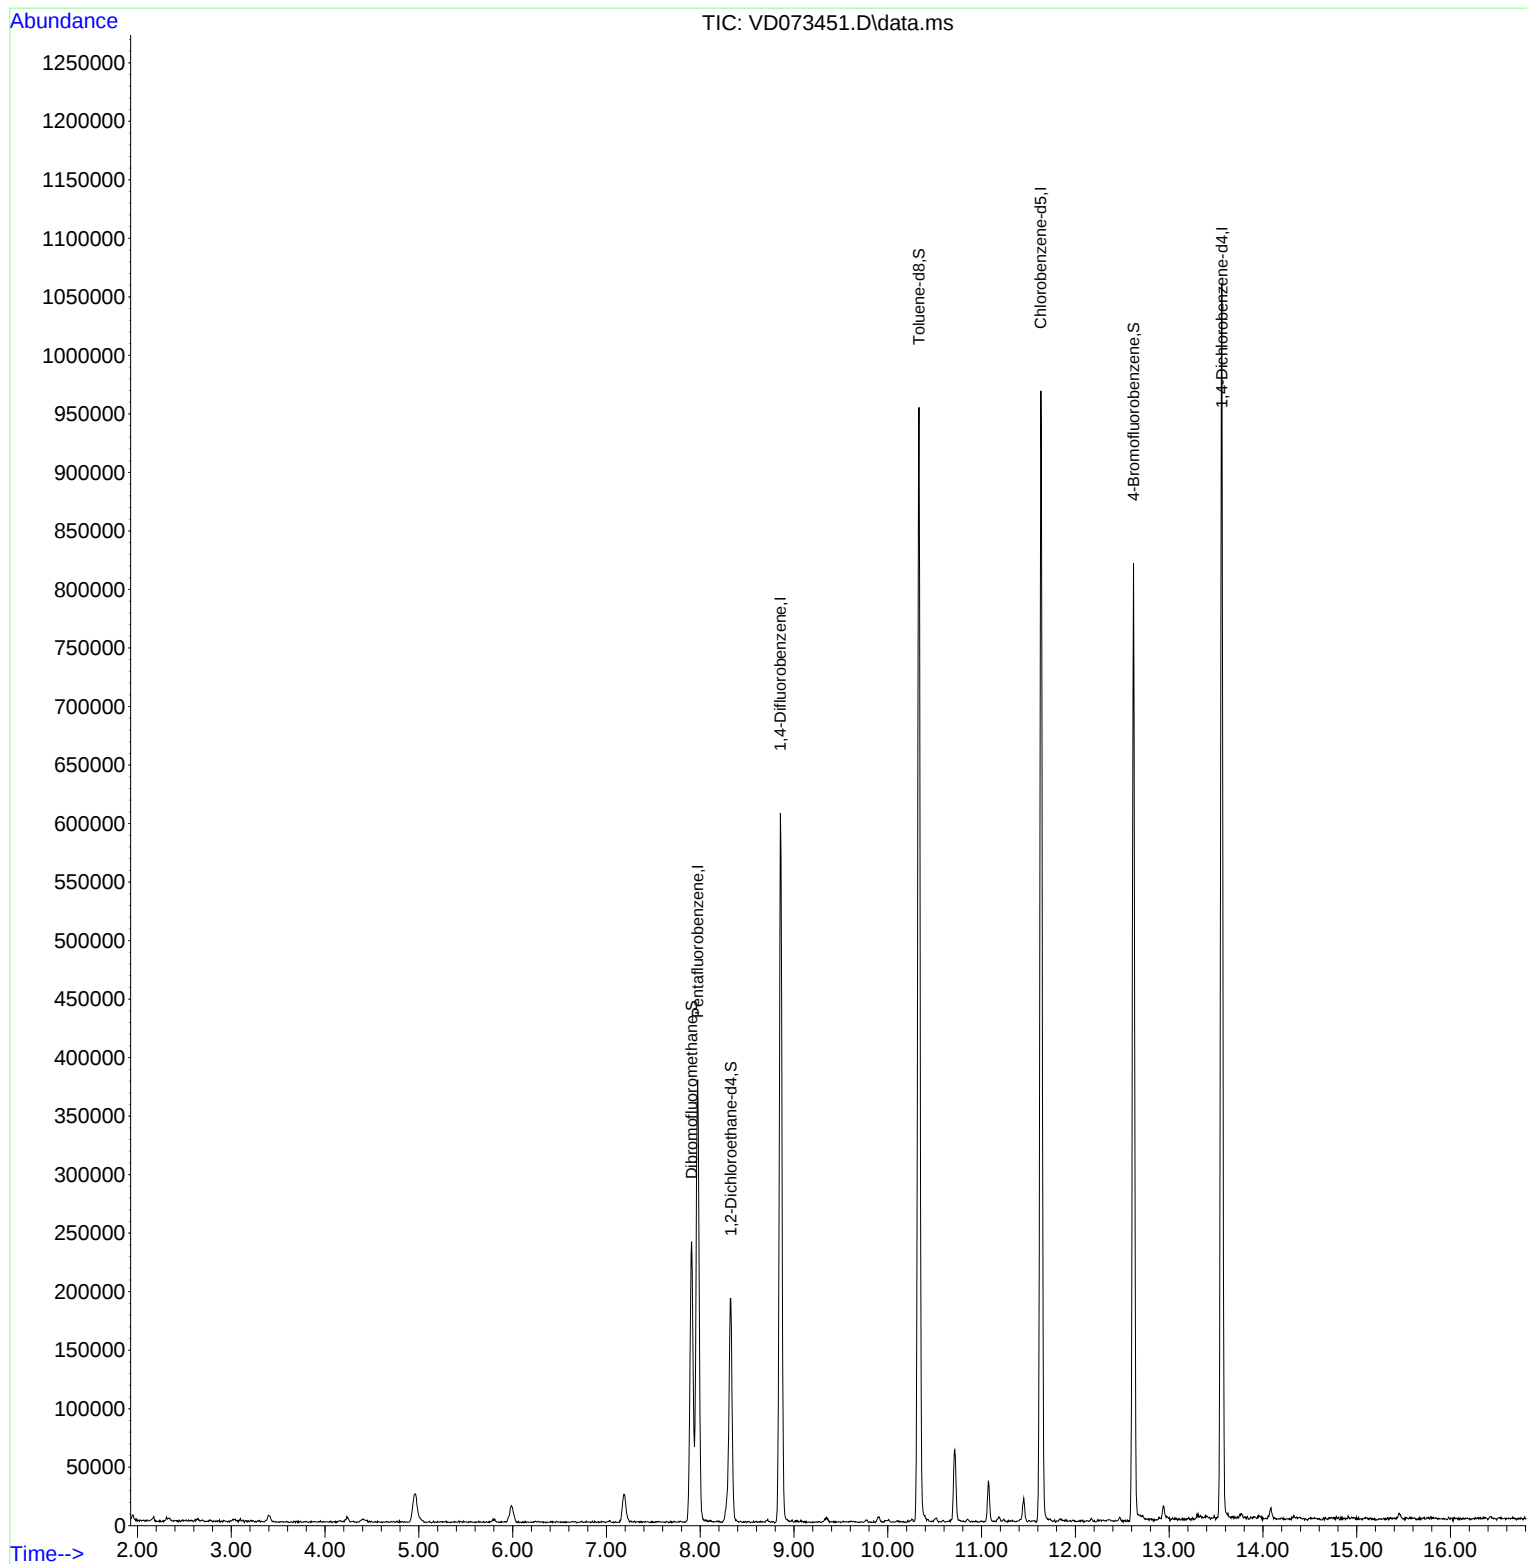


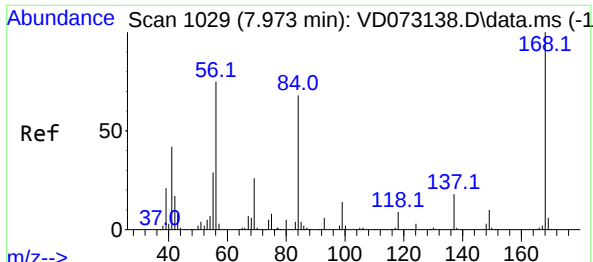

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 277615
Ion Ratio Lower Upper
168 100
99 59.2 49.8 74.6

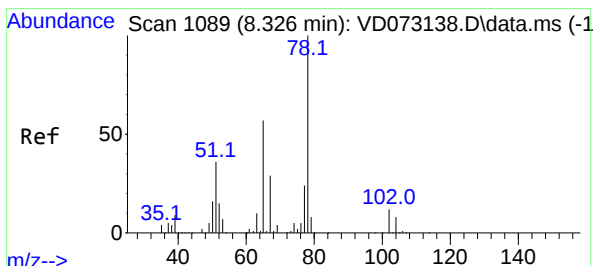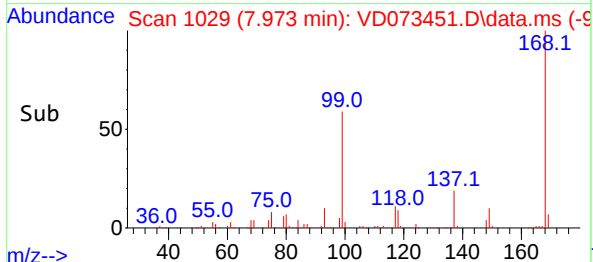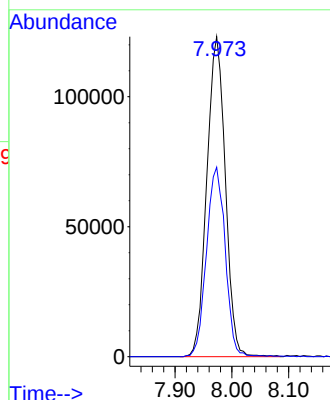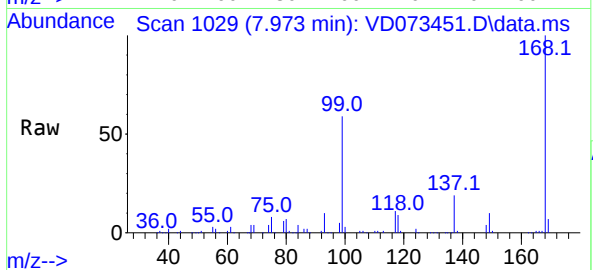

#33
1,2-Dichloroethane-d4
Concen: 48.789 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46

Tgt Ion: 65 Resp: 149686
Ion Ratio Lower Upper
65 100
67 53.9 0.0 101.4


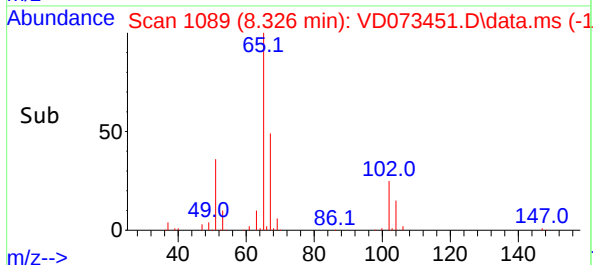
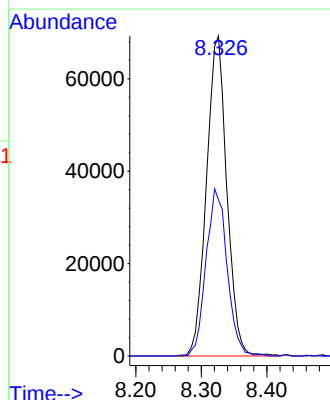
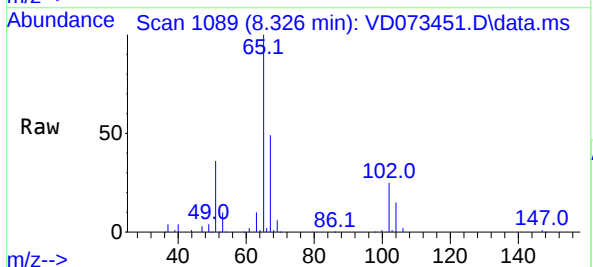


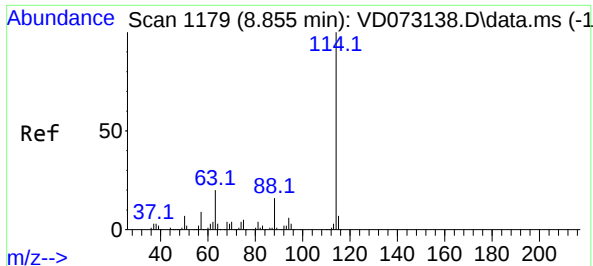

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.855 min Scan# 1179
Delta R.T. 0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 512879
Ion Ratio Lower Upper
114 100
63 19.4 0.0 46.6
88 15.9 0.0 33.2

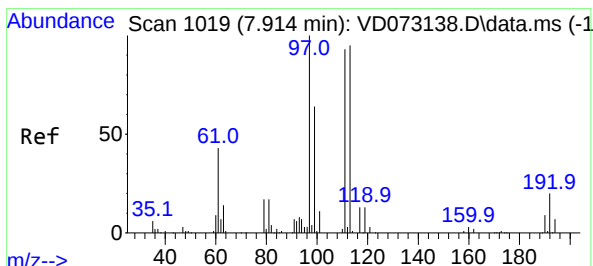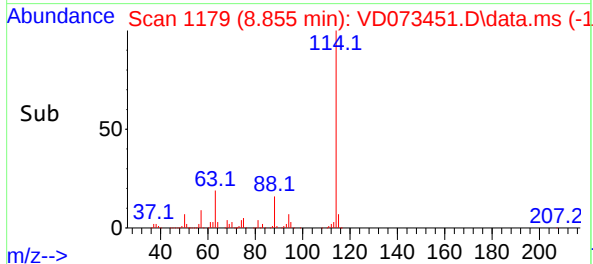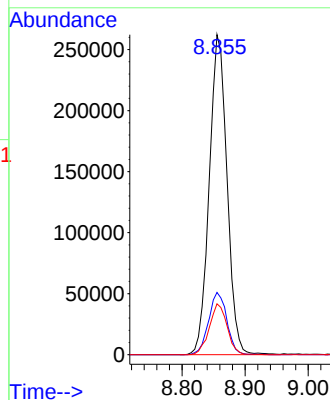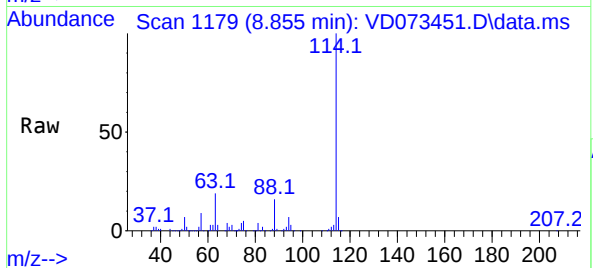

#35
Dibromofluoromethane
Concen: 50.919 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.006 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46

Tgt Ion:113 Resp: 172326
Ion Ratio Lower Upper
113 100
111 103.5 83.8 125.6
192 18.8 14.6 21.8


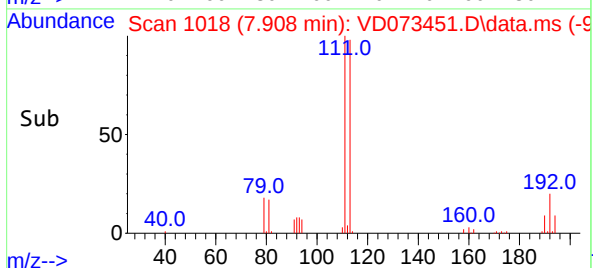
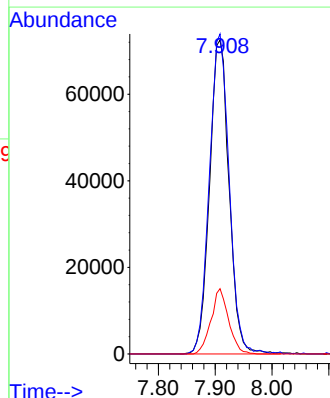
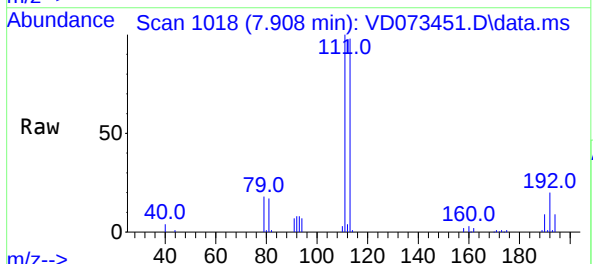


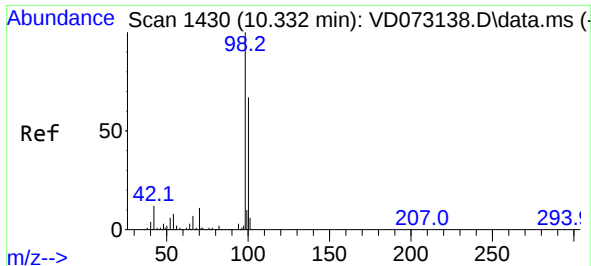

#50
Toluene-d8
Concen: 52.747 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46




Instrument :
MSVOA_D
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 658037
Ion Ratio Lower Upper
98 100
100 65.6 52.4 78.6

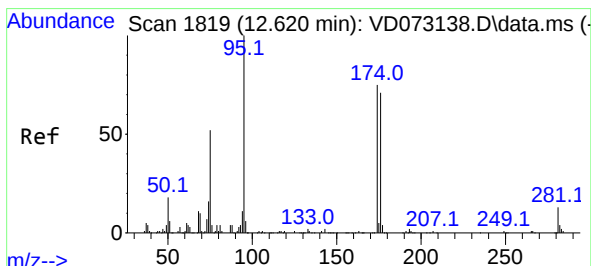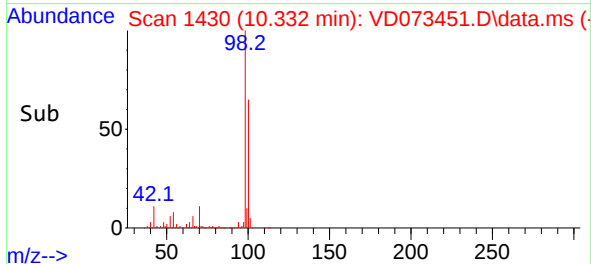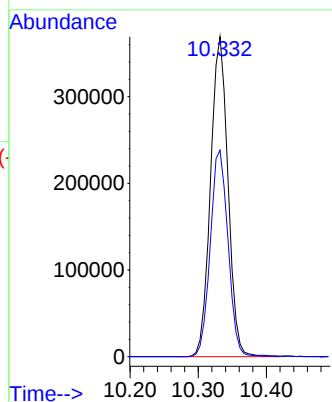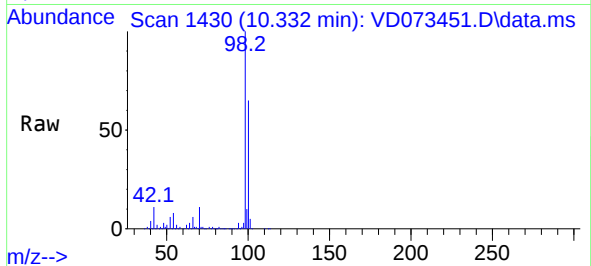

#62
4-Bromofluorobenzene
Concen: 60.353 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46

Tgt Ion: 95 Resp: 264232
Ion Ratio Lower Upper
95 100
174 78.3 0.0 152.8
176 75.2 0.0 145.4


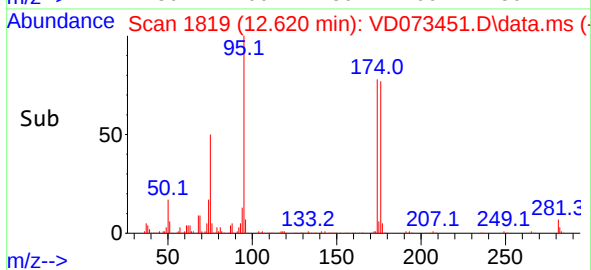
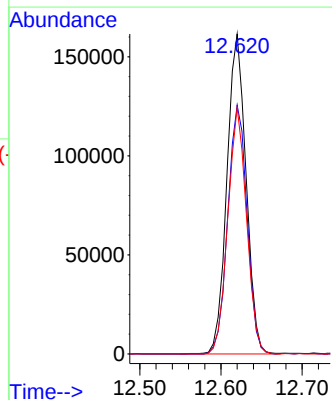
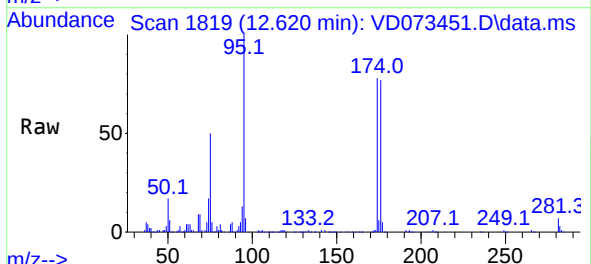


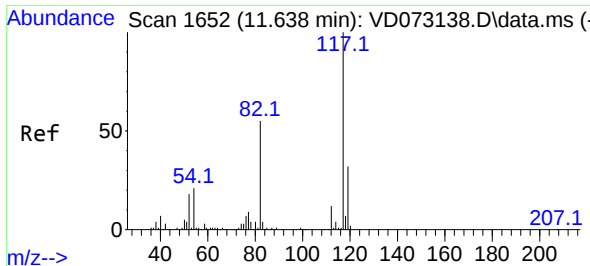

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 117
Delta R.T. -0.006 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46

Instrument :
MSVOA_D
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 577499
Ion Ratio Lower Upper
117 100
82 54.7 45.3 67.9
119 31.1 26.6 40.0

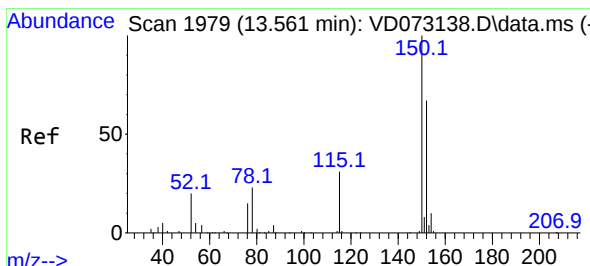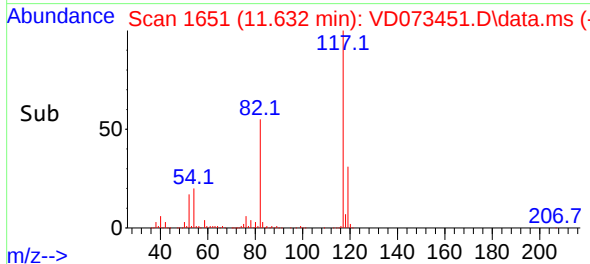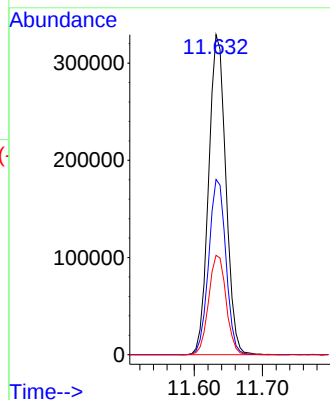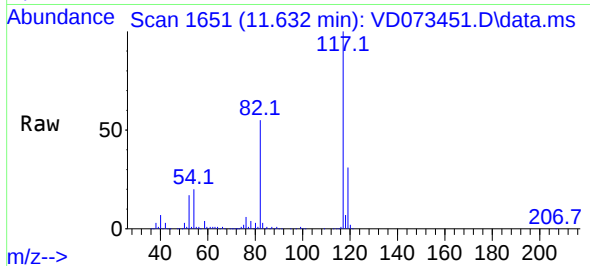

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073451.D
Acq: 01 Jun 2022 16:46

Tgt Ion:152 Resp: 284241
Ion Ratio Lower Upper
152 100
115 59.4 31.3 93.8
150 155.7 0.0 348.6

