
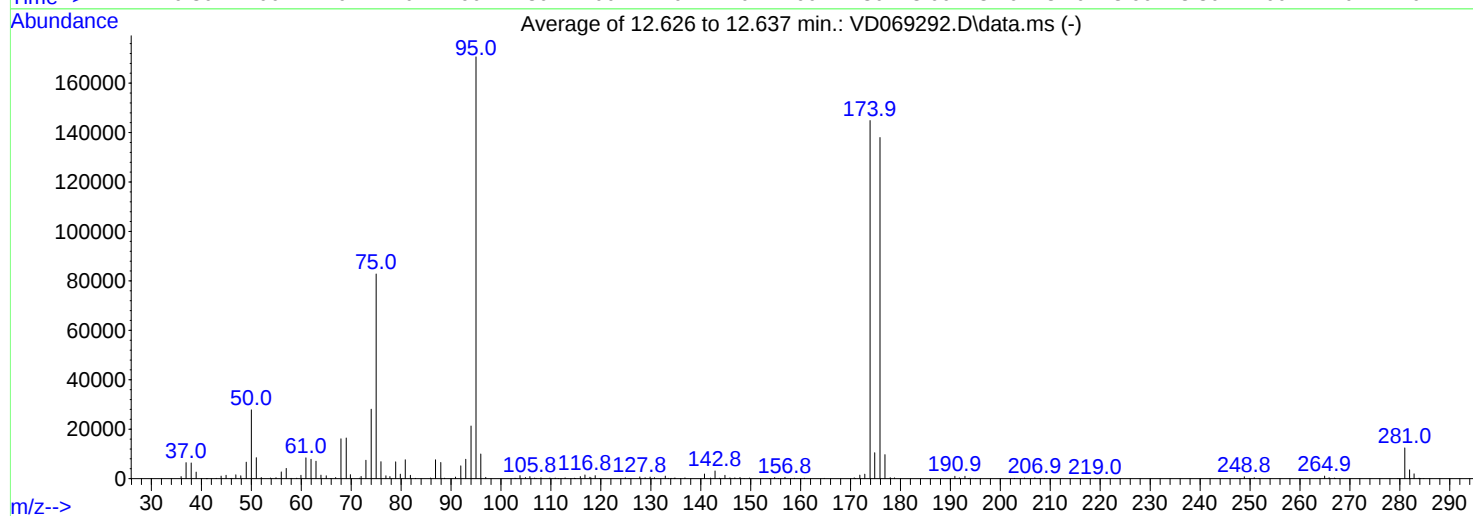


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060221\
 Data File : VD069292.D
 Acq On : 02 Jun 2021 10:38
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060121S.M
 Title : SW846 8260
 Last Update : Wed Jun 02 02:17:36 2021

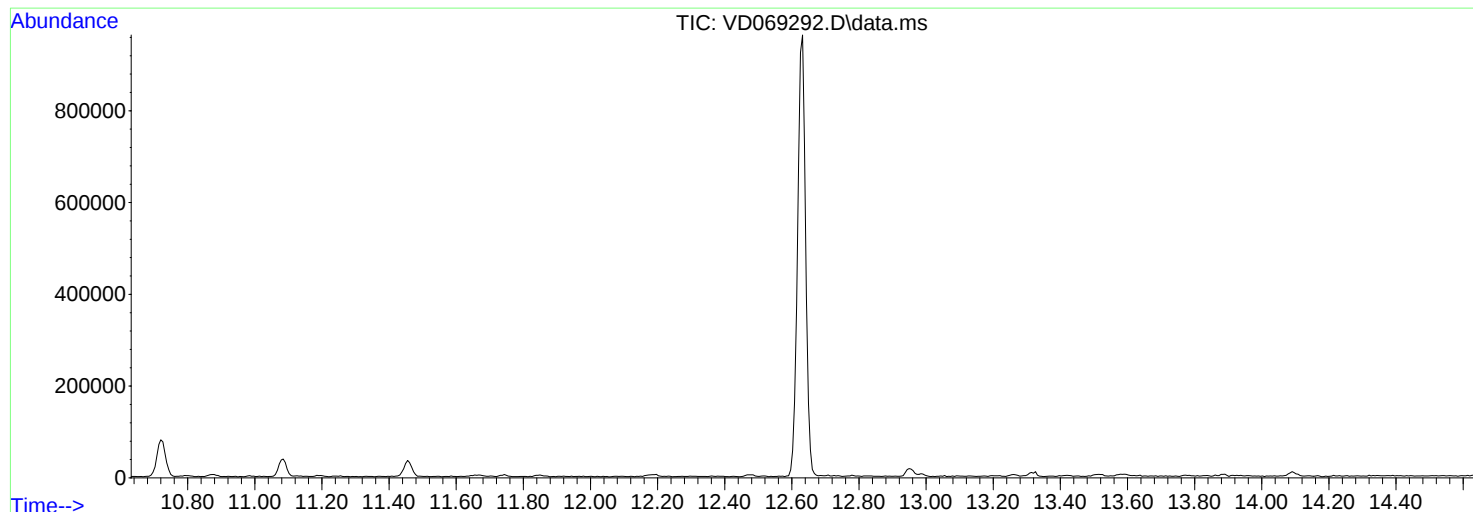

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	27837	PASS
75	95	30	60	48.5	82827	PASS
95	95	100	100	100.0	170645	PASS
96	95	5	9	5.9	9986	PASS
173	174	0.00	2	1.3	1827	PASS
174	95	50	100	84.9	144901	PASS
175	174	5	9	7.3	10513	PASS
176	174	95	101	95.2	138005	PASS
177	176	5	9	7.1	9744	PASS