
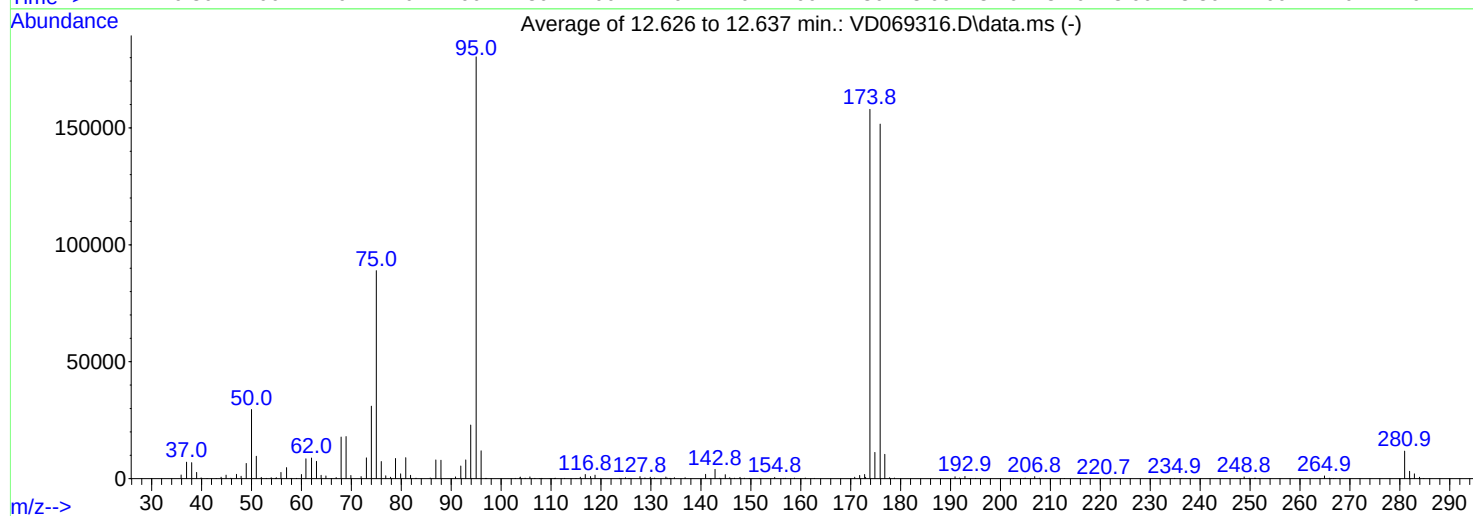


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060321\
Data File : VD069316.D
Acq On : 03 Jun 2021 10:13
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060121S.M
Title : SW846 8260
Last Update : Wed Jun 02 02:17:36 2021

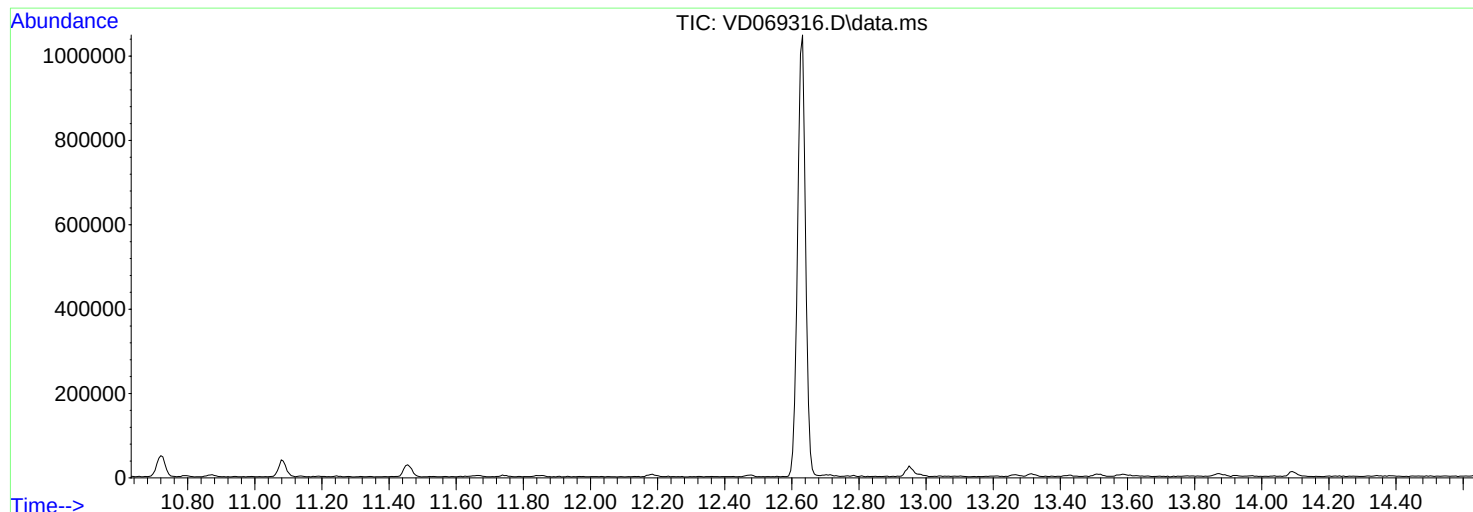

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	29560	PASS
75	95	30	60	49.3	88944	PASS
95	95	100	100	100.0	180373	PASS
96	95	5	9	6.6	11902	PASS
173	174	0.00	2	1.1	1810	PASS
174	95	50	100	87.6	157931	PASS
175	174	5	9	7.1	11216	PASS
176	174	95	101	96.0	151600	PASS
177	176	5	9	6.9	10389	PASS