
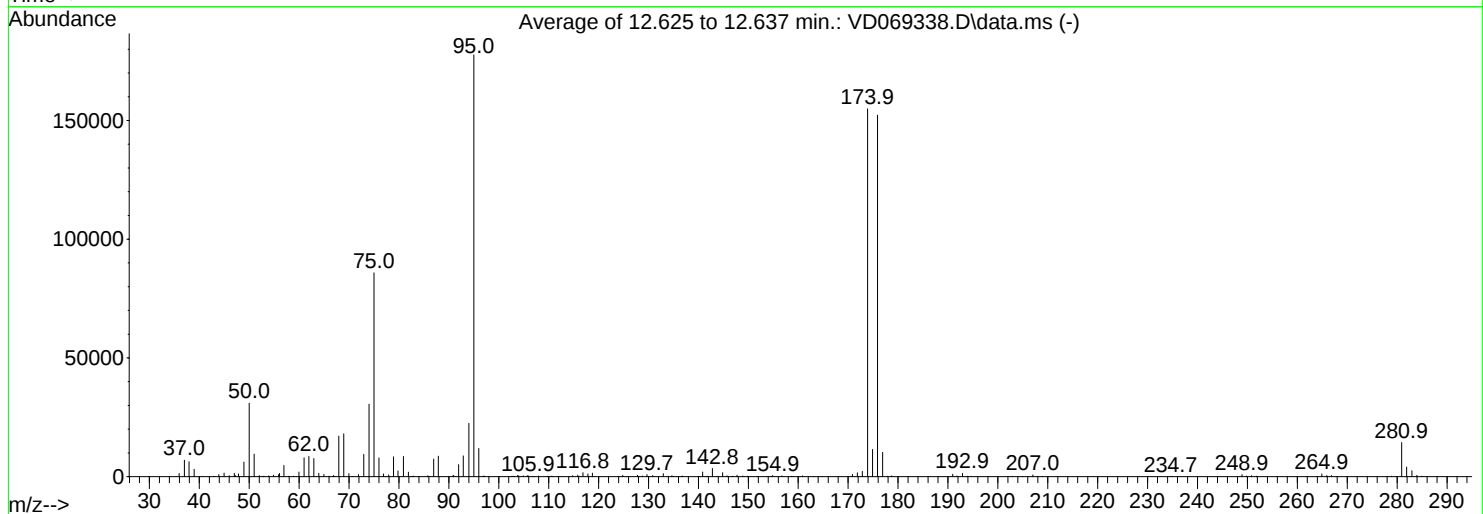


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060421\
Data File : VD069338.D
Acq On : 04 Jun 2021 09:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060121S.M
Title : SW846 8260
Last Update : Wed Jun 02 02:17:36 2021

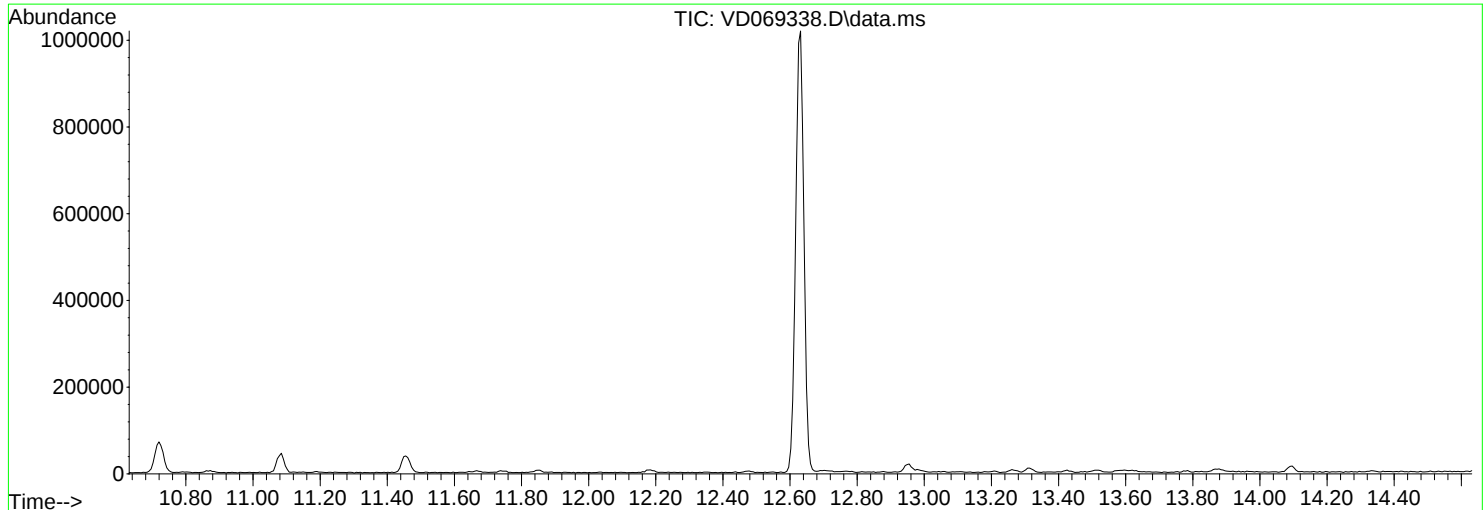

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	30965	PASS
75	95	30	60	48.3	85853	PASS
95	95	100	100	100.0	177643	PASS
96	95	5	9	6.7	11875	PASS
173	174	0.00	2	1.4	2233	PASS
174	95	50	100	87.2	154944	PASS
175	174	5	9	7.4	11435	PASS
176	174	95	101	98.3	152235	PASS
177	176	5	9	6.7	10235	PASS