


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD060519\
 Data File : VD062618.D
 Acq On : 6 Jun 2019 10:27
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060519S.M
 Title : SW846 8260
 Last Update : Thu Jun 06 05:42:40 2019

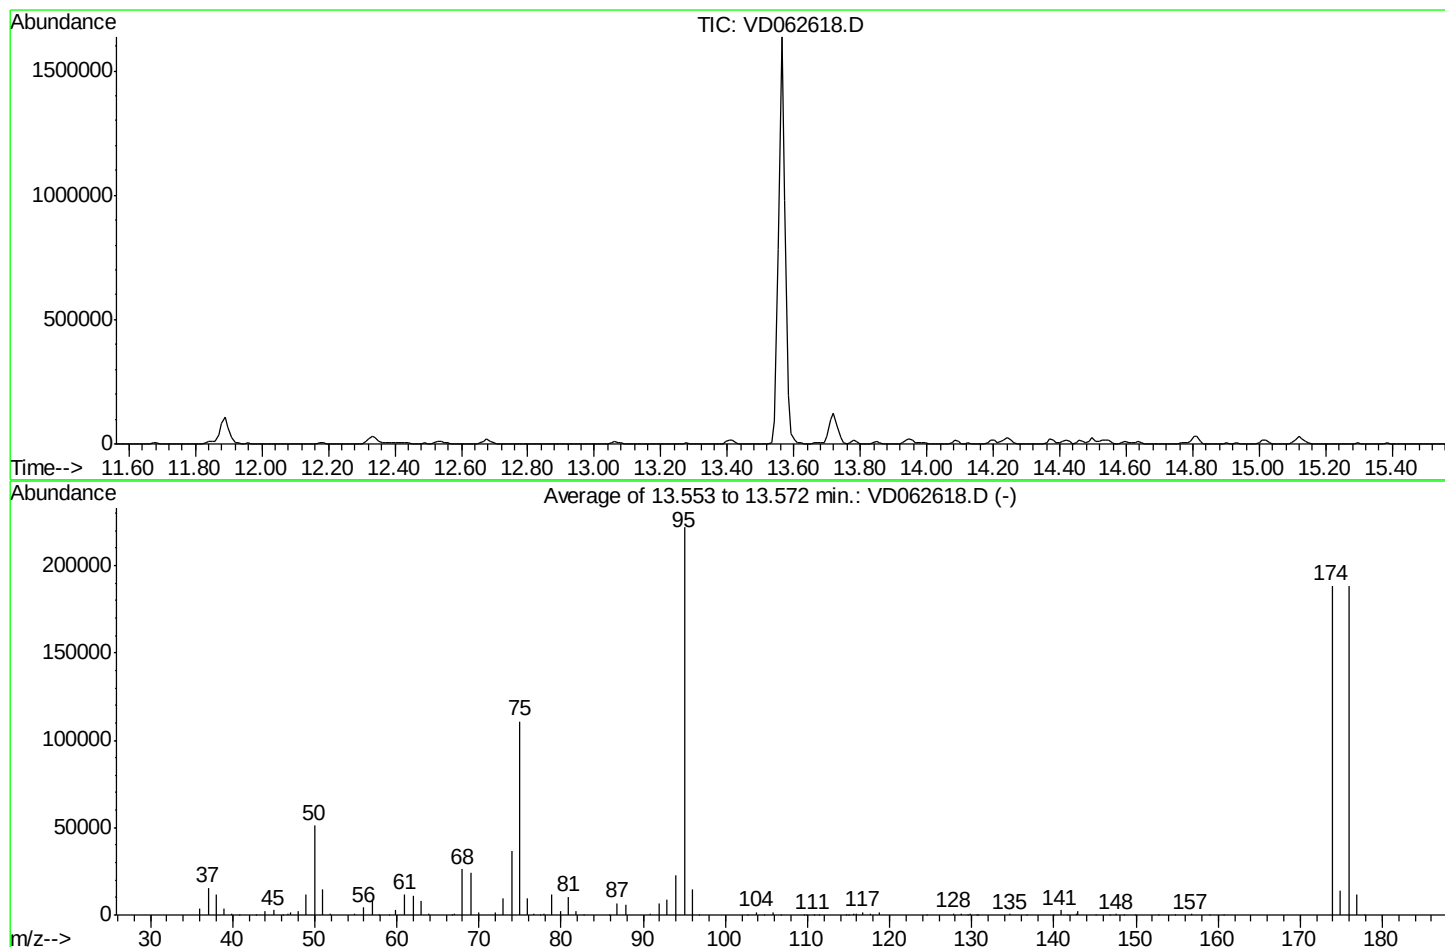

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	51034	PASS
75	95	30	60	50.0	110936	PASS
95	95	100	100	100.0	221845	PASS
96	95	5	9	6.7	14932	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.0	188509	PASS
175	174	5	9	7.3	13721	PASS
176	174	95	101	99.8	188069	PASS
177	176	5	9	6.2	11586	PASS