



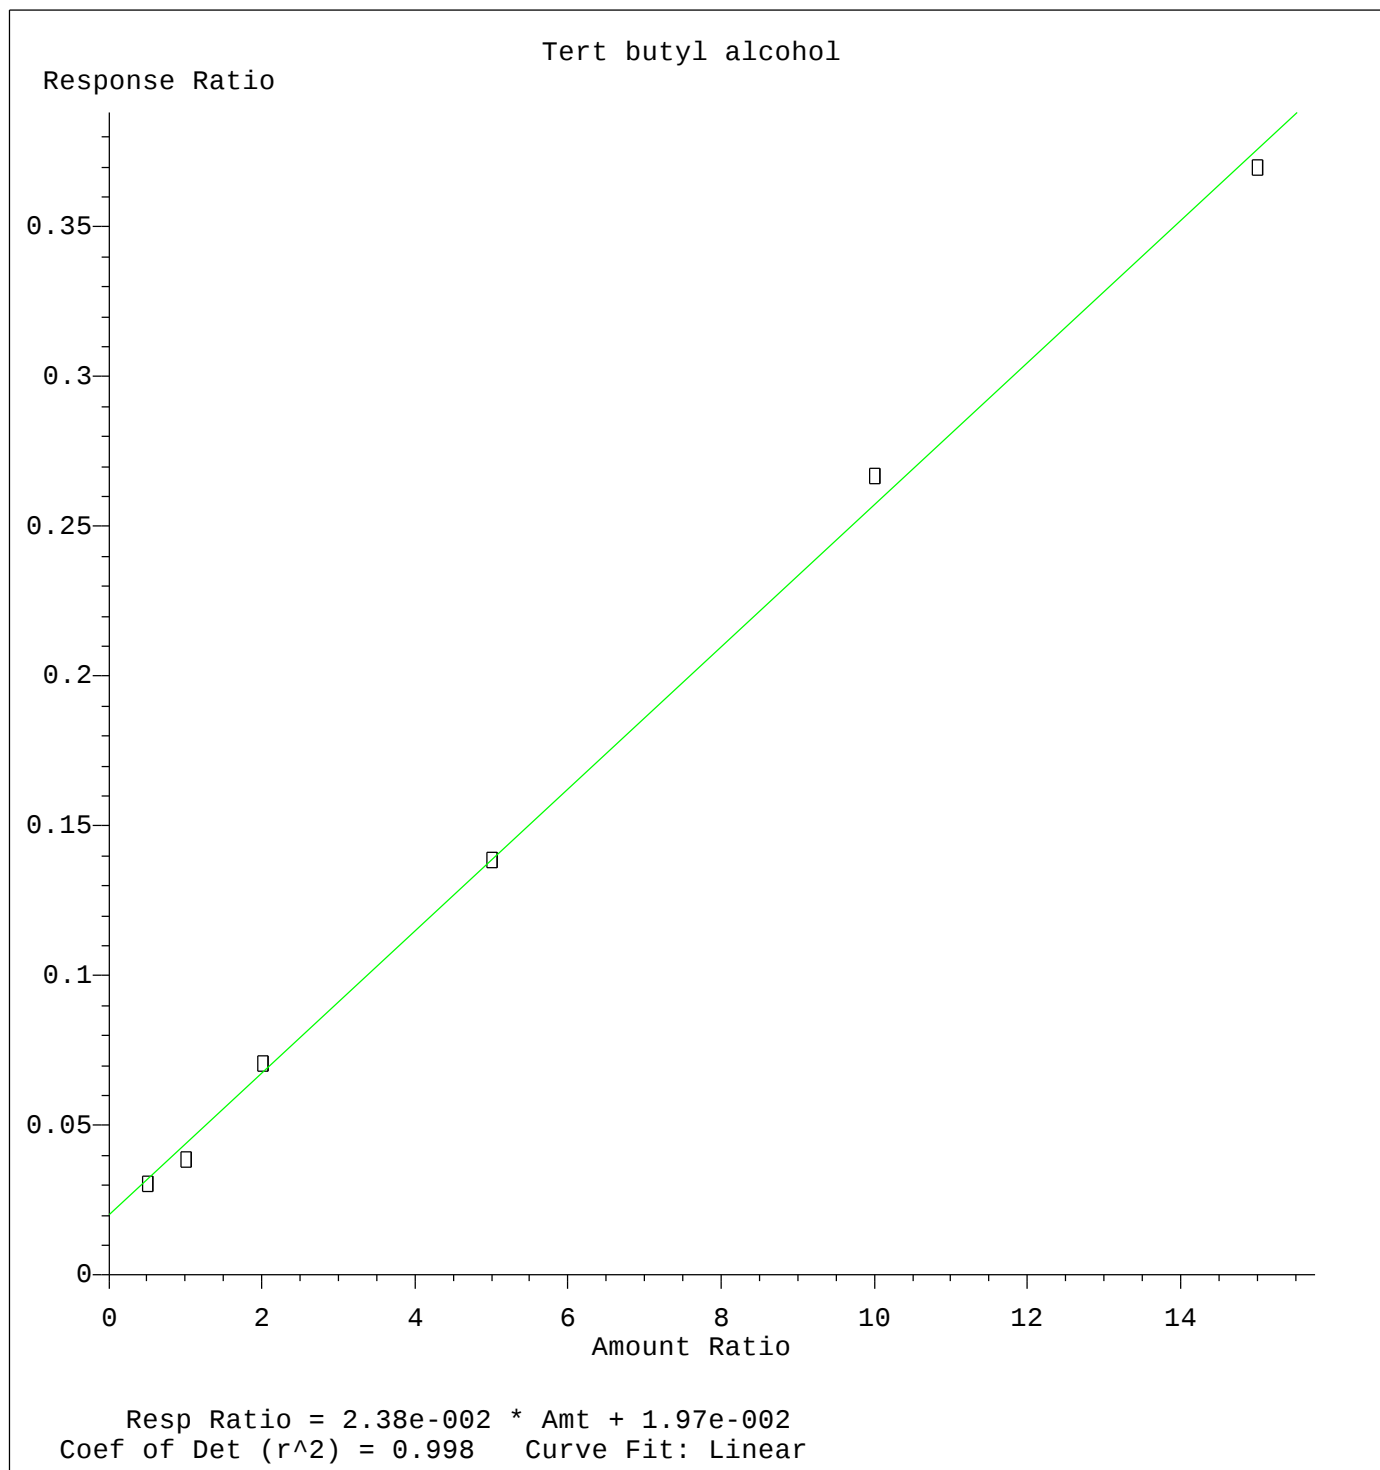

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Calibration Table Last Updated: Fri Jun 05 13:07:30 2020


Methylene Chloride

Response Ratio

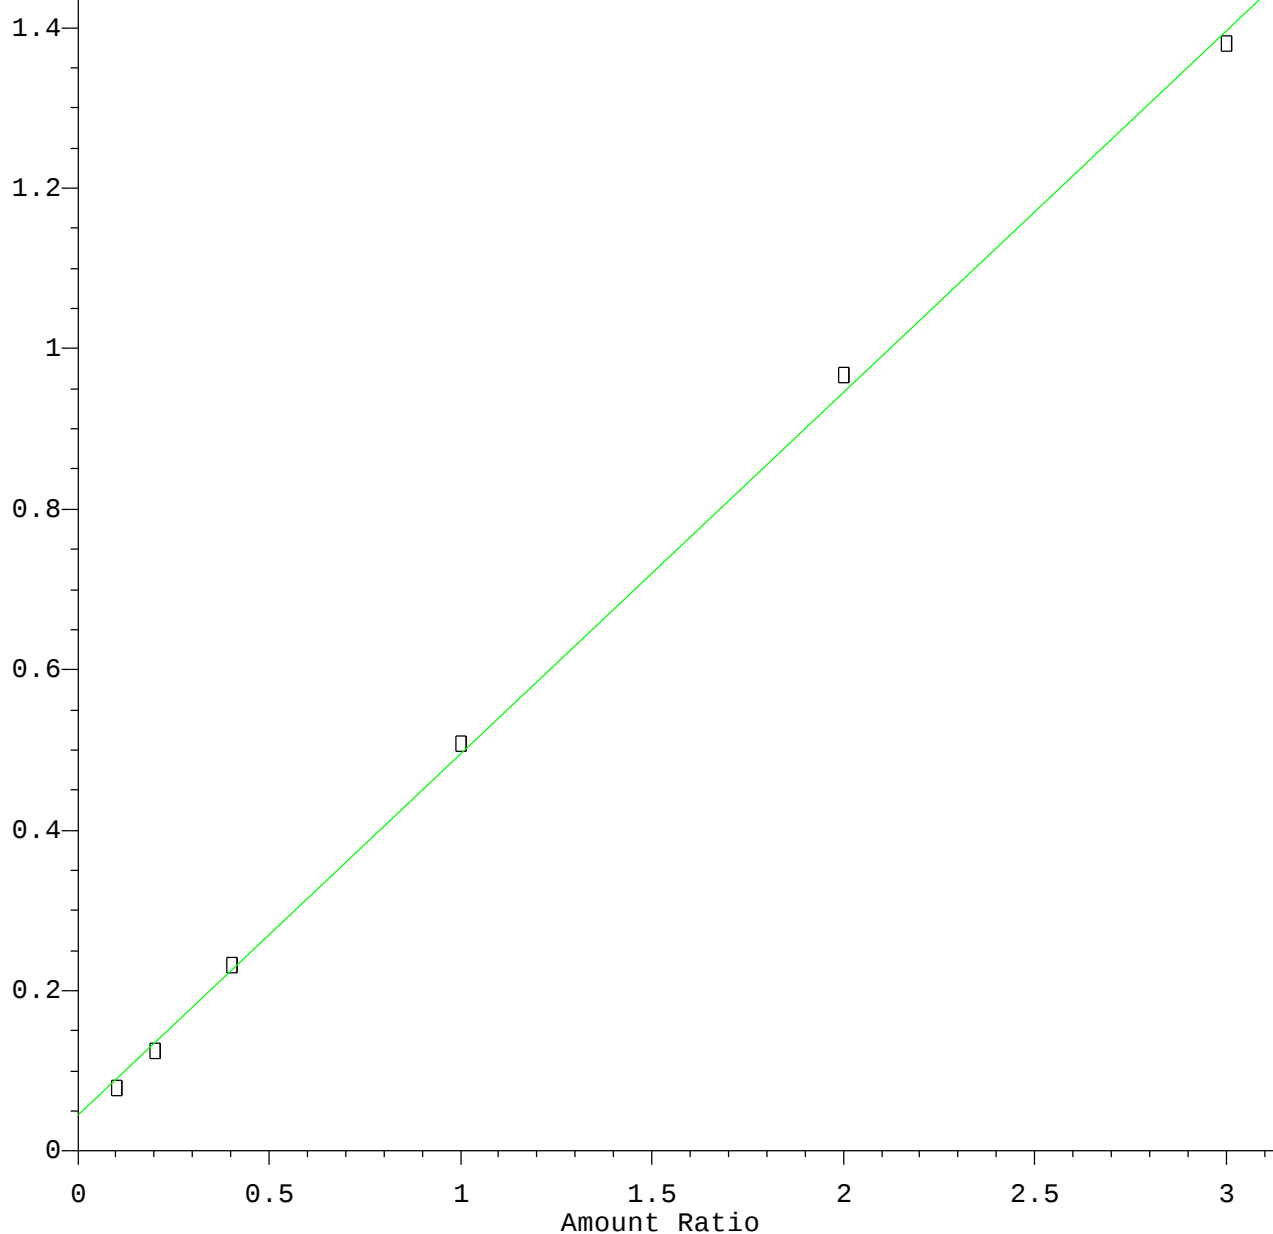


Resp Ratio = $4.51 \times 10^{-1} \times \text{Amt} + 4.40 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Calibration Table Last Updated: Fri Jun 05 13:07:30 2020

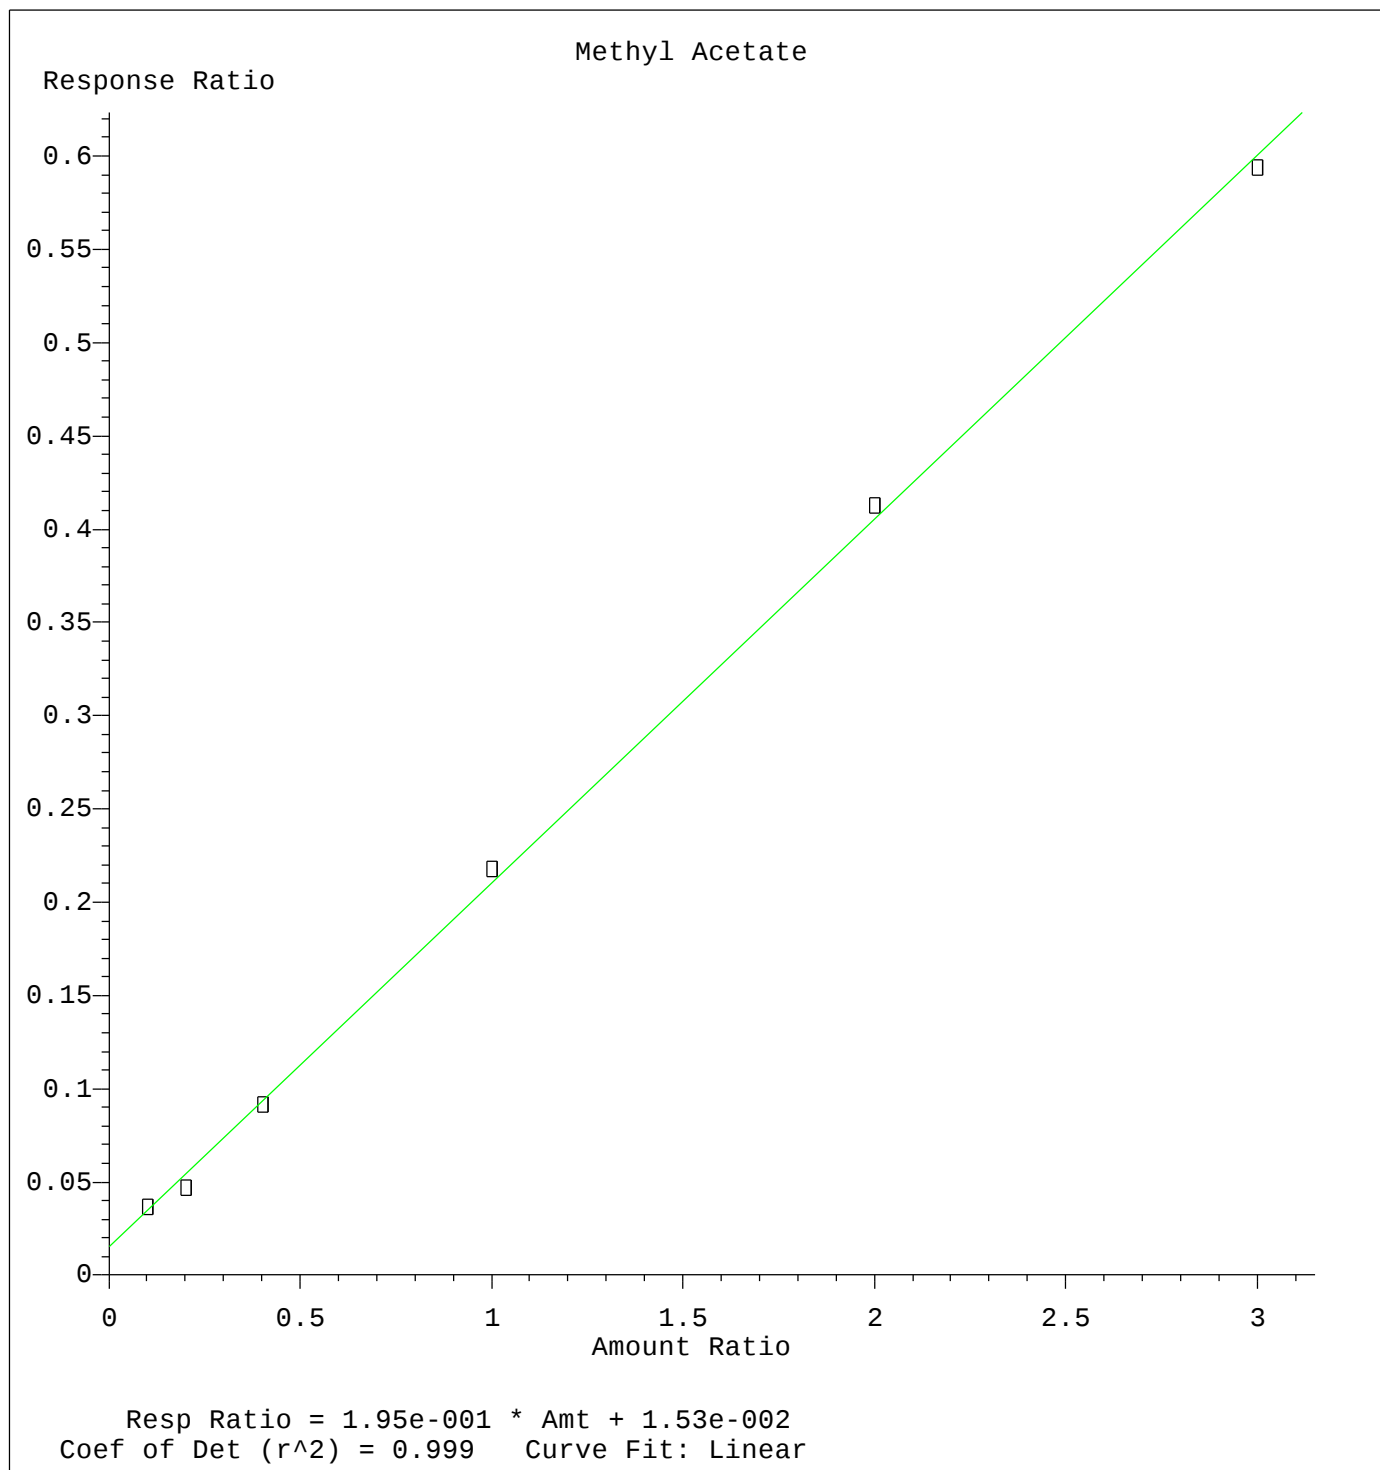


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Calibration Table Last Updated: Fri Jun 05 13:07:30 2020

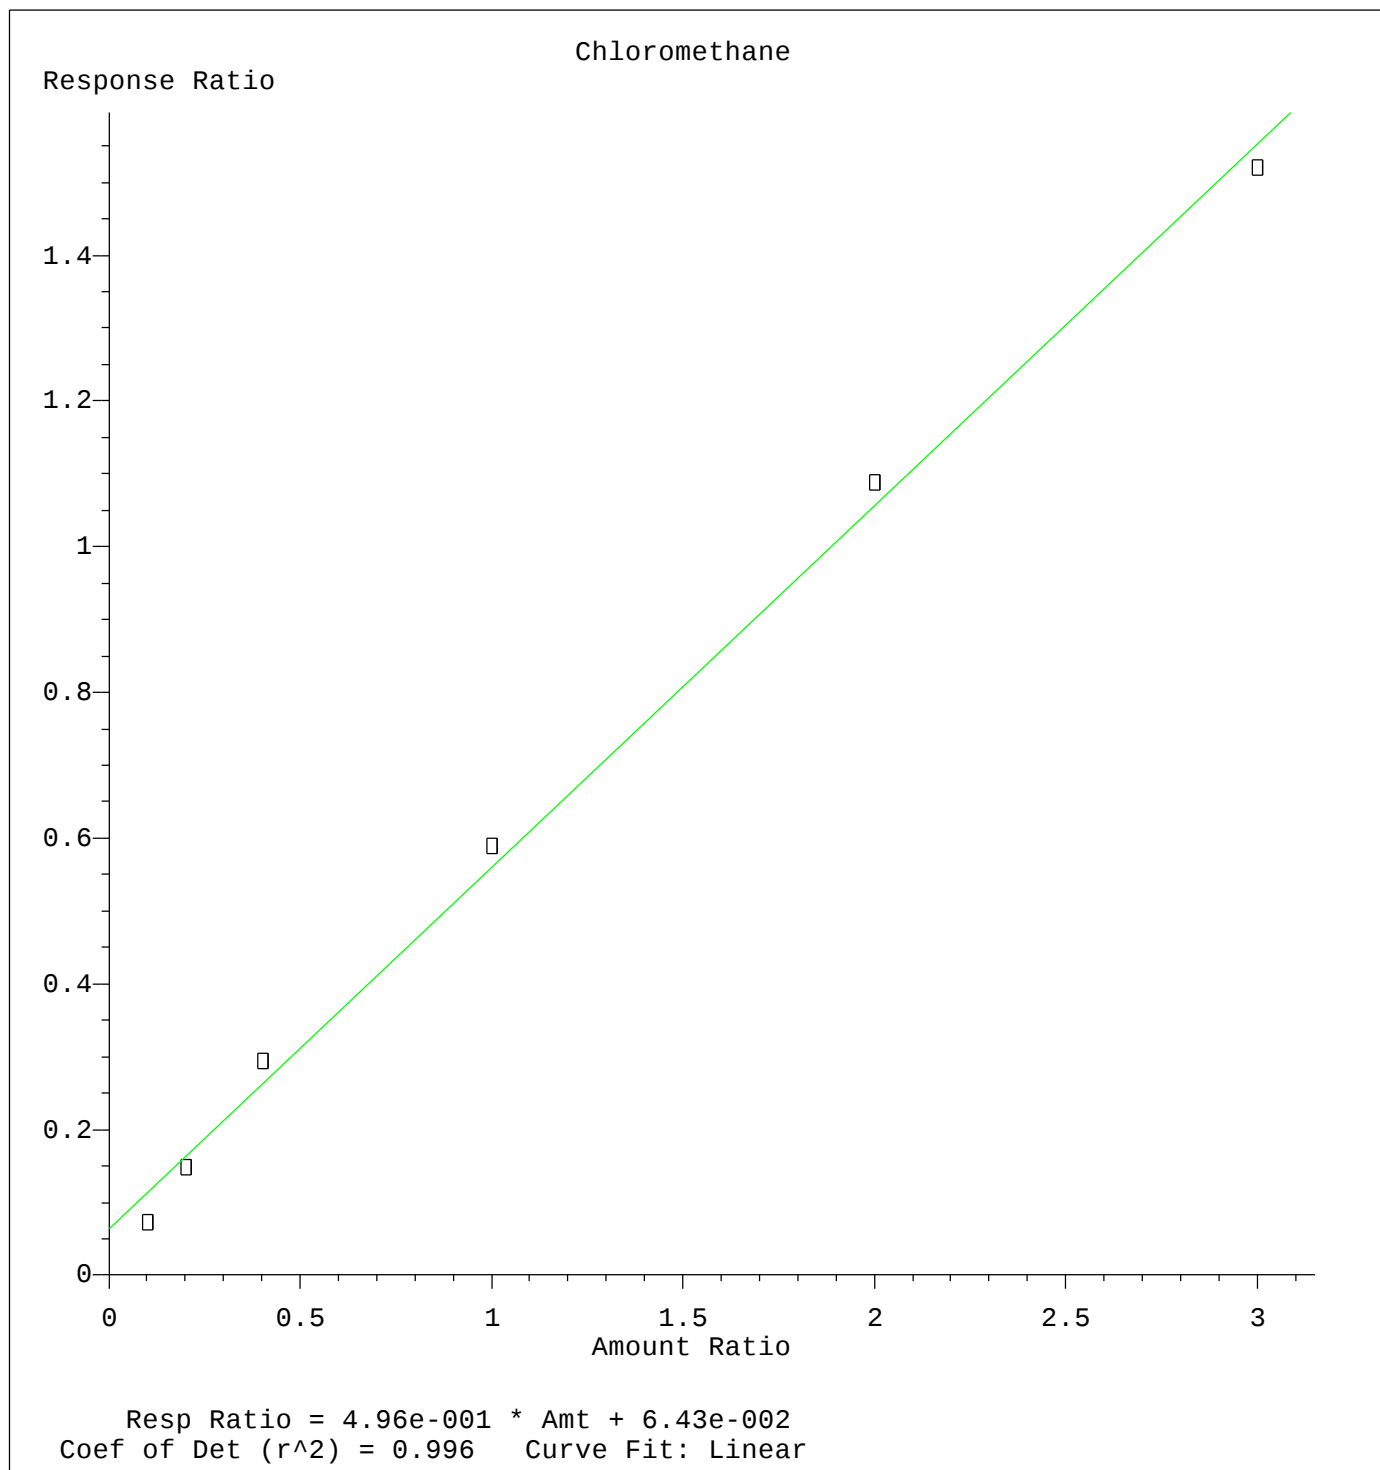

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Calibration Table Last Updated: Fri Jun 05 13:07:30 2020

Dichlorodifluoromethane

Response Ratio

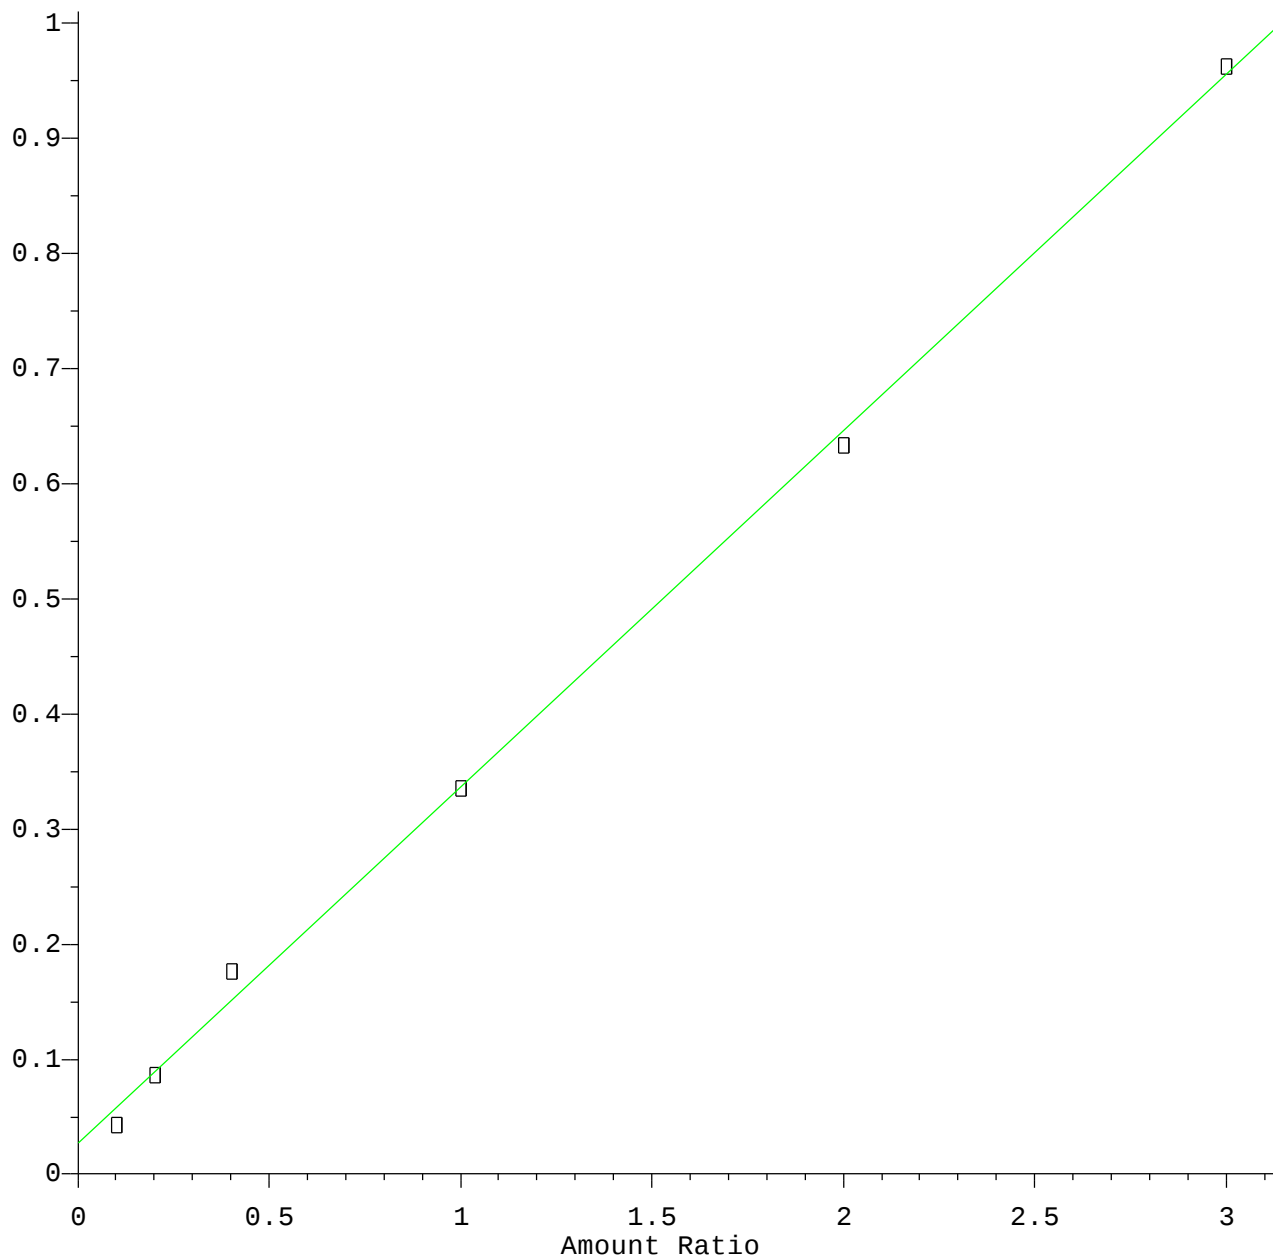

Resp Ratio = $3.10 \times 10^{-1} \times \text{Amt} + 2.65 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Calibration Table Last Updated: Fri Jun 05 13:07:30 2020