


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD060520\
Data File : VD065766.D
Acq On : 05 Jun 2020 09:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
Title : SW846 8260
Last Update : Fri Jun 05 13:07:30 2020

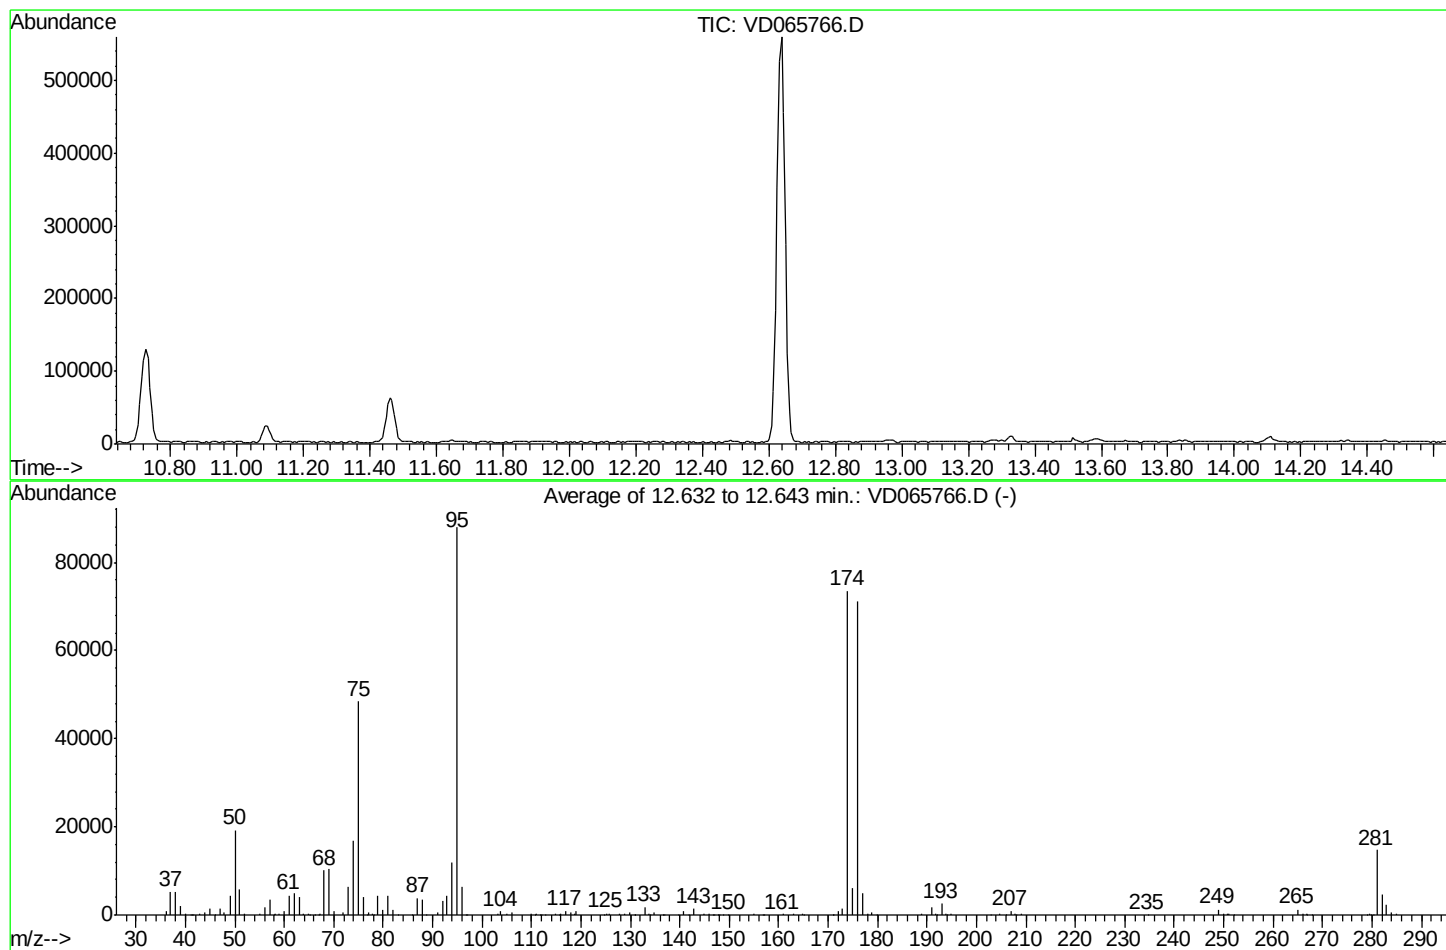

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	19202	PASS
75	95	30	60	55.1	48442	PASS
95	95	100	100	100.0	87954	PASS
96	95	5	9	7.1	6269	PASS
173	174	0.00	2	1.9	1371	PASS
174	95	50	100	83.6	73533	PASS
175	174	5	9	8.5	6227	PASS
176	174	95	101	96.8	71181	PASS
177	176	5	9	7.0	4966	PASS