


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD060619\
Data File : VD062626.D
Acq On : 6 Jun 2019 15:24
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060619S.M
Title : SW846 8260
Last Update : Fri Jun 07 05:01:52 2019

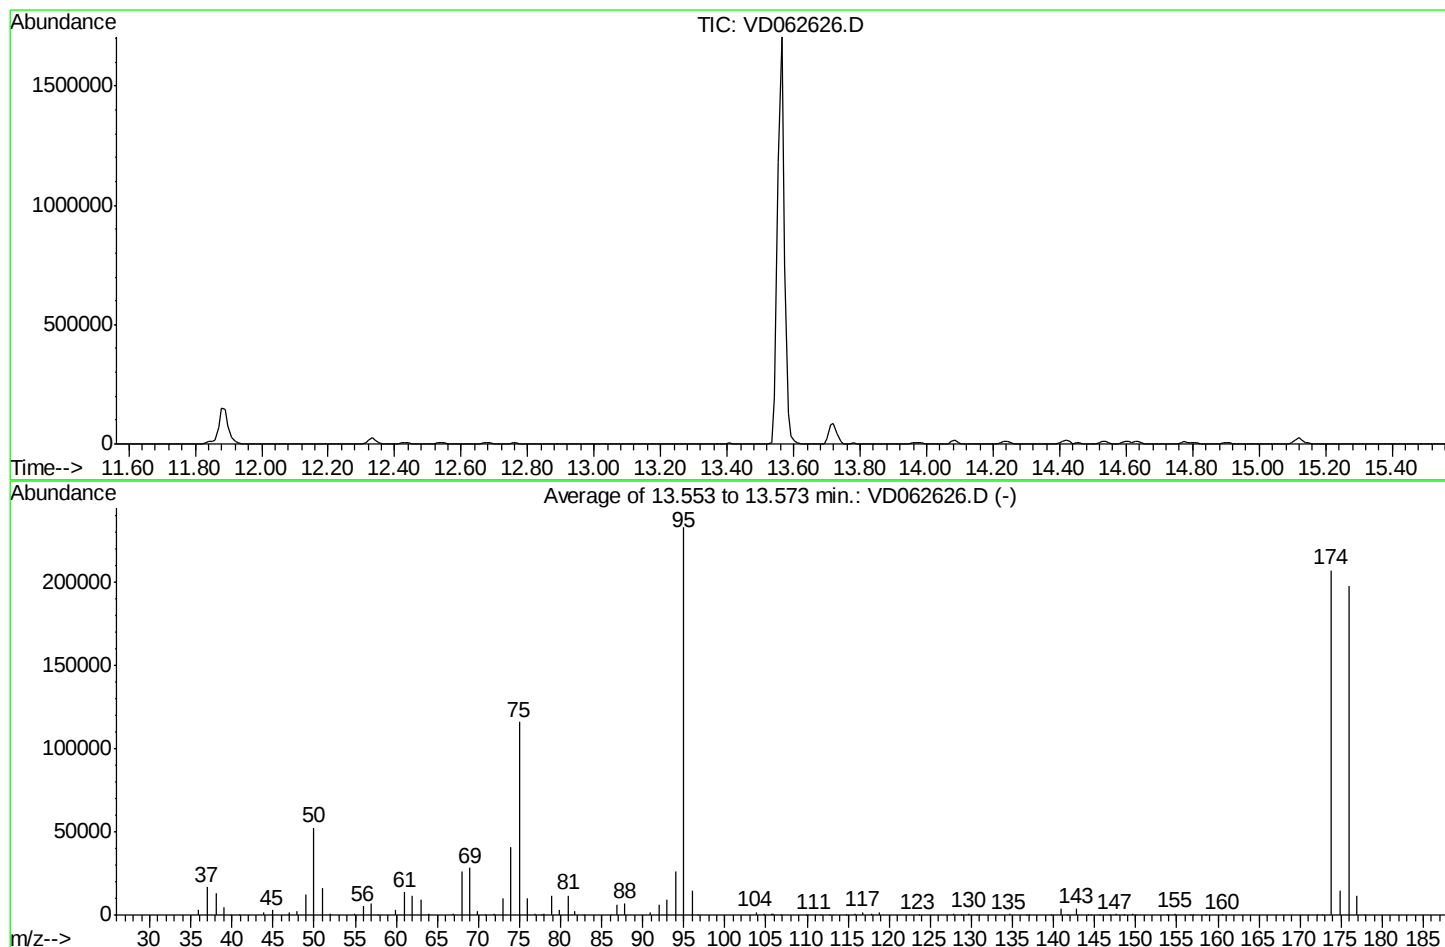

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	52621	PASS
75	95	30	60	49.7	115952	PASS
95	95	100	100	100.0	233178	PASS
96	95	5	9	6.2	14450	PASS
173	174	0.00	2	0.2	383	PASS
174	95	50	100	89.0	207445	PASS
175	174	5	9	6.9	14366	PASS
176	174	95	101	95.6	198229	PASS
177	176	5	9	5.8	11470	PASS