

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD060622\  
 Data File : VD073481.D  
 Acq On : 06 Jun 2022 18:17  
 Operator : VA/SY  
 Sample : N3186-03  
 Misc : 5.04G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 VNJ-218

Quant Time: Jun 07 01:13:56 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D051922S.M  
 Quant Title : SW846 8260  
 QLast Update : Thu May 19 15:13:42 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.973  | 168  | 283785   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.855  | 114  | 518808   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.632 | 117  | 600271   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.561 | 152  | 310845   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.320  | 65    | 144748   | 46.154   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 92.300%  |
| 35) Dibromofluoromethane    | 7.908  | 113   | 163506   | 47.761   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 95.520%  |
| 50) Toluene-d8              | 10.332 | 98    | 644728   | 51.089   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 102.180% |
| 62) 4-Bromofluorobenzene    | 12.620 | 95    | 301081   | 67.983   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 135.960% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD060622\  
Data File : VD073481.D  
Acq On : 06 Jun 2022 18:17  
Operator : VA/SY  
Sample : N3186-03  
Misc : 5.04G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-218

Quant Time: Jun 07 01:13:56 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D051922S.M  
Quant Title : SW846 8260  
QLast Update : Thu May 19 15:13:42 2022  
Response via : Initial Calibration




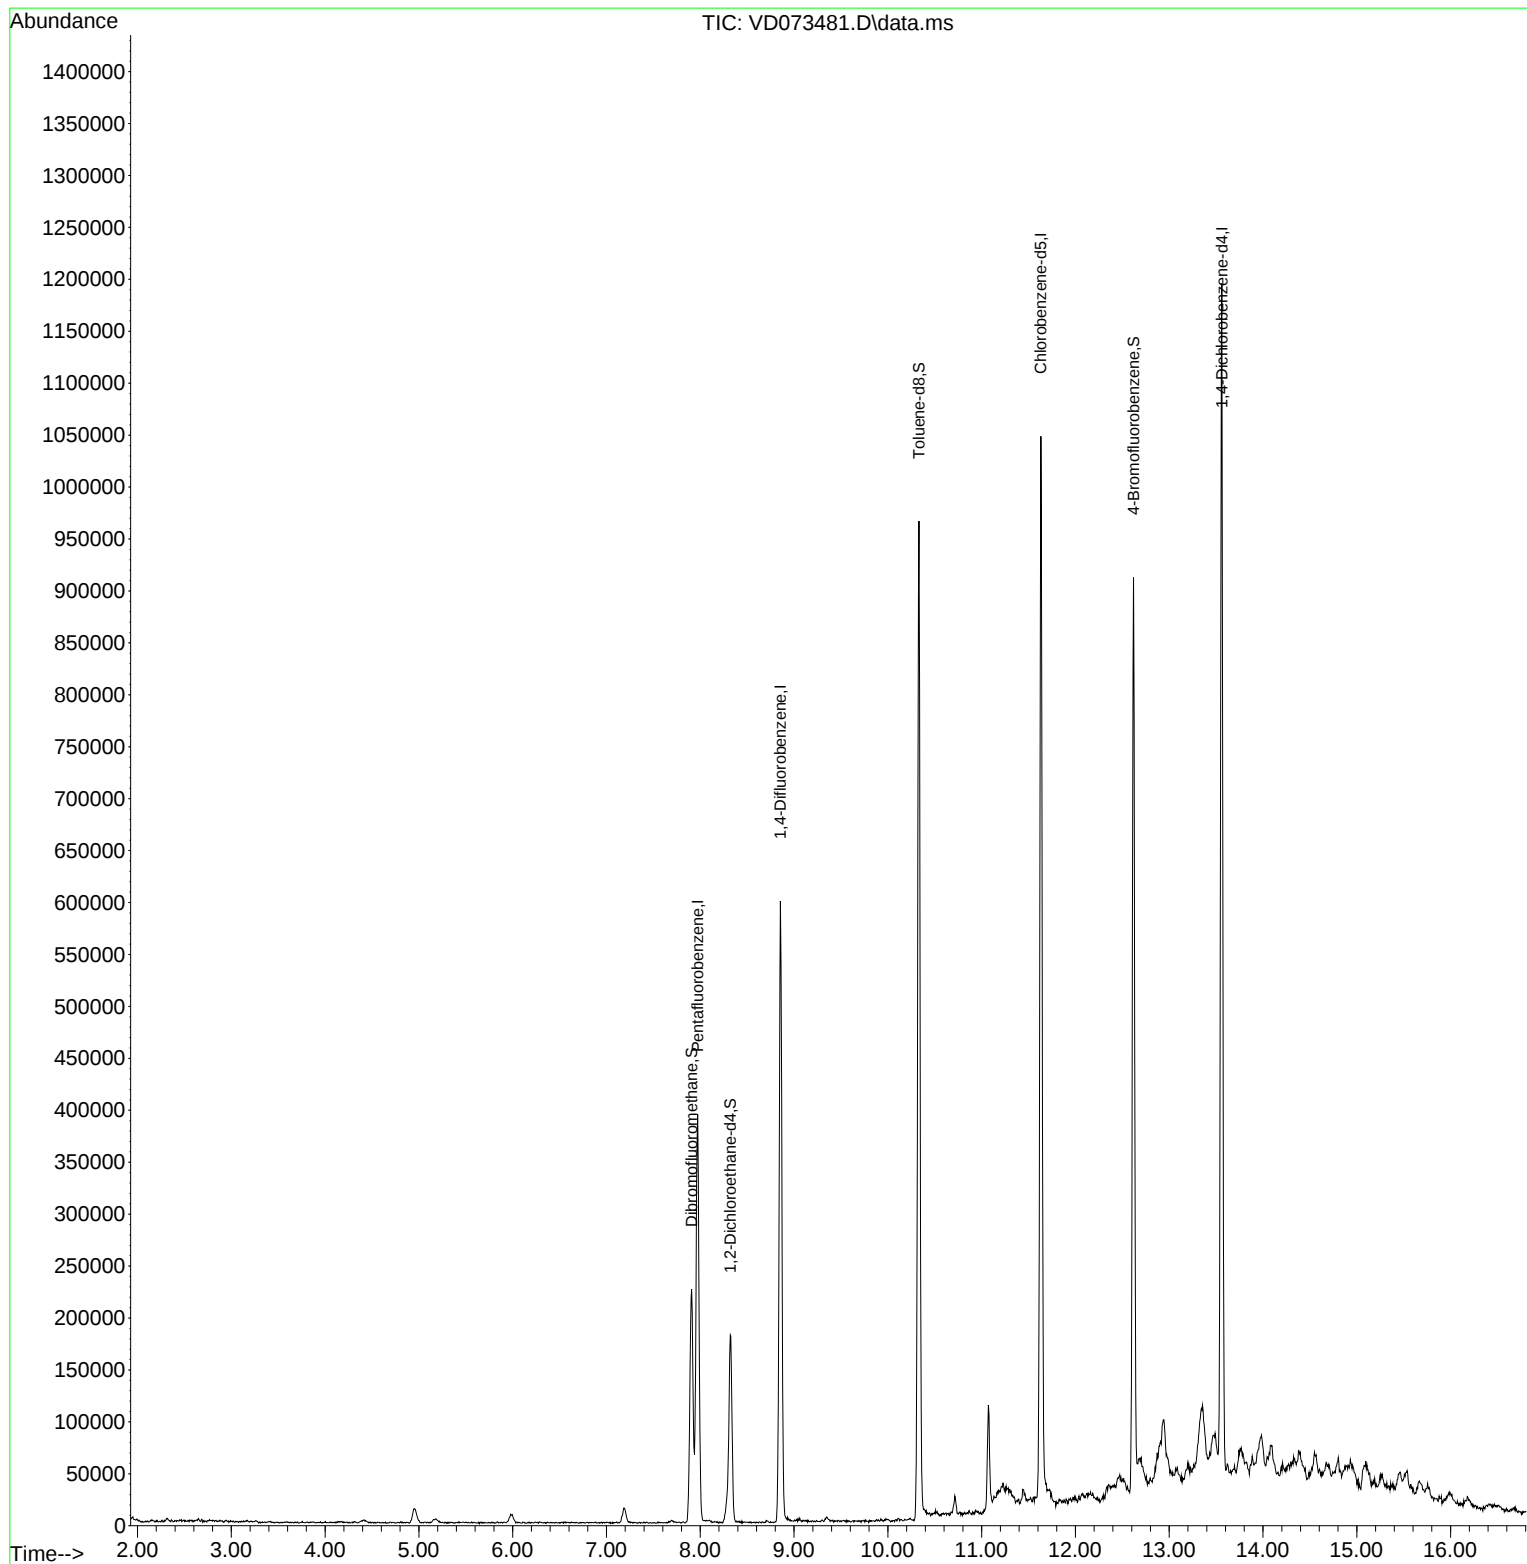


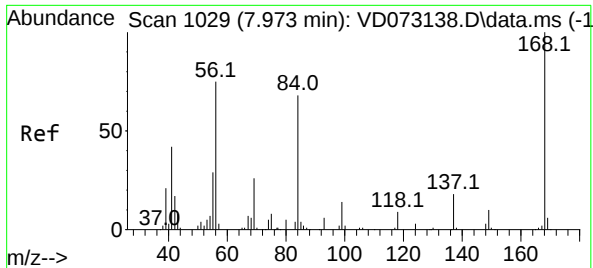

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.973 min Scan# 1029  
Delta R.T. -0.000 min  
Lab File: VD073481.D  
Acq: 06 Jun 2022 18:17




Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-218


Tgt Ion:168 Resp: 283785  
Ion Ratio Lower Upper  
168 100  
99 58.2 49.8 74.6

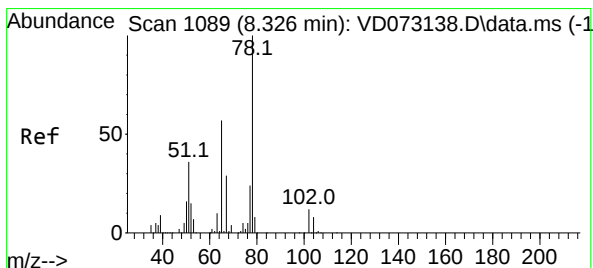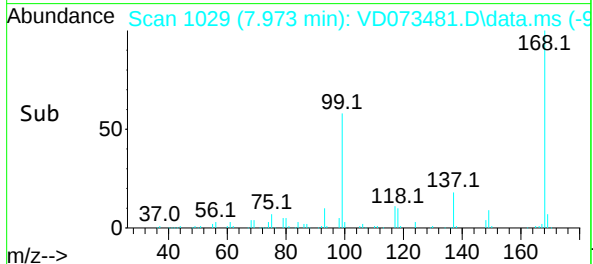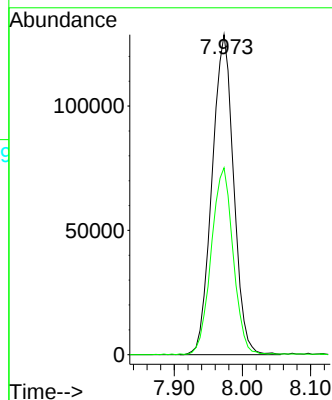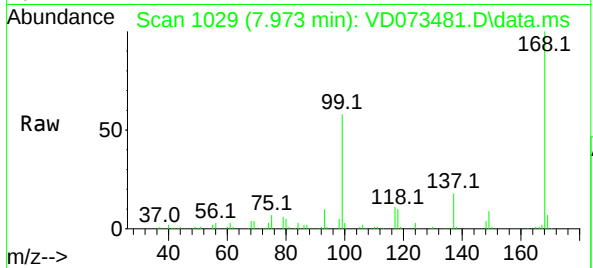

#33  
1,2-Dichloroethane-d4  
Concen: 46.154 ug/l  
RT: 8.320 min Scan# 1088  
Delta R.T. -0.006 min  
Lab File: VD073481.D  
Acq: 06 Jun 2022 18:17

Tgt Ion: 65 Resp: 144748  
Ion Ratio Lower Upper  
65 100  
67 52.9 0.0 101.4

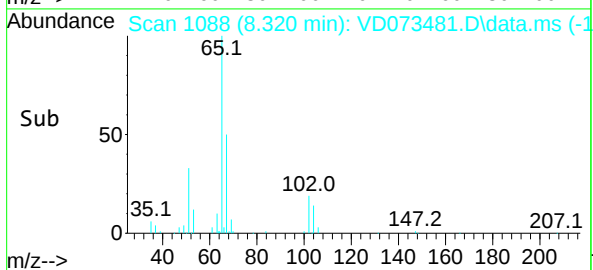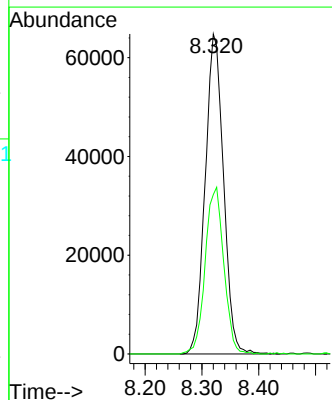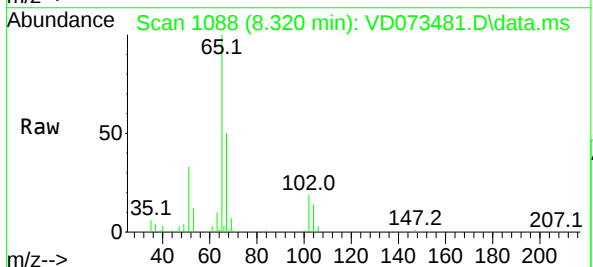

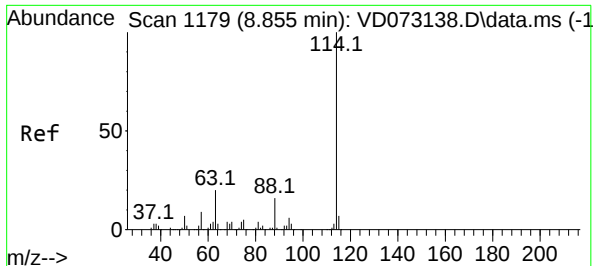

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VD073481.D

Acq: 06 Jun 2022 18:17

Instrument :

MSVOA\_D

ClientSampleId :

VNJ-218





Tgt Ion:114 Resp: 518808

Ion Ratio Lower Upper

114 100

63 19.6 0.0 46.6

88 14.9 0.0 33.2

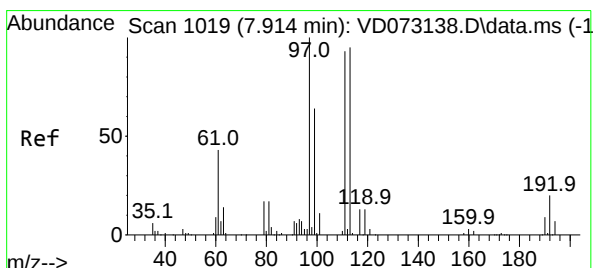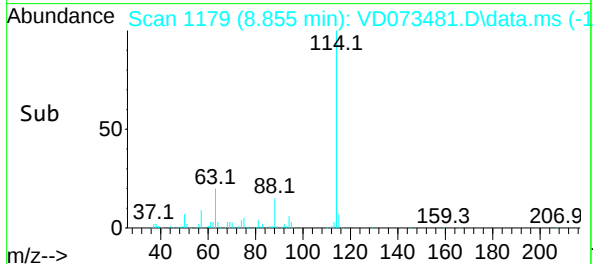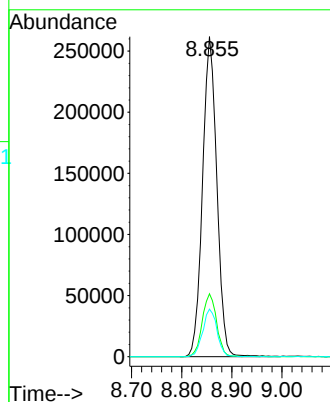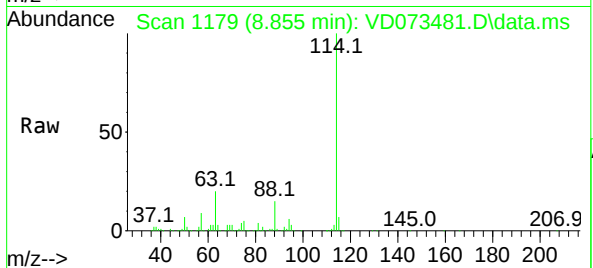

#35

Dibromofluoromethane

Concen: 47.761 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. -0.006 min

Lab File: VD073481.D

Acq: 06 Jun 2022 18:17




Tgt Ion:113 Resp: 163506


Ion Ratio Lower Upper

113 100

111 105.2 83.8 125.6

192 18.4 14.6 21.8

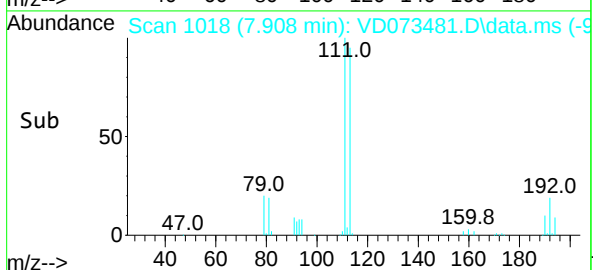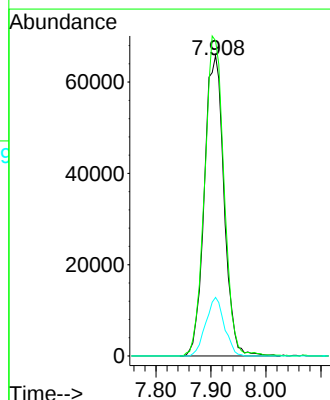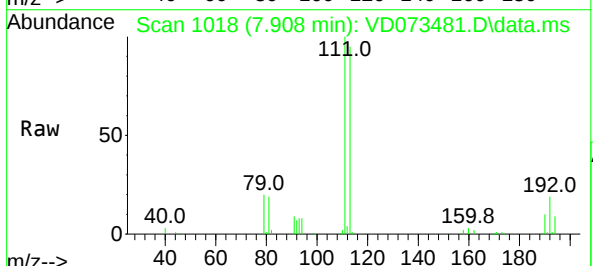

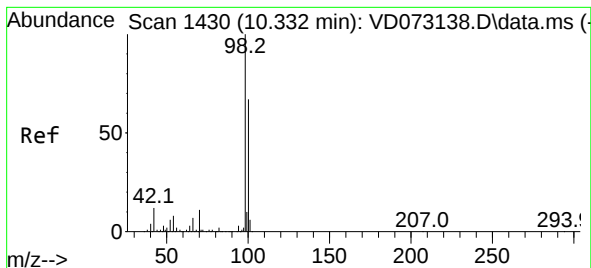

#50

Toluene-d8

Concen: 51.089 ug/l

RT: 10.332 min Scan# 1430

Delta R.T. -0.000 min

Lab File: VD073481.D

Acq: 06 Jun 2022 18:17

Instrument :

MSVOA\_D

ClientSampleId :





VNJ-218

Tgt Ion: 98 Resp: 644728

Ion Ratio Lower Upper

98 100

100 66.9 52.4 78.6

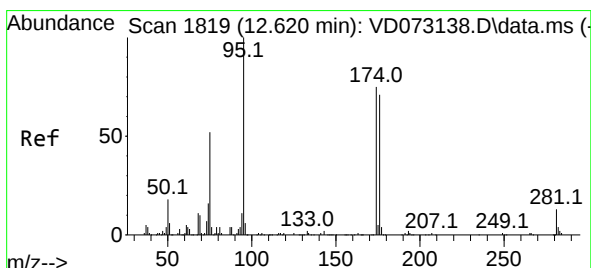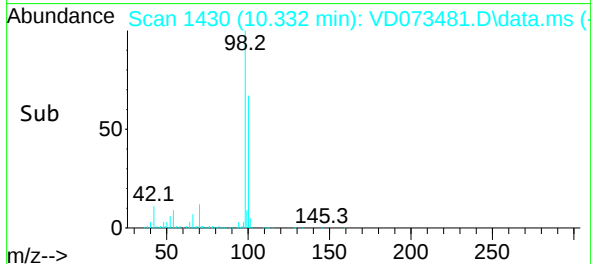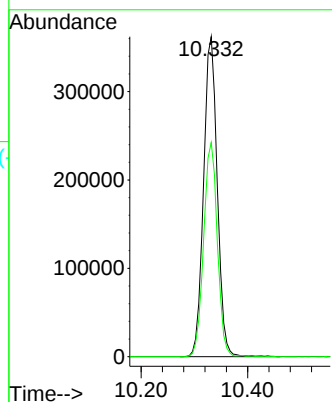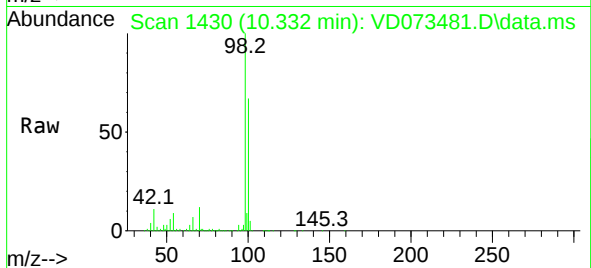

#62

4-Bromofluorobenzene

Concen: 67.983 ug/l

RT: 12.620 min Scan# 1819

Delta R.T. -0.000 min

Lab File: VD073481.D

Acq: 06 Jun 2022 18:17




Tgt Ion: 95 Resp: 301081


Ion Ratio Lower Upper

95 100

174 77.4 0.0 152.8

176 74.2 0.0 145.4


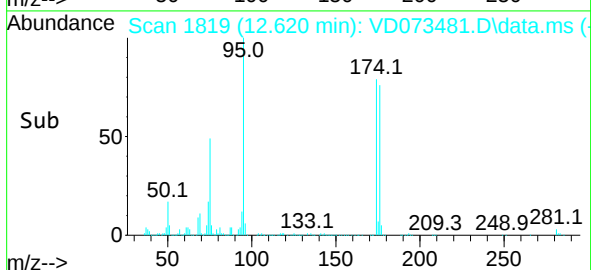
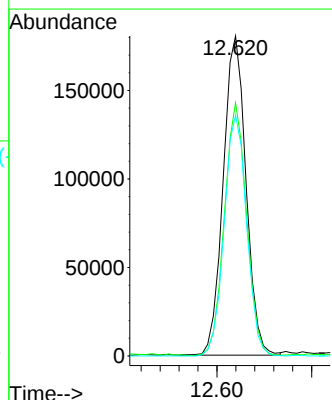
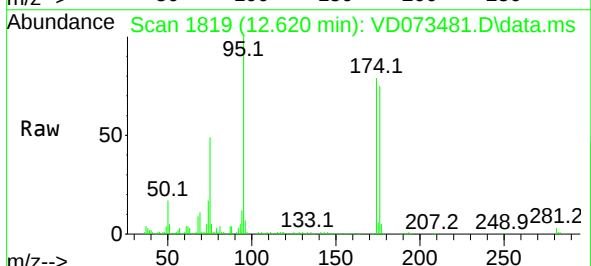


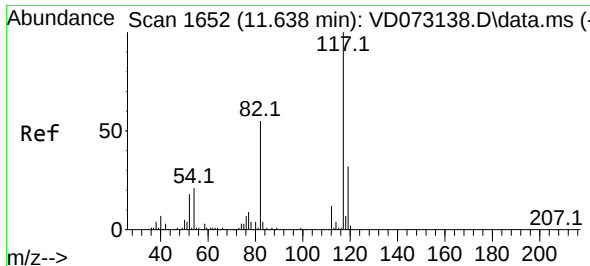

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.632 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: VD073481.D  
Acq: 06 Jun 2022 18:17

Instrument :  
MSVOA\_D  
ClientSampleId :  
VNJ-218

Tgt Ion:117 Resp: 600271  
Ion Ratio Lower Upper  
117 100  
82 53.9 45.3 67.9  
119 33.1 26.6 40.0

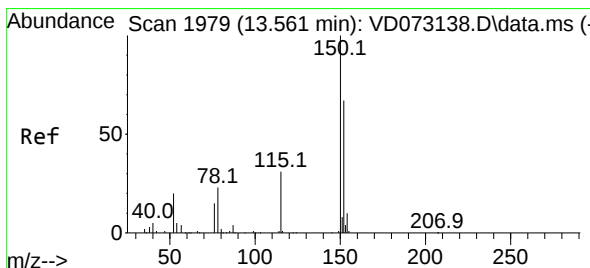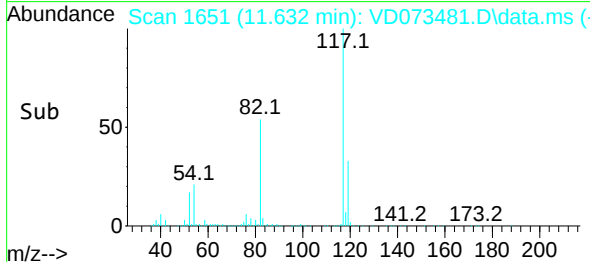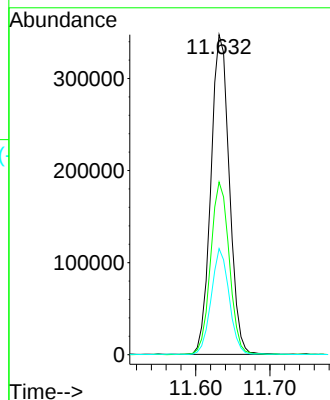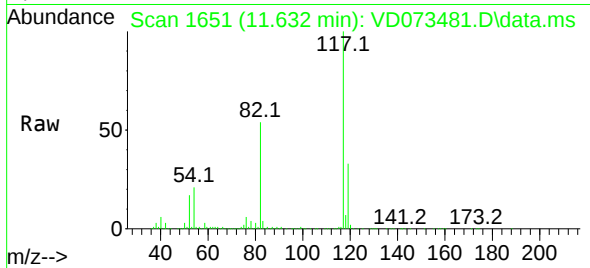

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.561 min Scan# 1979  
Delta R.T. -0.000 min  
Lab File: VD073481.D  
Acq: 06 Jun 2022 18:17

Tgt Ion:152 Resp: 310845  
Ion Ratio Lower Upper  
152 100  
115 60.3 31.3 93.8  
150 158.2 0.0 348.6

