
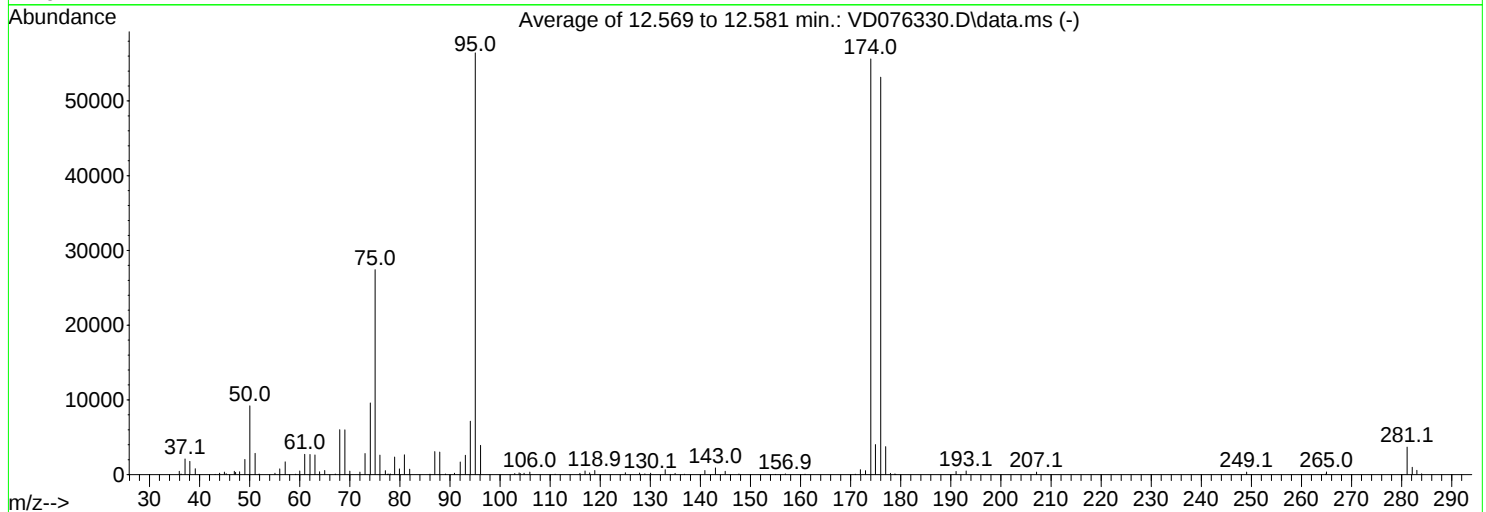


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060623\
Data File : VD076330.D
Acq On : 06 Jun 2023 09:23
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060523S.M
Title : SW846 8260
Last Update : Tue Jun 06 02:52:23 2023

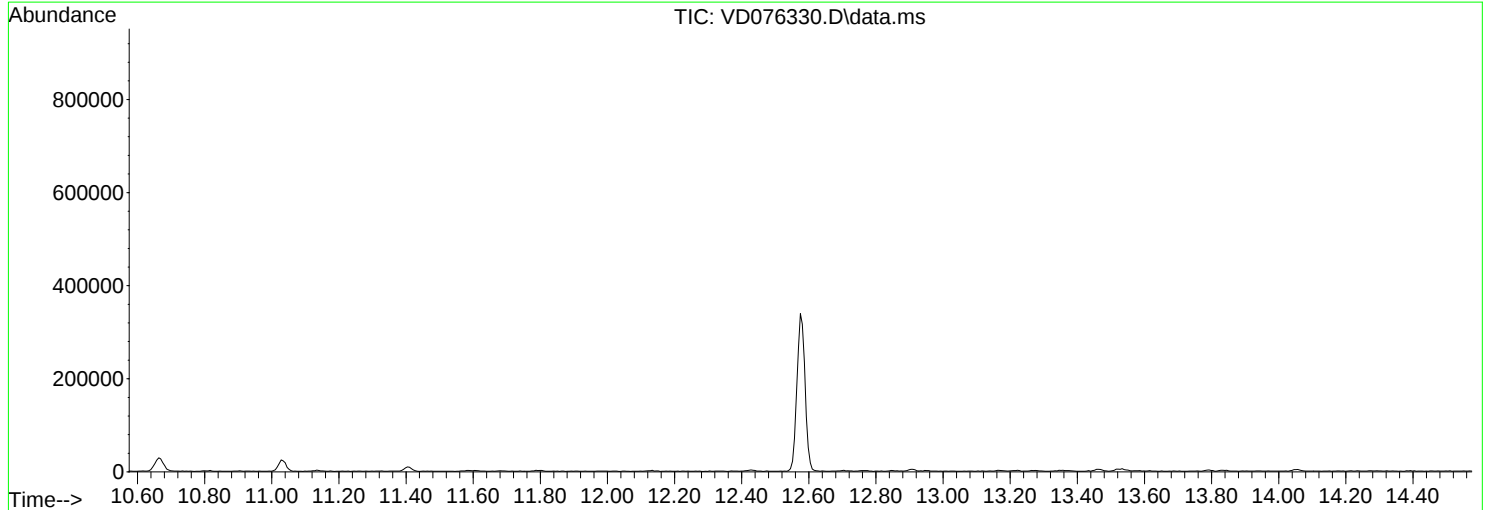

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9216	PASS
75	95	30	60	48.6	27424	PASS
95	95	100	100	100.0	56437	PASS
96	95	5	9	7.0	3927	PASS
173	174	0.00	2	1.0	529	PASS
174	95	50	100	98.6	55627	PASS
175	174	5	9	7.3	4035	PASS
176	174	95	101	95.6	53173	PASS
177	176	5	9	7.1	3753	PASS