


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD060718\  
 Data File : VD057965.D  
 Acq On : 7 Jun 2018 10:12  
 Operator : JC/SY  
 Sample : BFB  
 Misc : 5.00q/5ml/MSVOA D/SOIL  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D060618S.M  
 Title : SW846 8260  
 Last Update : Thu Jun 07 08:57:33 2018

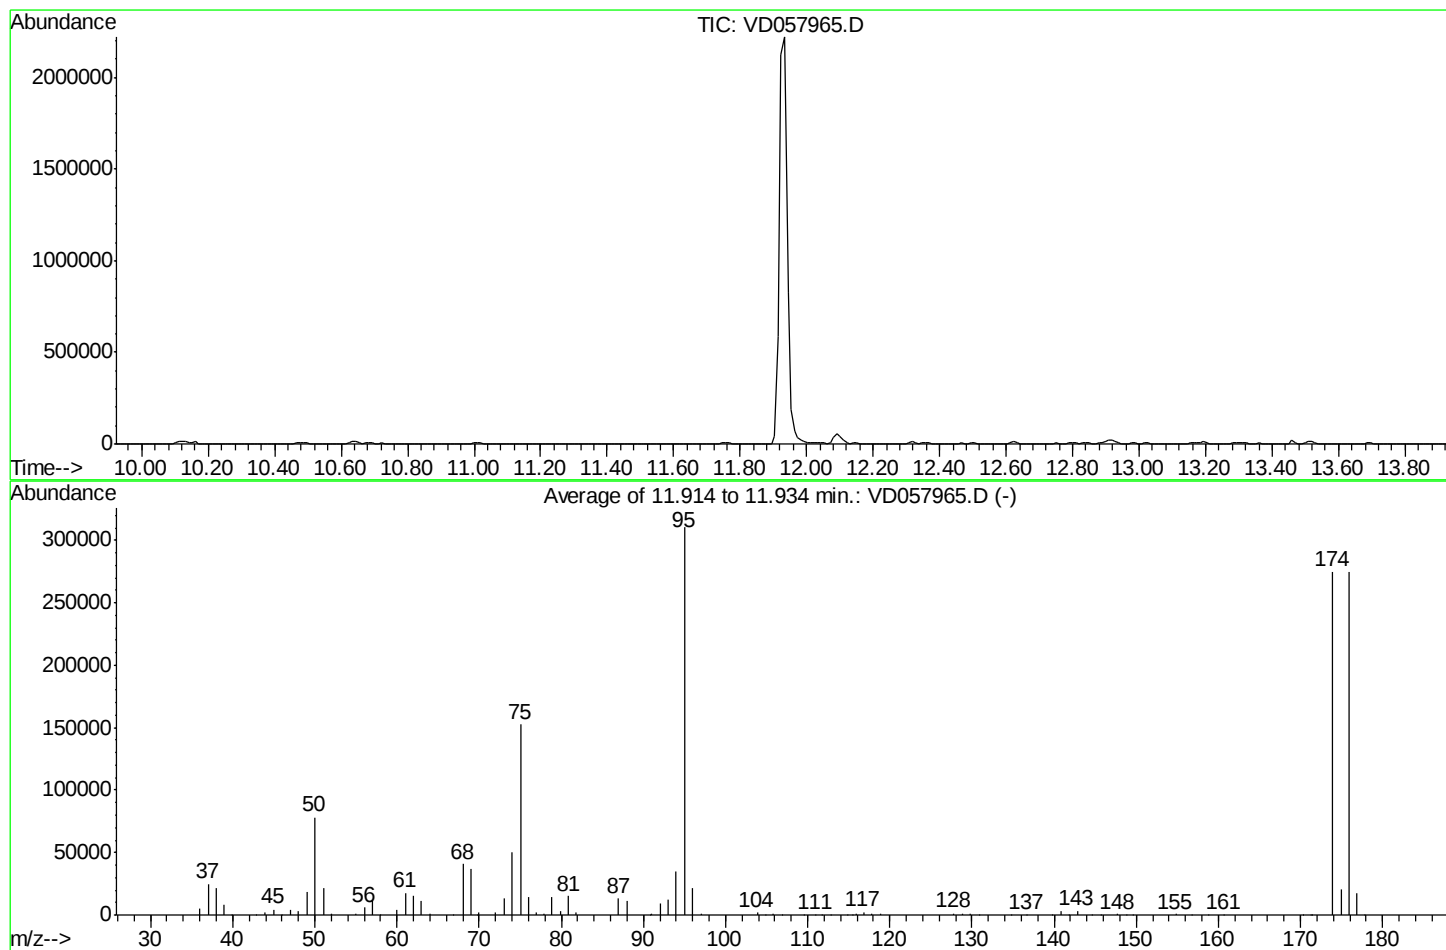

AutoFind: Scans 1187, 1188, 1189; Background Corrected with Scan 1183

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 25.3      | 78477   | PASS             |
| 75          | 95           | 30           | 60           | 49.1      | 152616  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 310528  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 21382   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 88.6      | 275229  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 20761   | PASS             |
| 176         | 174          | 95           | 101          | 99.7      | 274418  | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 17961   | PASS             |