


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD060718\
Data File : VD057987.D
Acq On : 7 Jun 2018 23:24
Operator : JC/SY
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
Title : SW846 8260
Last Update : Thu Jun 07 08:57:33 2018

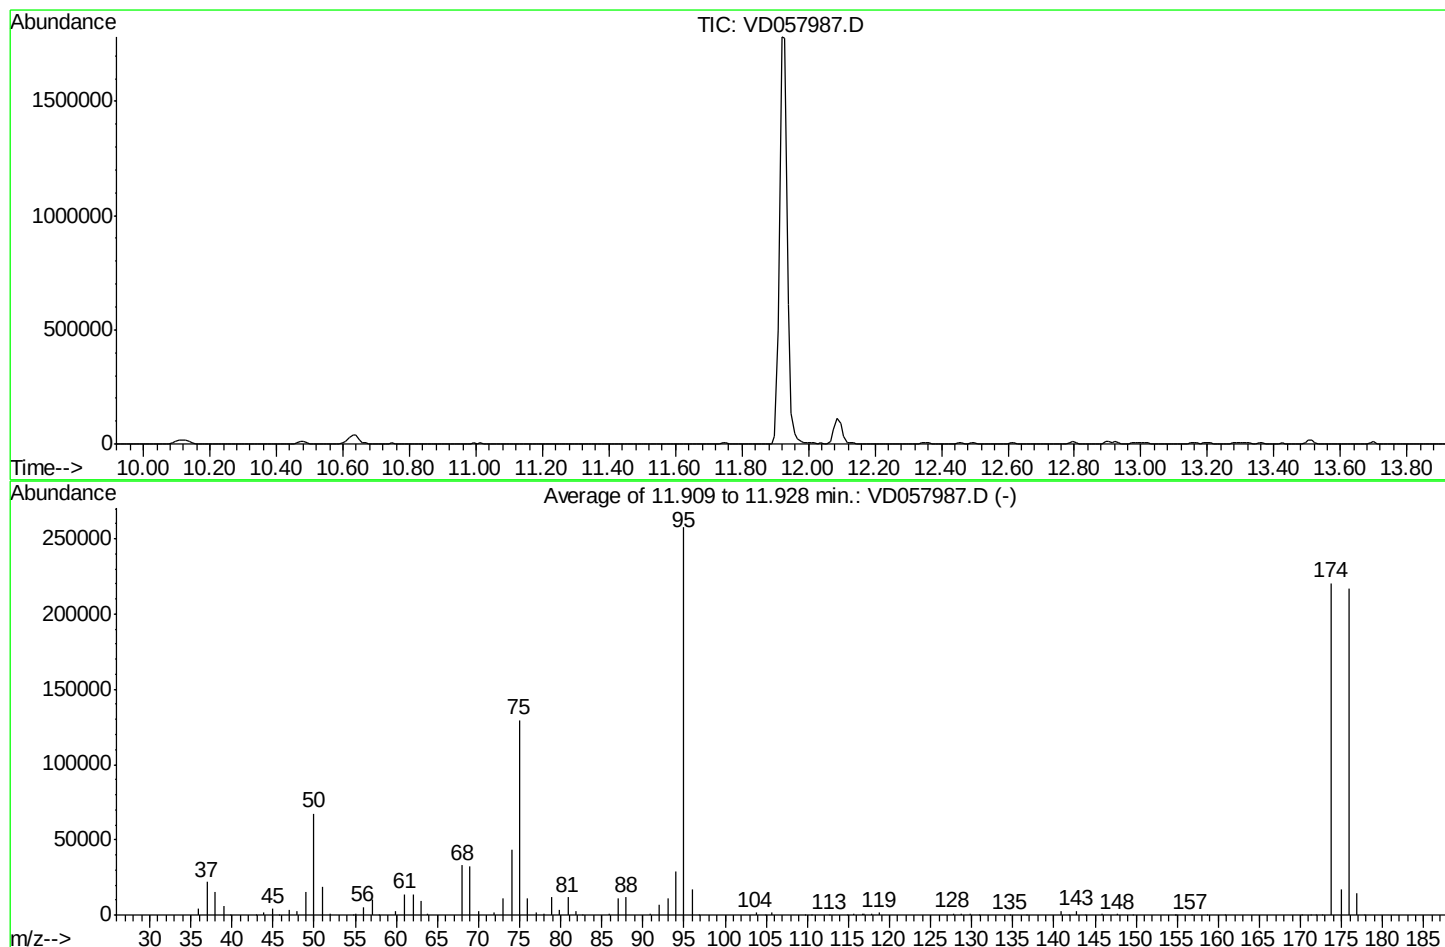

AutoFind: Scans 1187, 1188, 1189; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	67666	PASS
75	95	30	60	50.2	129432	PASS
95	95	100	100	100.0	257706	PASS
96	95	5	9	6.6	17068	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.6	220621	PASS
175	174	5	9	7.6	16766	PASS
176	174	95	101	98.3	216813	PASS
177	176	5	9	6.6	14370	PASS