



Methylene Chloride

Response Ratio

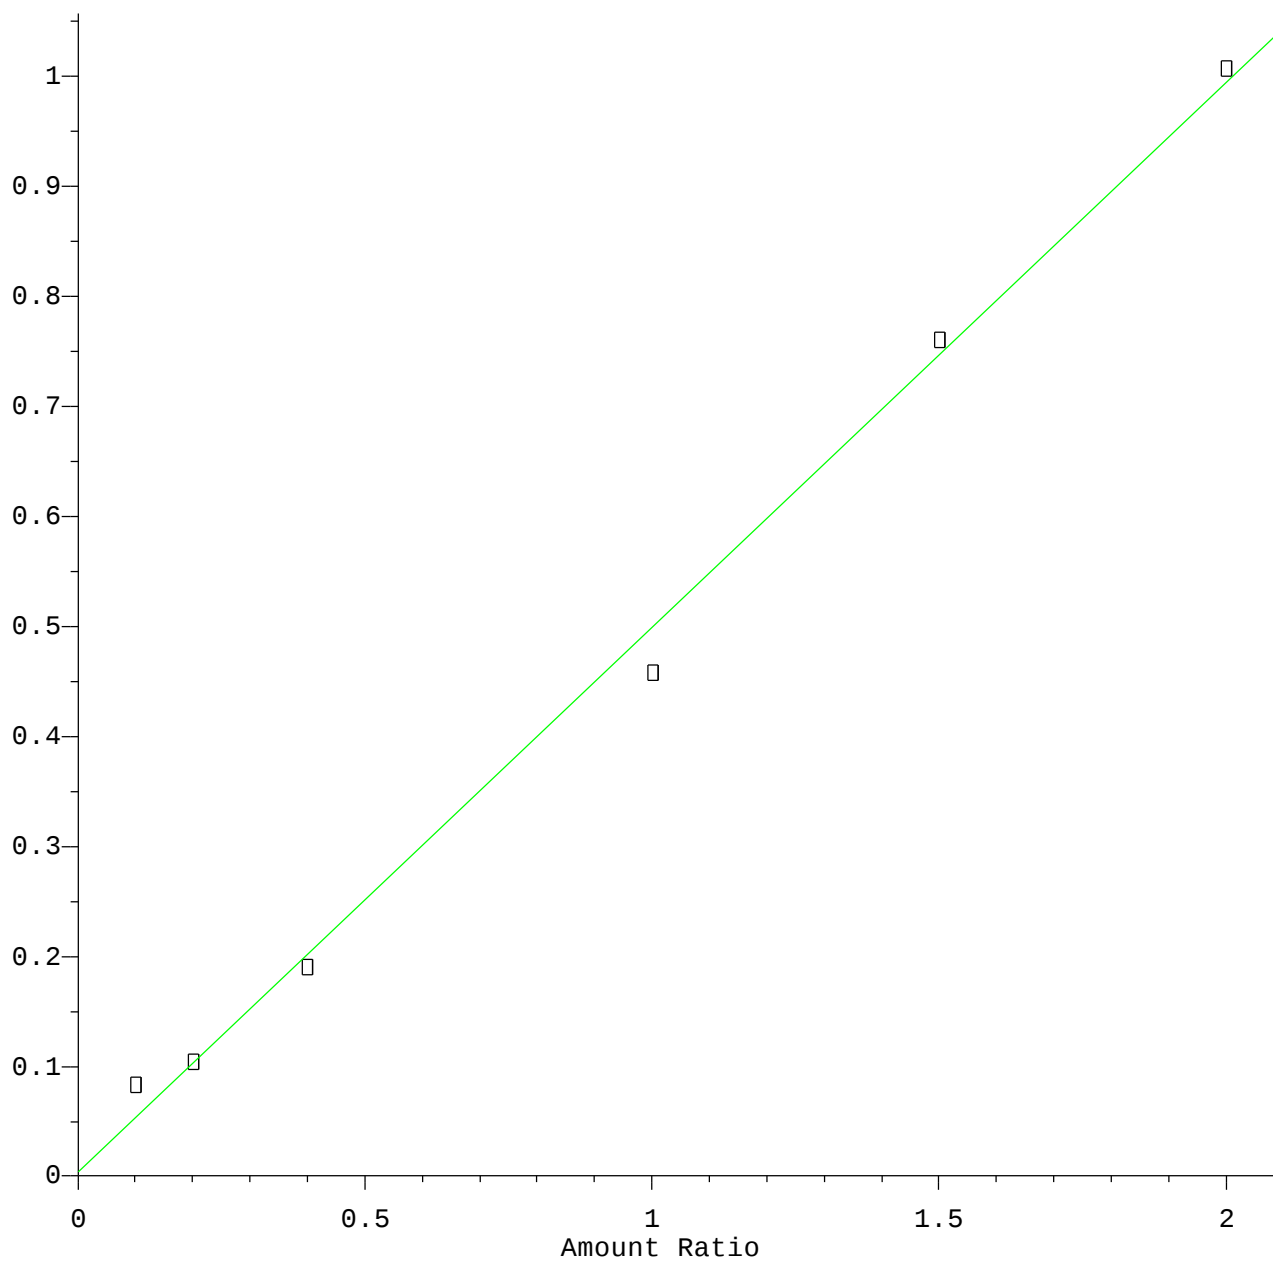


Resp Ratio = $4.95 \times 10^{-1} \times \text{Amt} + 4.41 \times 10^{-3}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

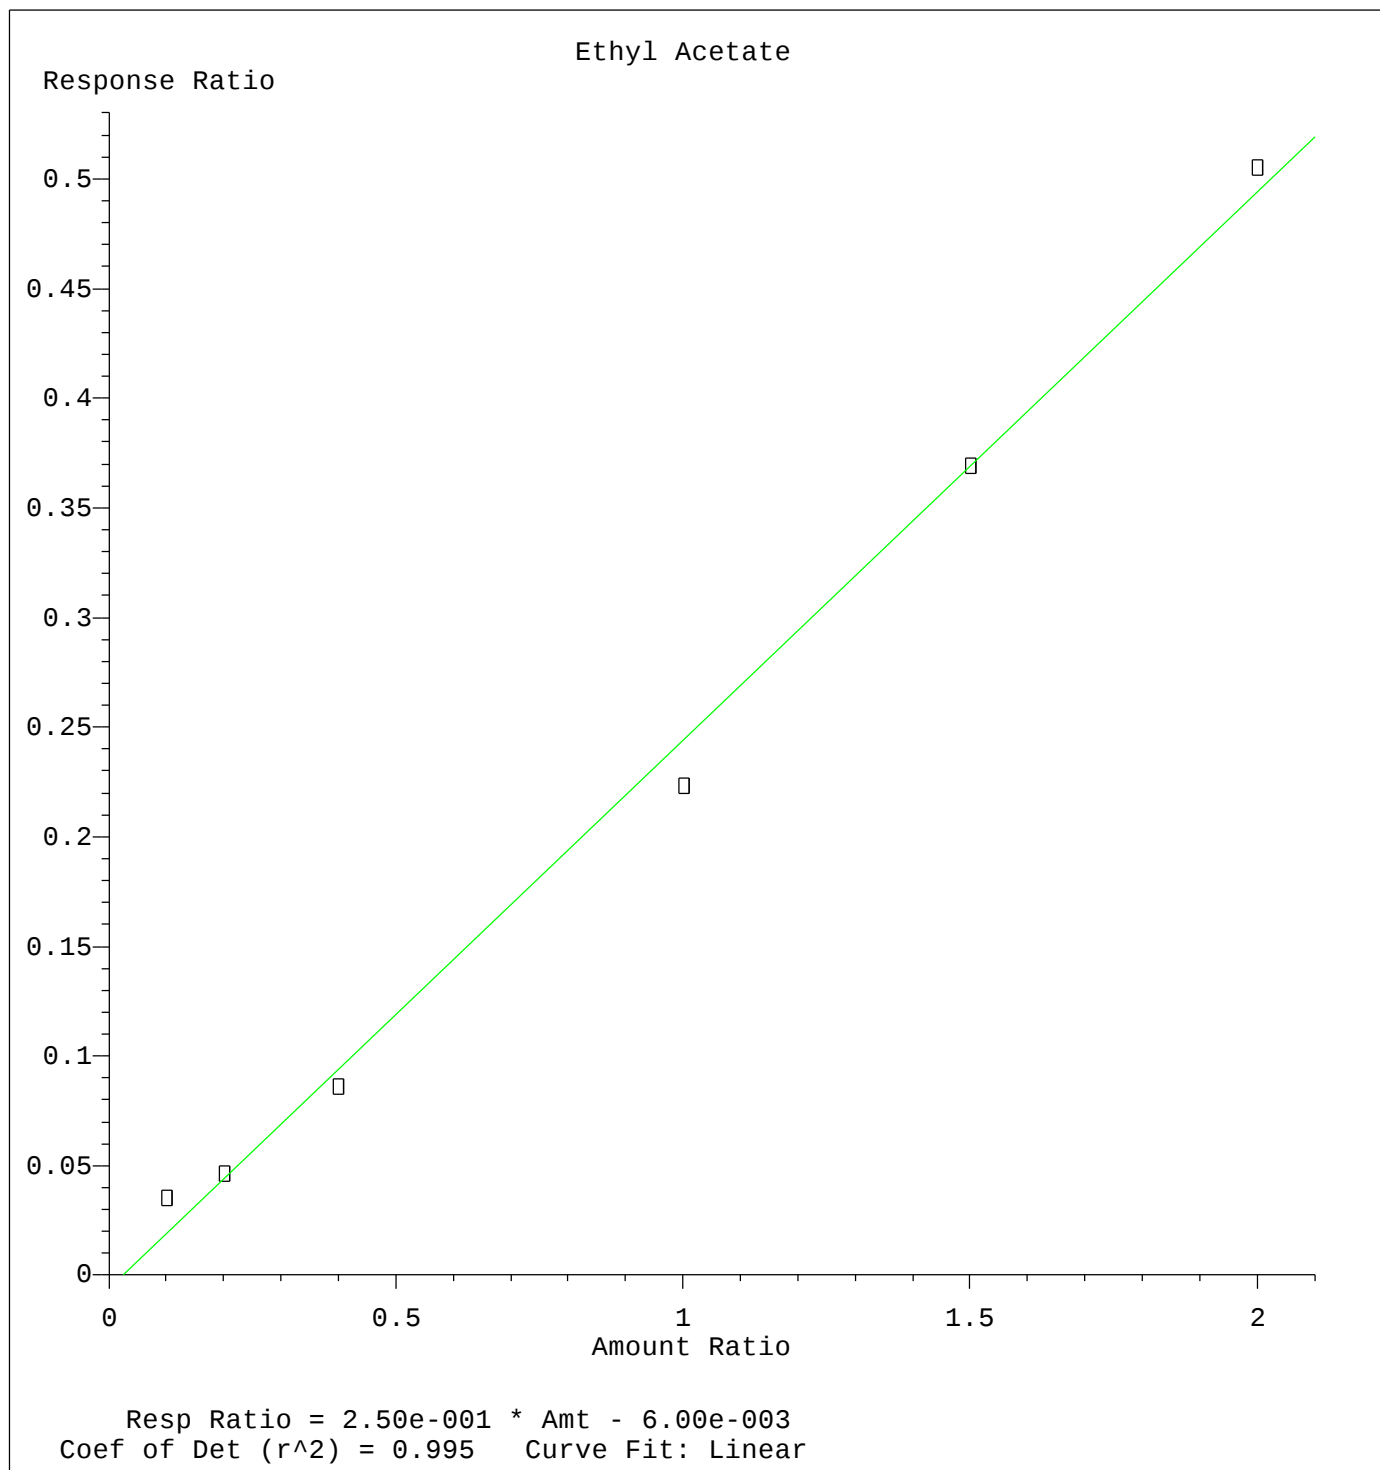


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

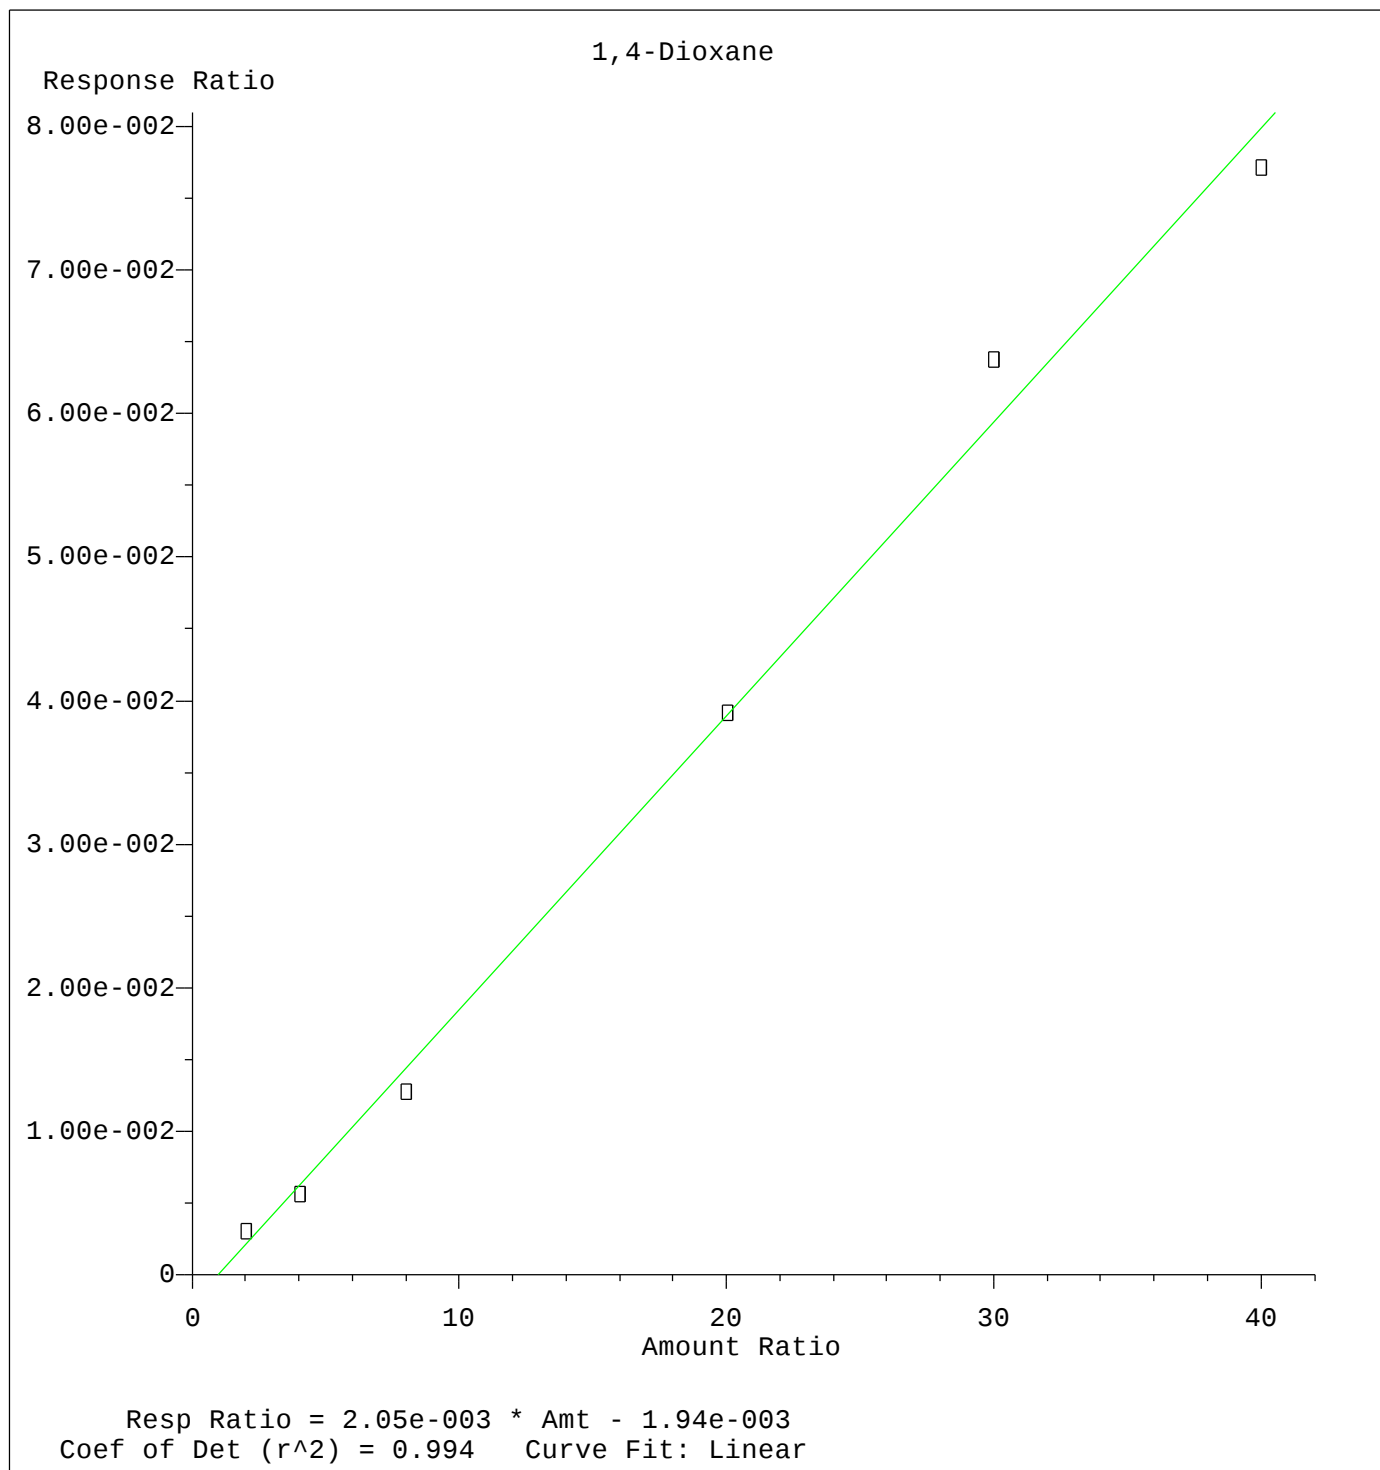

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

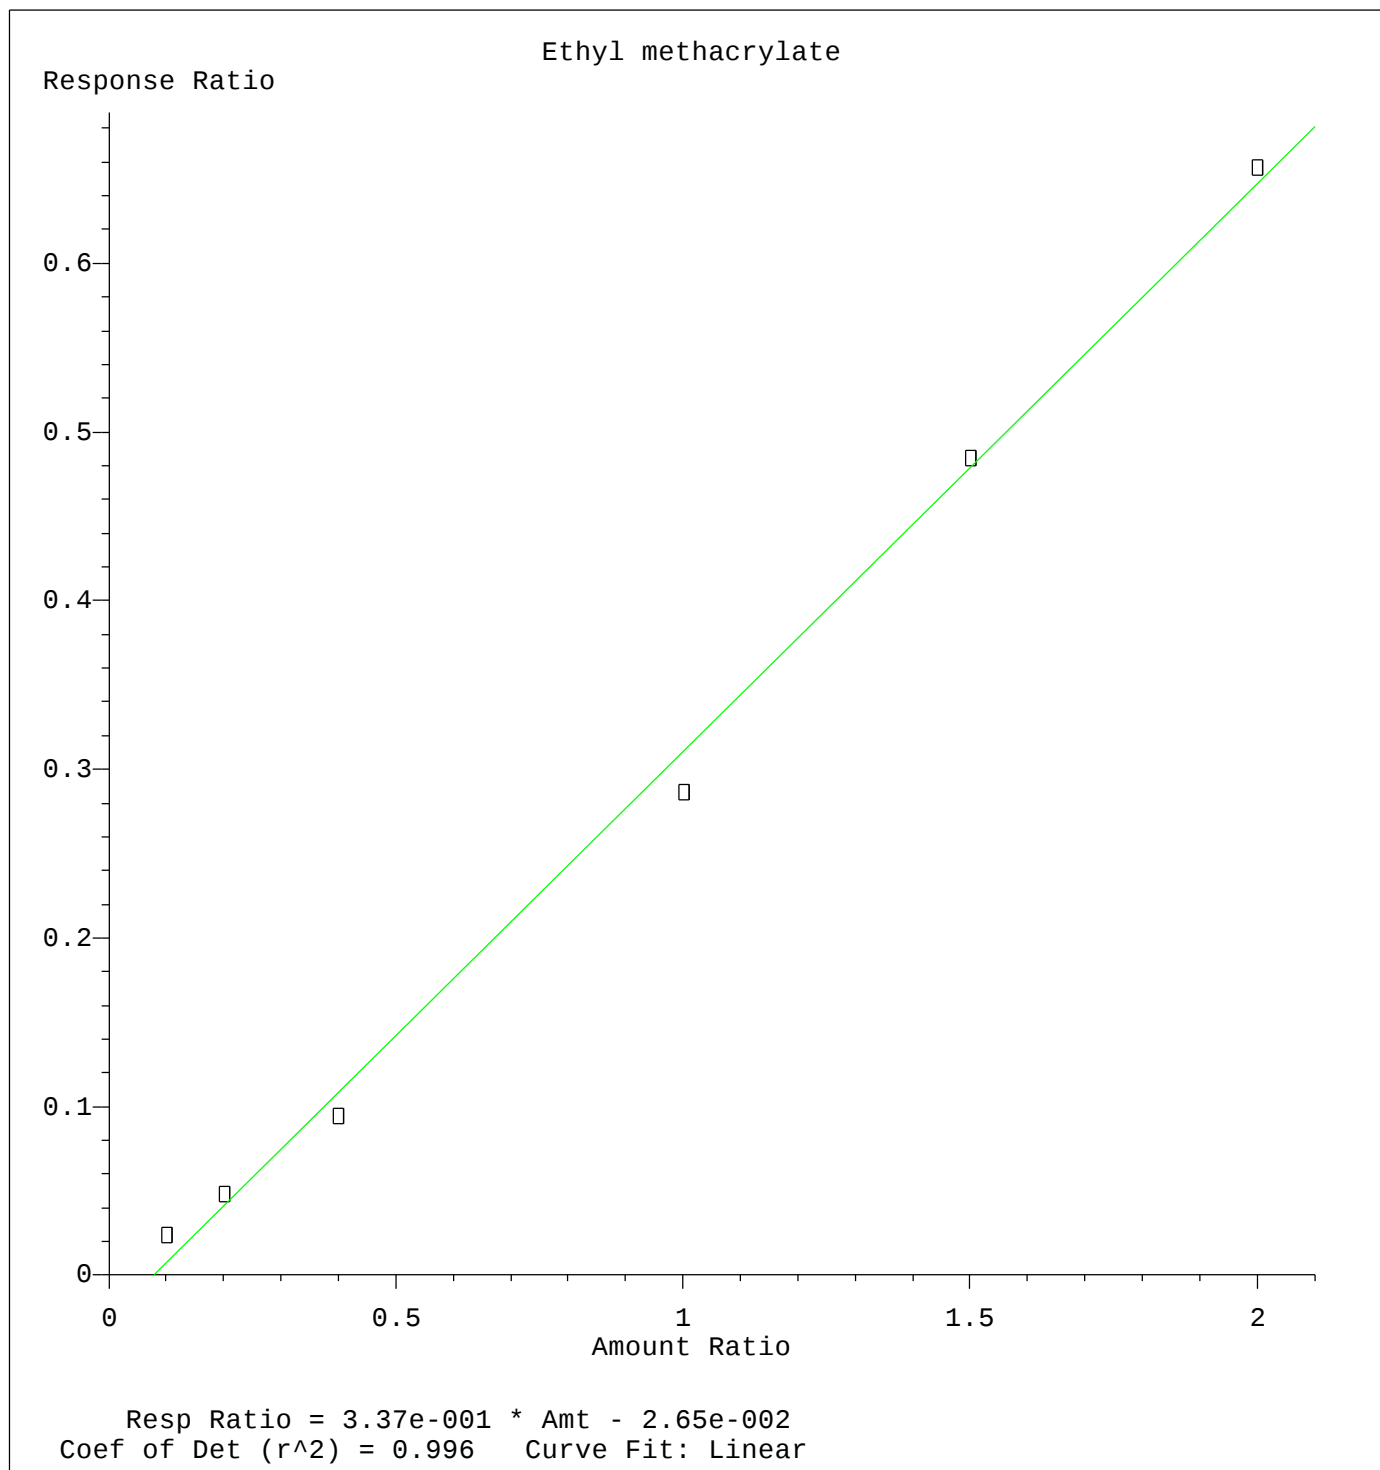


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

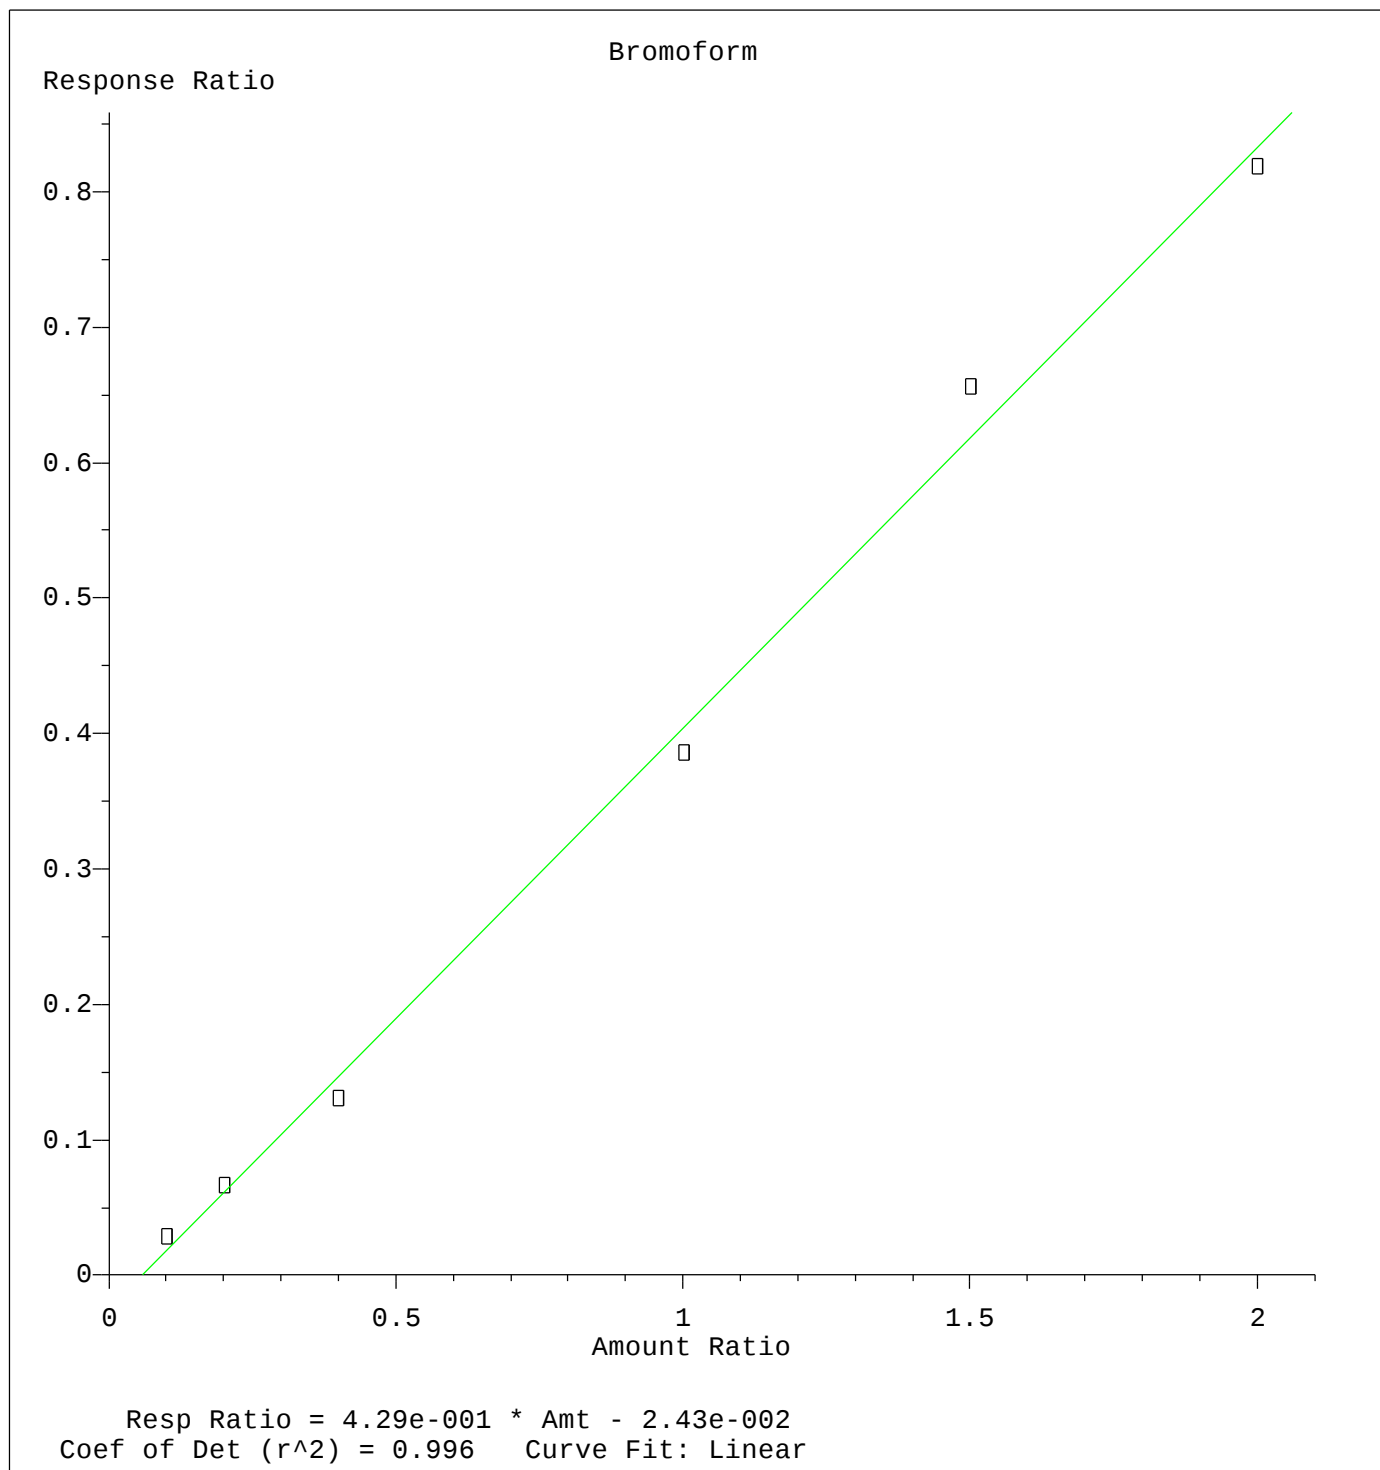

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

trans-1,4-Dichloro-2-butene

Response Ratio

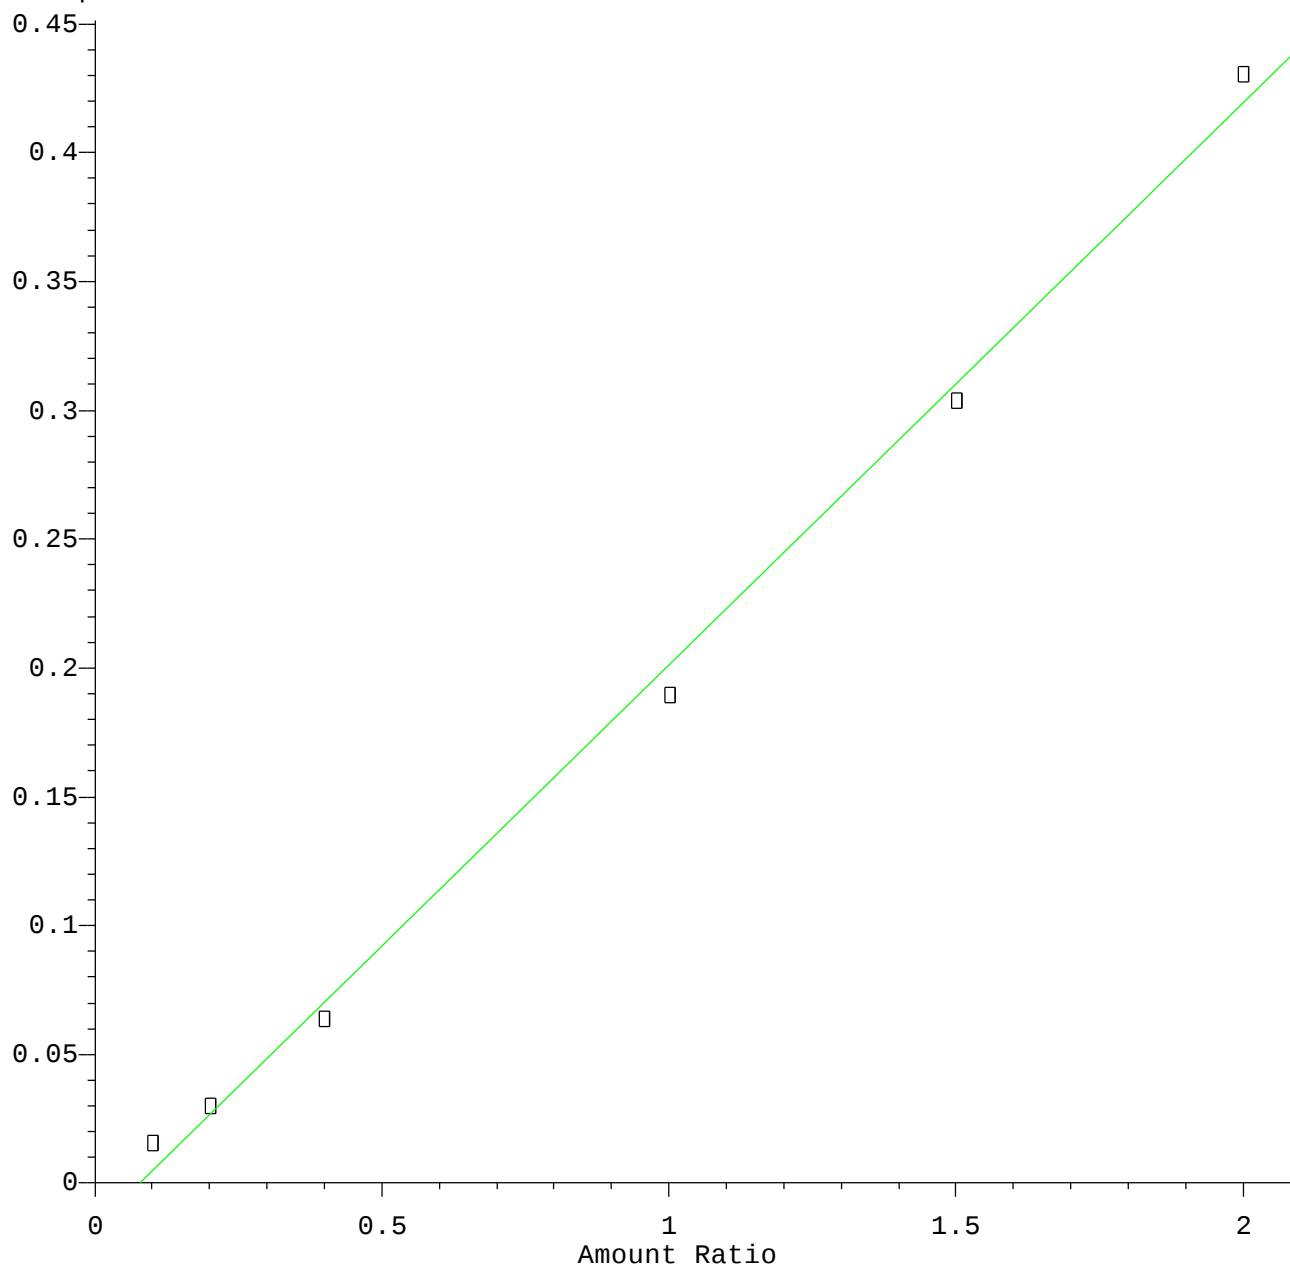


Resp Ratio = $2.18 \times 10^{-1} \times \text{Amt} - 1.70 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019


1,2,4-Trichlorobenzene

Response Ratio

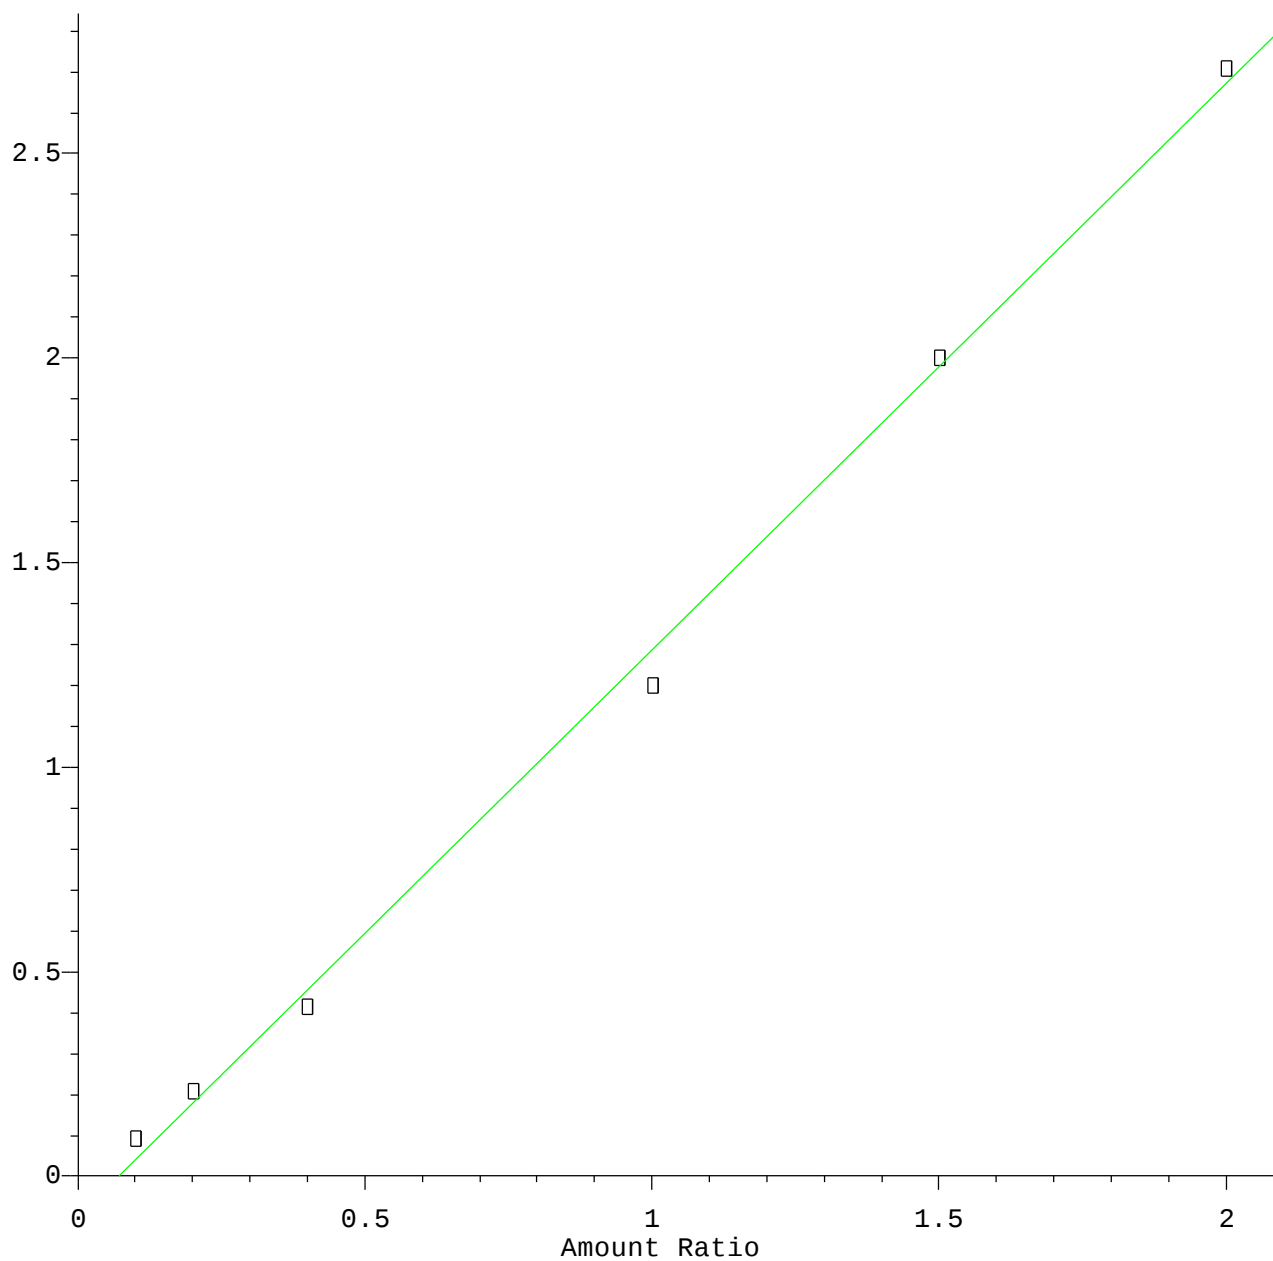


Resp Ratio = 1.39e+000 * Amt - 9.89e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

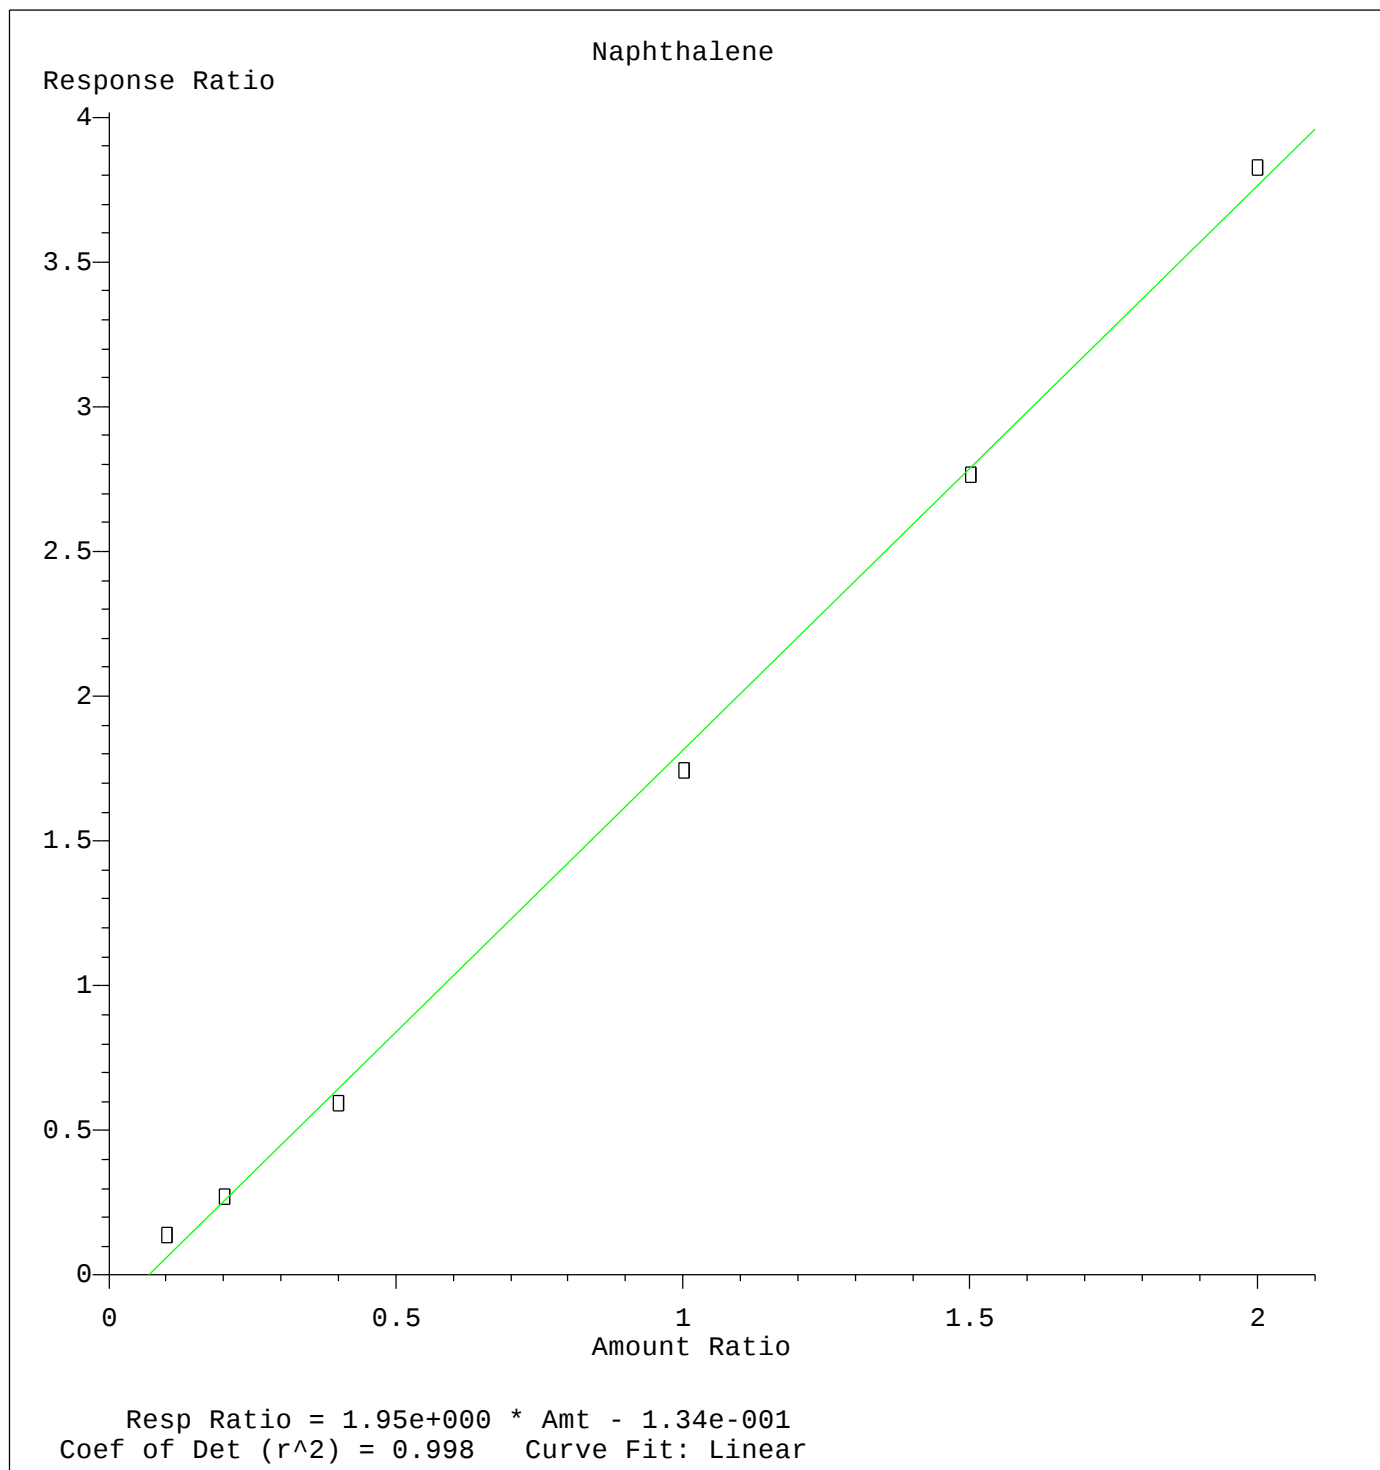

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

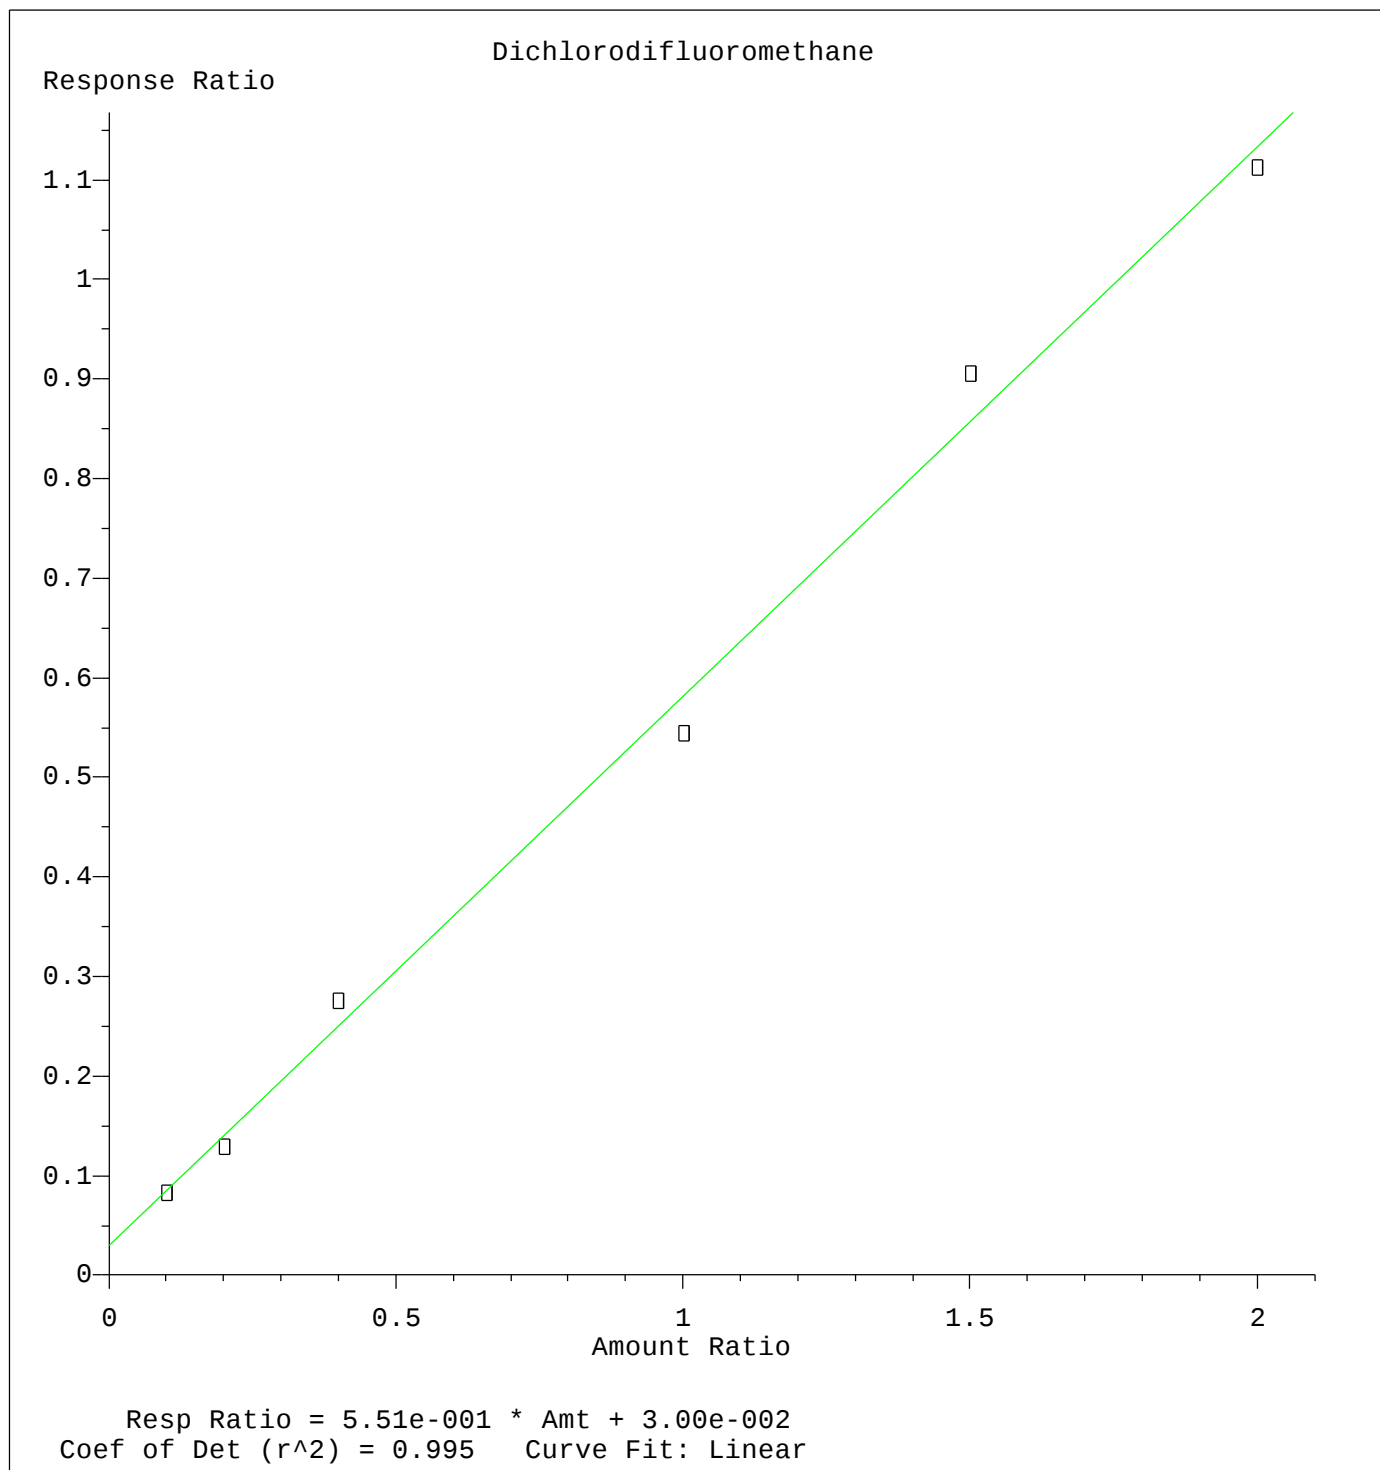

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019

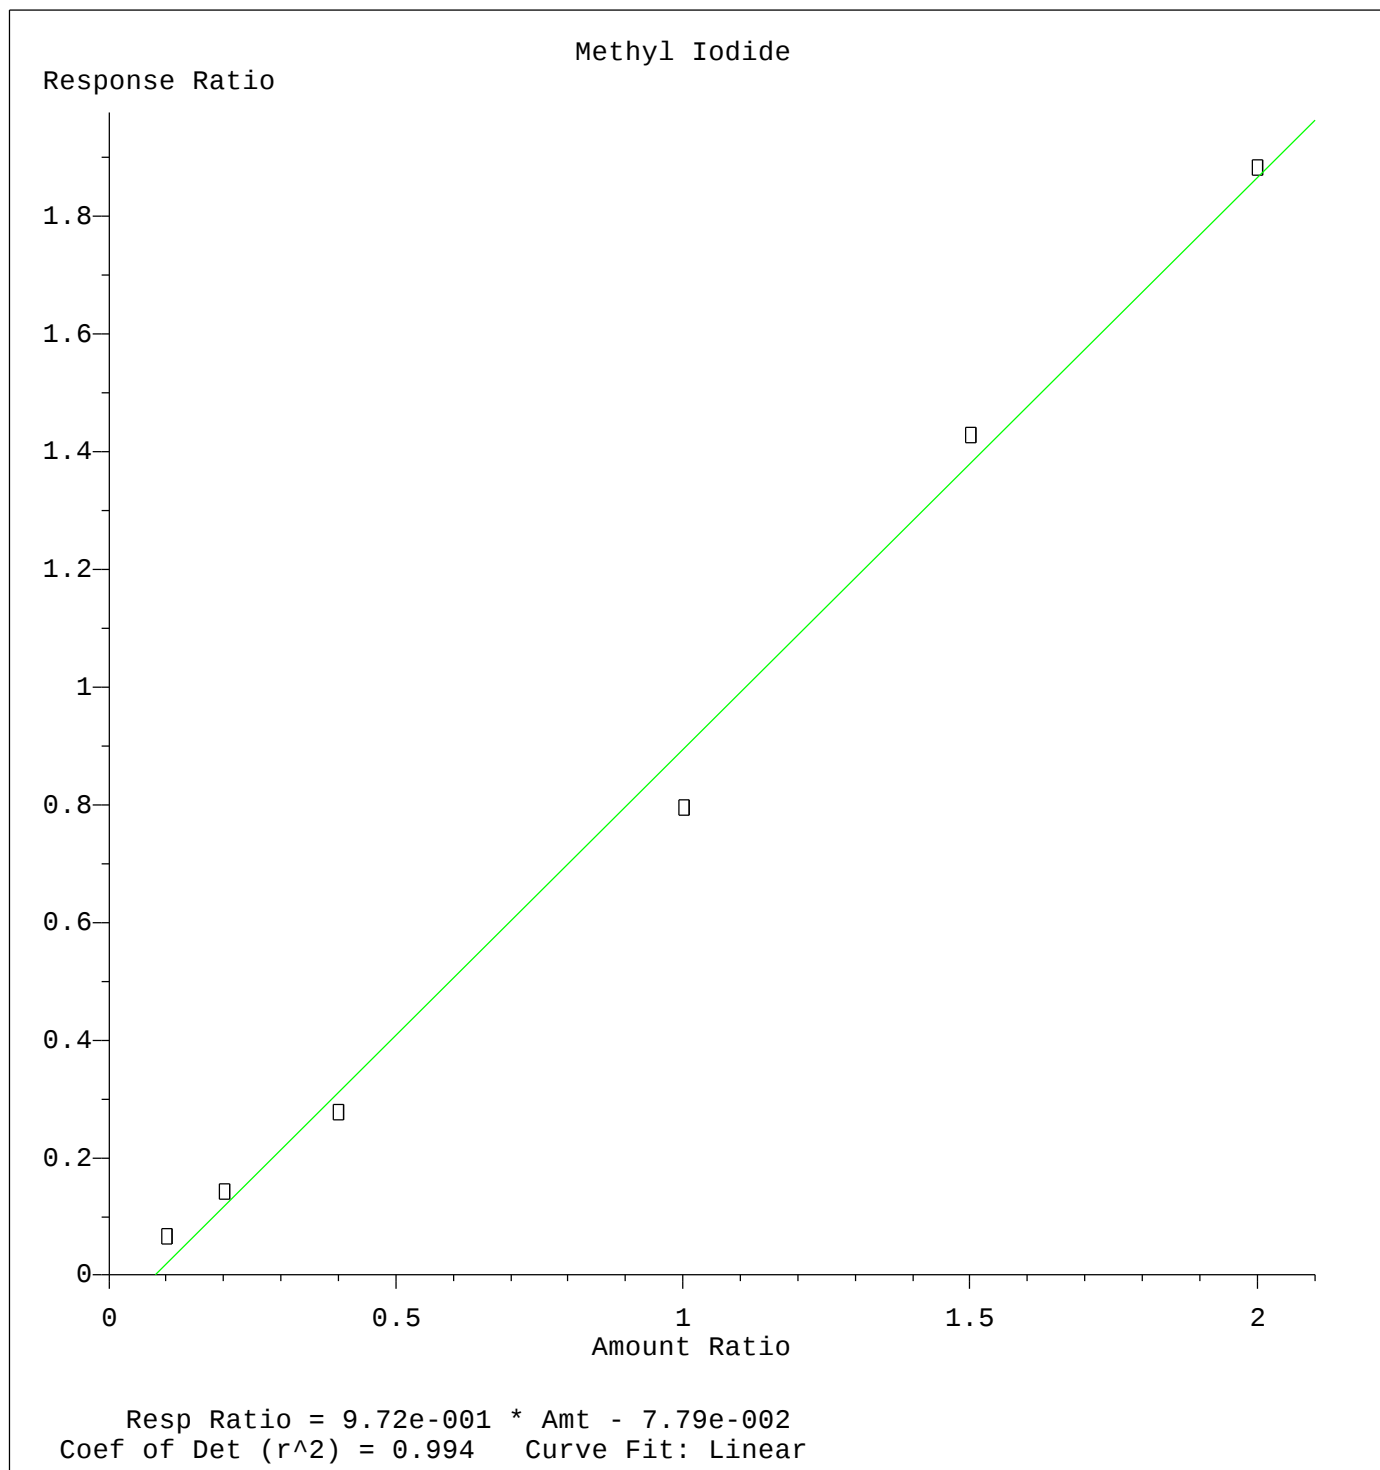

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Calibration Table Last Updated: Sat Jun 08 00:02:21 2019