


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD060719\
Data File : VD062634.D
Acq On : 7 Jun 2019 9:48
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Title : SW846 8260
Last Update : Sat Jun 08 00:02:21 2019

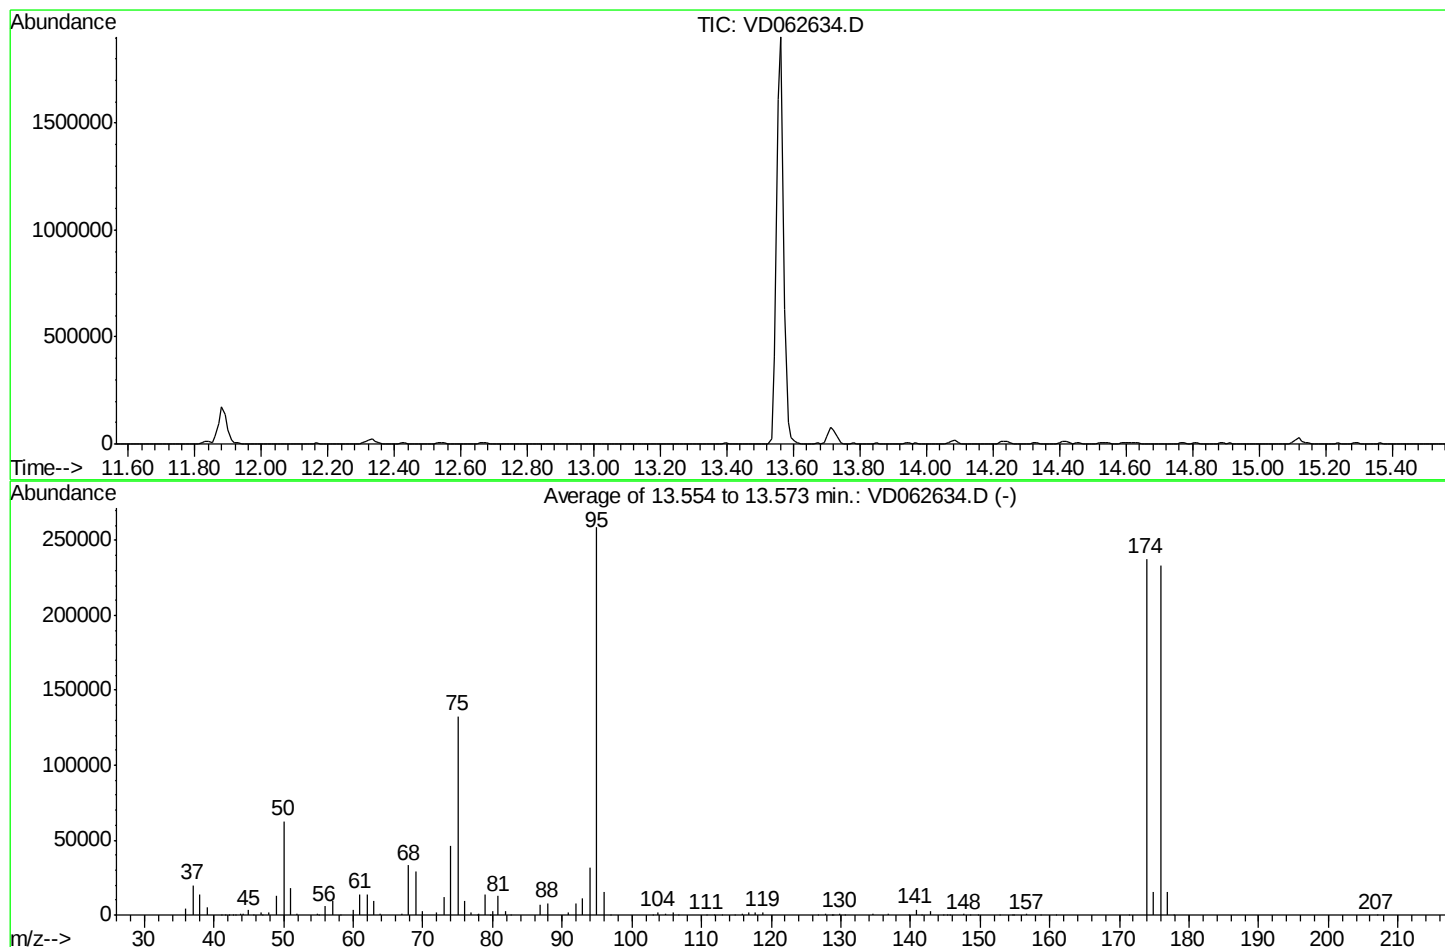

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	62482	PASS
75	95	30	60	51.3	132752	PASS
95	95	100	100	100.0	258760	PASS
96	95	5	9	5.9	15250	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.0	237952	PASS
175	174	5	9	6.6	15592	PASS
176	174	95	101	98.1	233429	PASS
177	176	5	9	6.7	15622	PASS