
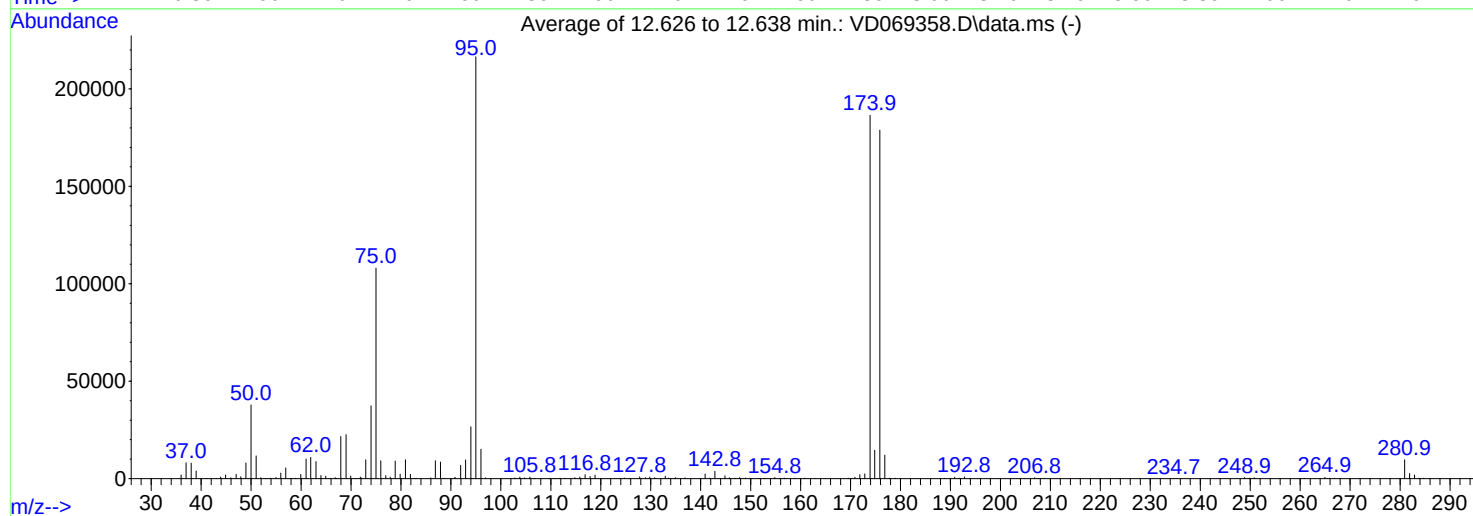


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060721\
 Data File : VD069358.D
 Acq On : 07 Jun 2021 10:11
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D0601215.M
 Title : SW846 8260
 Last Update : Wed Jun 02 02:17:36 2021

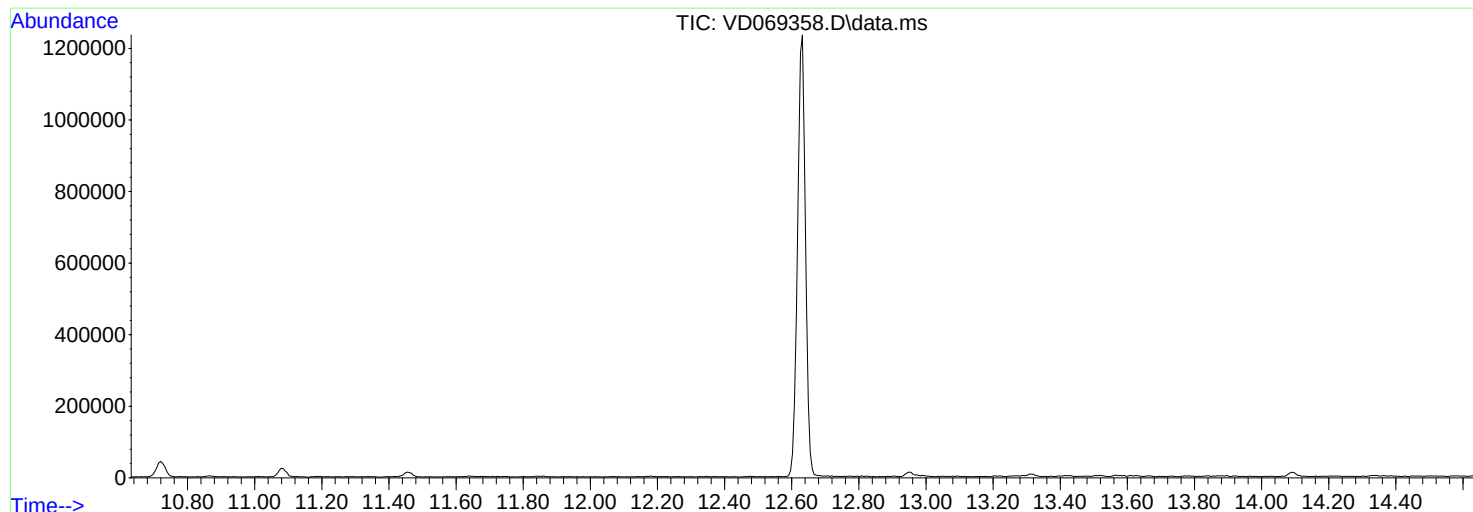

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	37837	PASS
75	95	30	60	49.9	108096	PASS
95	95	100	100	100.0	216469	PASS
96	95	5	9	7.0	15124	PASS
173	174	0.00	2	1.3	2489	PASS
174	95	50	100	86.2	186496	PASS
175	174	5	9	7.8	14517	PASS
176	174	95	101	95.9	178880	PASS
177	176	5	9	6.8	12099	PASS