

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD060818\
 Data File : VD058029.D
 Acq On : 8 Jun 2018 20:31
 Operator : VA/AP
 Sample : J3360-02
 Misc : 6.25g/5ml/MSVOA D/SOIL
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Jun 08 23:57:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 07 08:57:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-5.65
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-6.70
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-10.69
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-12.91

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue



(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD060818\
Data File : VD058029.D
Acq On : 8 Jun 2018 20:31
Operator : VA/AP
Sample : J3360-02
Misc : 6.25g/5ml/MSVOA D/SOIL
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Jun 08 23:57:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 07 08:57:33 2018
Response via : Initial Calibration

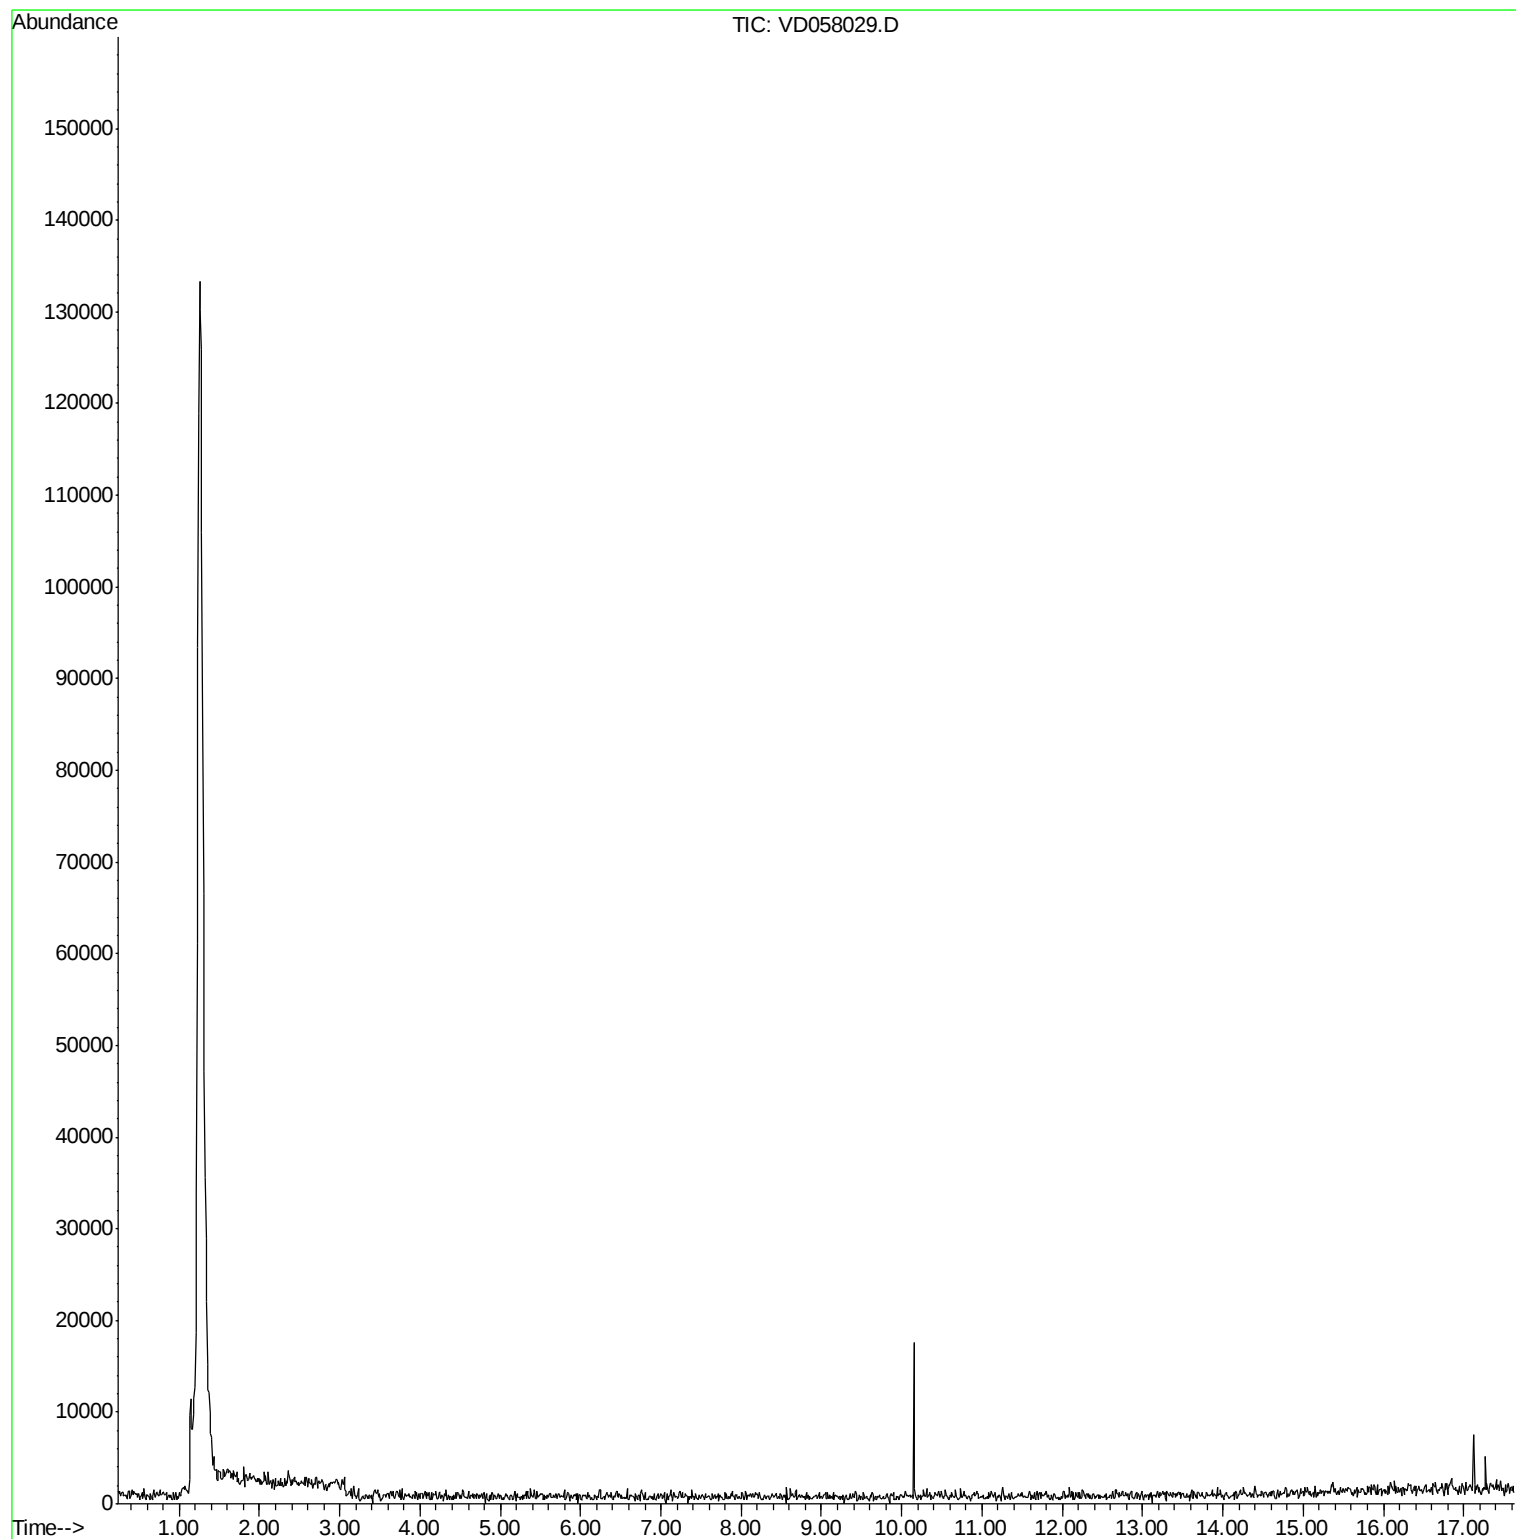

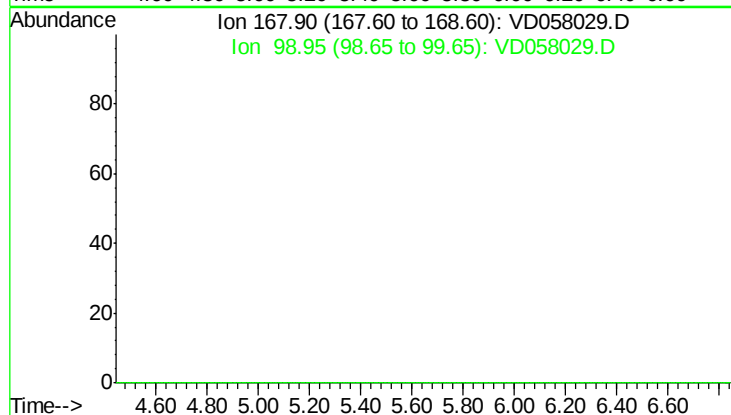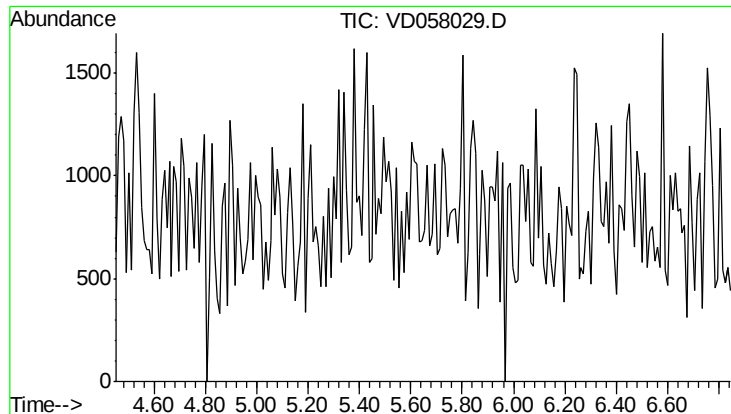

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 5.65 min

Lab File: VD058029.D

Acq: 8 Jun 2018 20:31

Tot Ion: 168

Sig Exp Ratio



168 100

99 58.5

Instrument :

MSVOA_D

ClientSampleId :

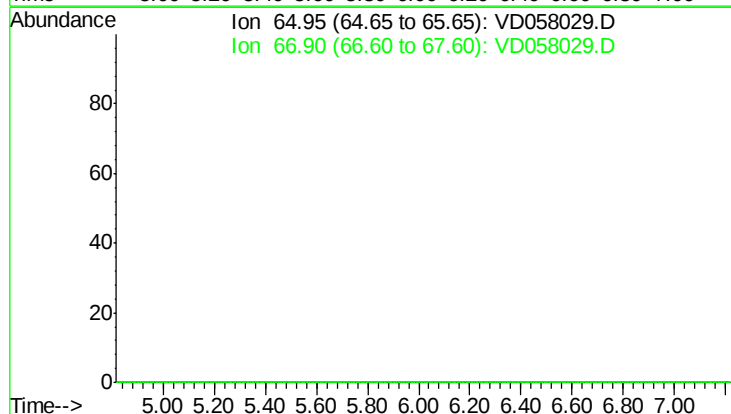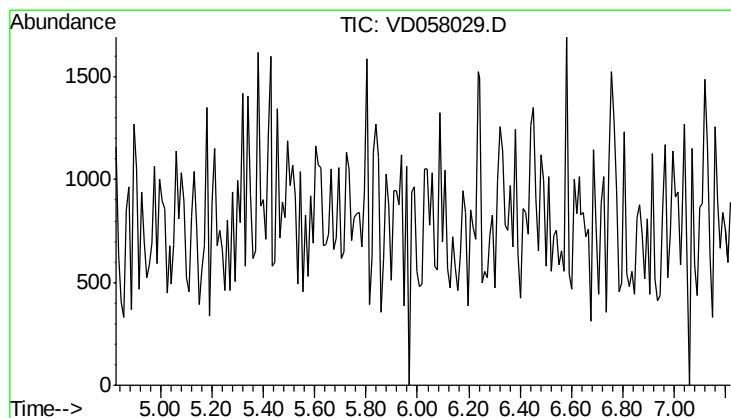

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

Expected RT: 6.02 min

Lab File: VD058029.D


Acq: 8 Jun 2018 20:31

Tgt Ion: 65

Sig Exp Ratio

65 100



67 47.0

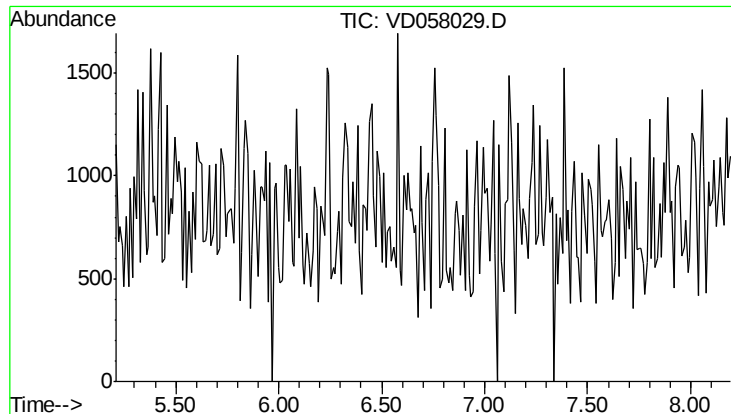

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 6.70 min
 Lab File: VD058029.D
 Acq: 8 Jun 2018 20:31


Instrument :
 MSVOA_D
 ClientSampleId :


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.4
88	18.9

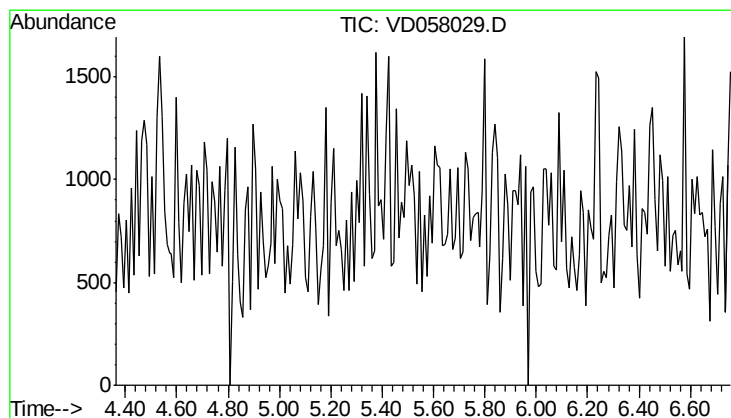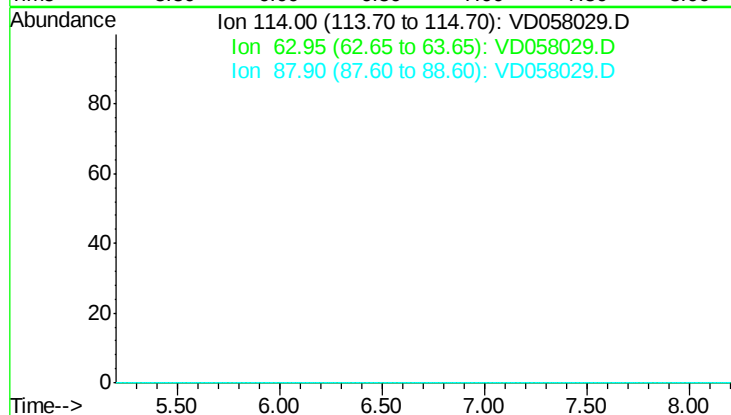

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 5.56 min
 Lab File: VD058029.D
 Acq: 8 Jun 2018 20:31

Tgt Ion	113
Sig	Exp Ratio
113	100
111	101.9
192	20.5

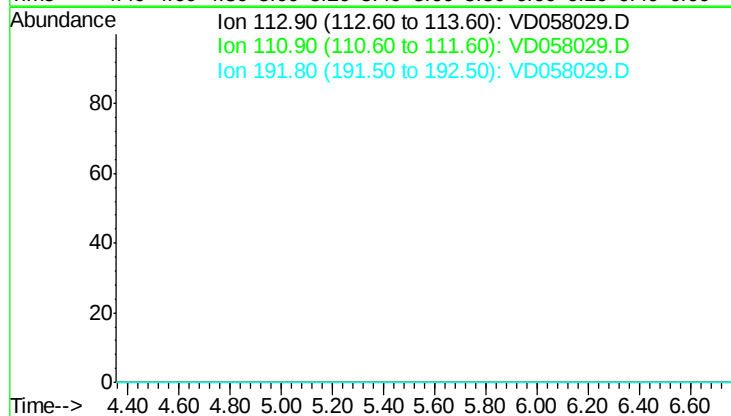


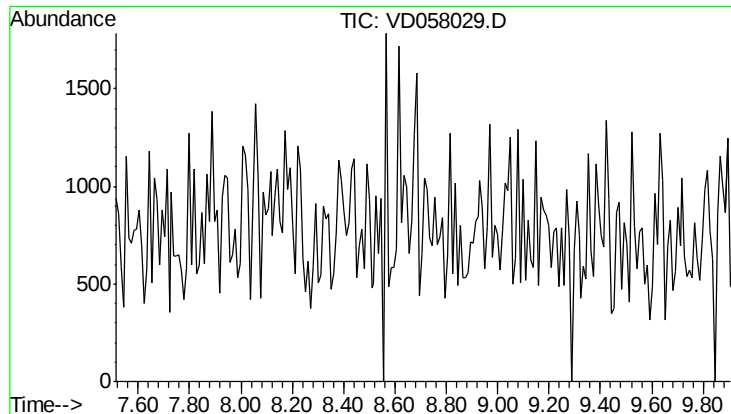


#50
Toluene-d8
Concen: N.D. ug/l
Expected RT: 8.71 min

Lab File: VD058029.D
Acq: 8 Jun 2018 20:31

Instrument :
MSVOA_D
ClientSampleId :


Tot Ion: 98
Sig Exp Ratio
98 100
100 66.7

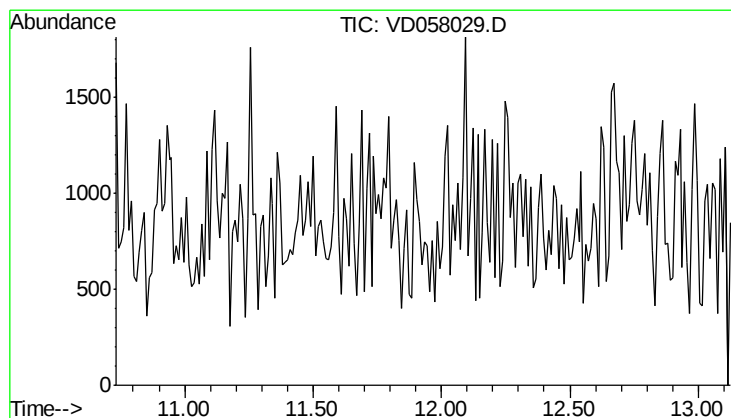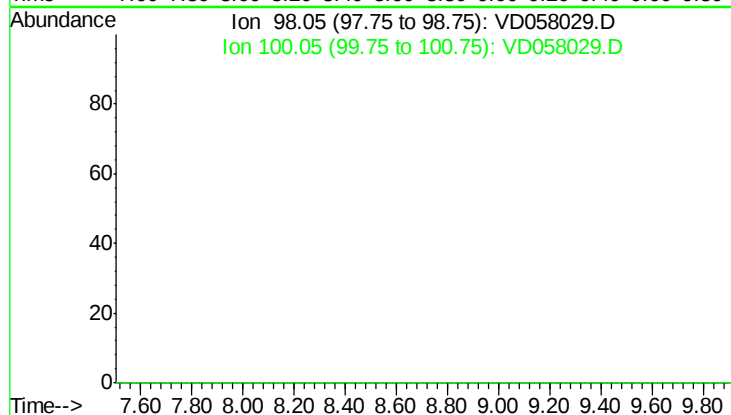


#62
4-Bromofluorobenzene
Concen: N.D. ug/l
Expected RT: 11.93 min

Lab File: VD058029.D
Acq: 8 Jun 2018 20:31

Tgt Ion: 95
Sig Exp Ratio
95 100
174 84.7
176 81.3


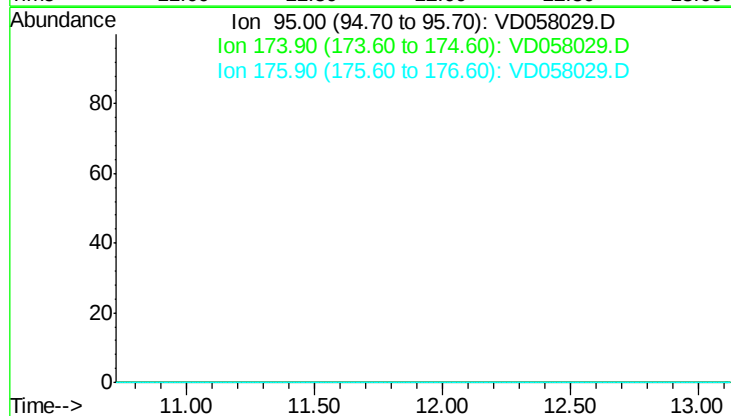


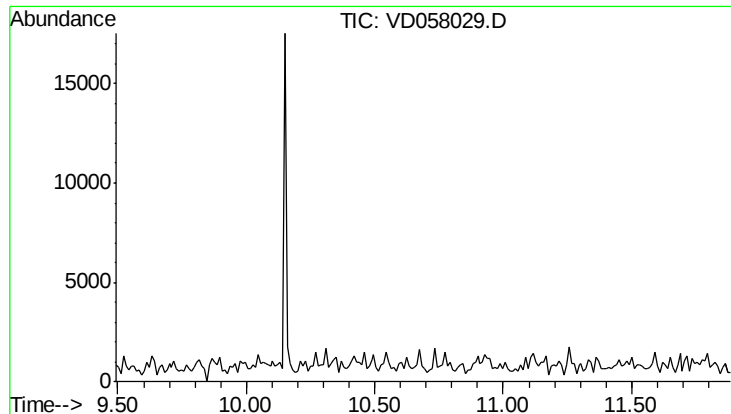

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 10.69 min
 Lab File: VD058029.D
 Acq: 8 Jun 2018 20:31

Instrument :
 MSVOA_D
 ClientSampleId :

Tot Ion	117
Sig	Exp Ratio
117	100
82	58.5
119	32.2

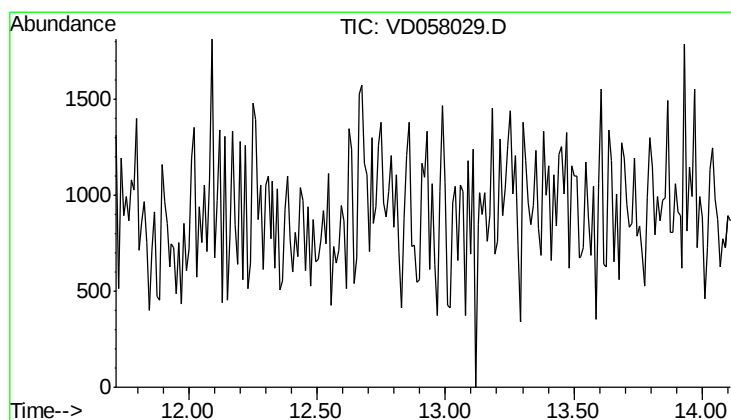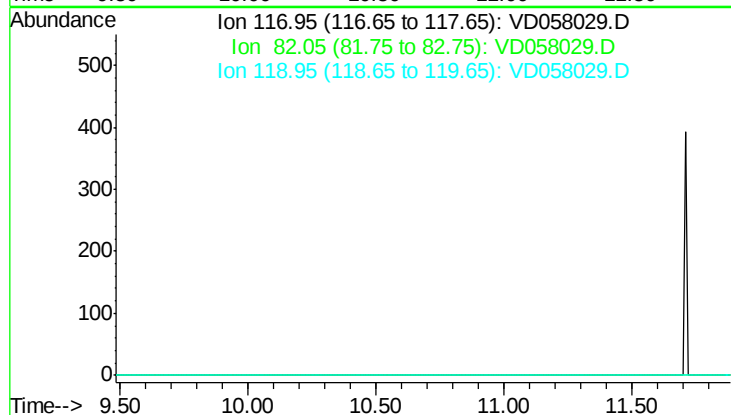

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.91 min
 Lab File: VD058029.D
 Acq: 8 Jun 2018 20:31

Tgt Ion	152
Sig	Exp Ratio
152	100
115	51.1
150	153.4

