


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD060818\
Data File : VD058010.D
Acq On : 8 Jun 2018 11:10
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
Title : SW846 8260
Last Update : Thu Jun 07 08:57:33 2018

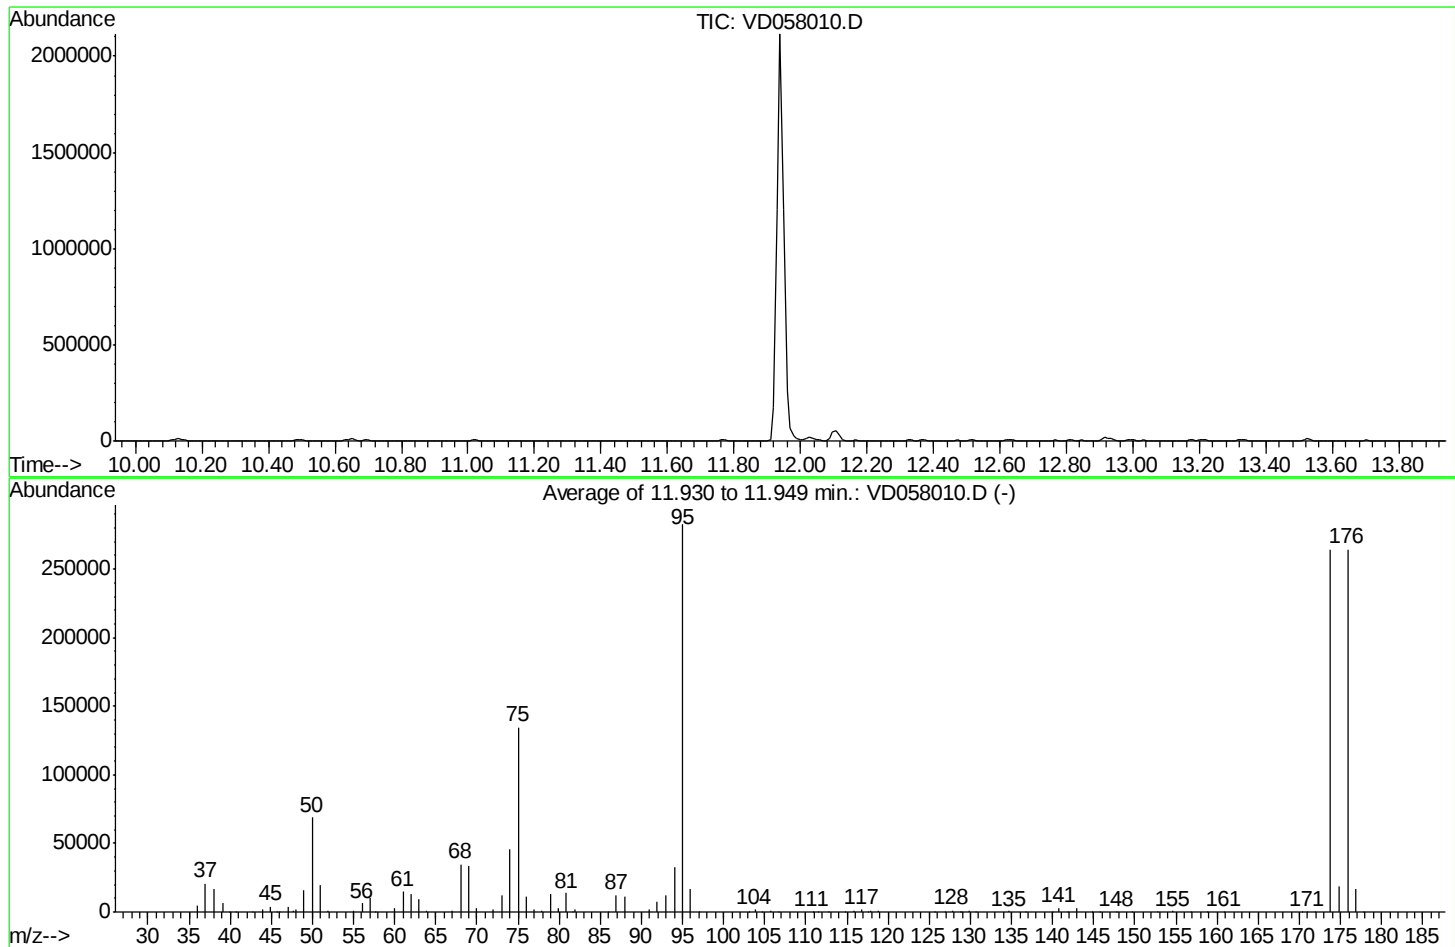

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	68845	PASS
75	95	30	60	47.7	134760	PASS
95	95	100	100	100.0	282666	PASS
96	95	5	9	6.1	17236	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.3	263722	PASS
175	174	5	9	7.1	18702	PASS
176	174	95	101	100.3	264448	PASS
177	176	5	9	6.4	16877	PASS