
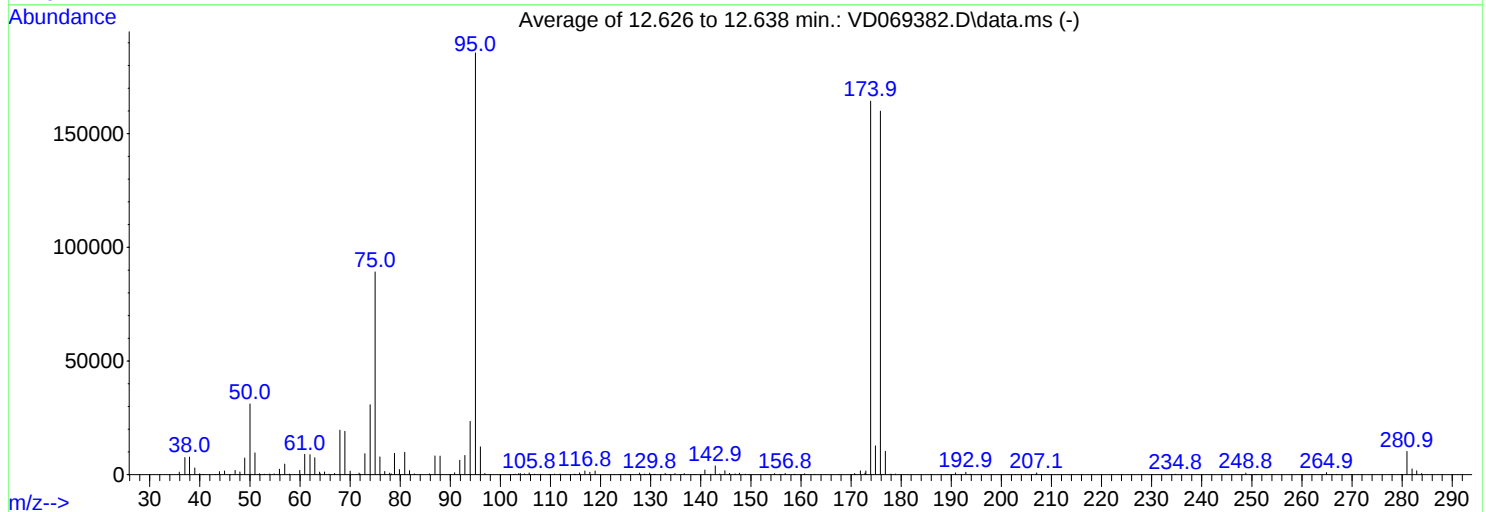


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060821\
 Data File : VD069382.D
 Acq On : 08 Jun 2021 09:12
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060121S.M
 Title : SW846 8260
 Last Update : Wed Jun 02 02:17:36 2021

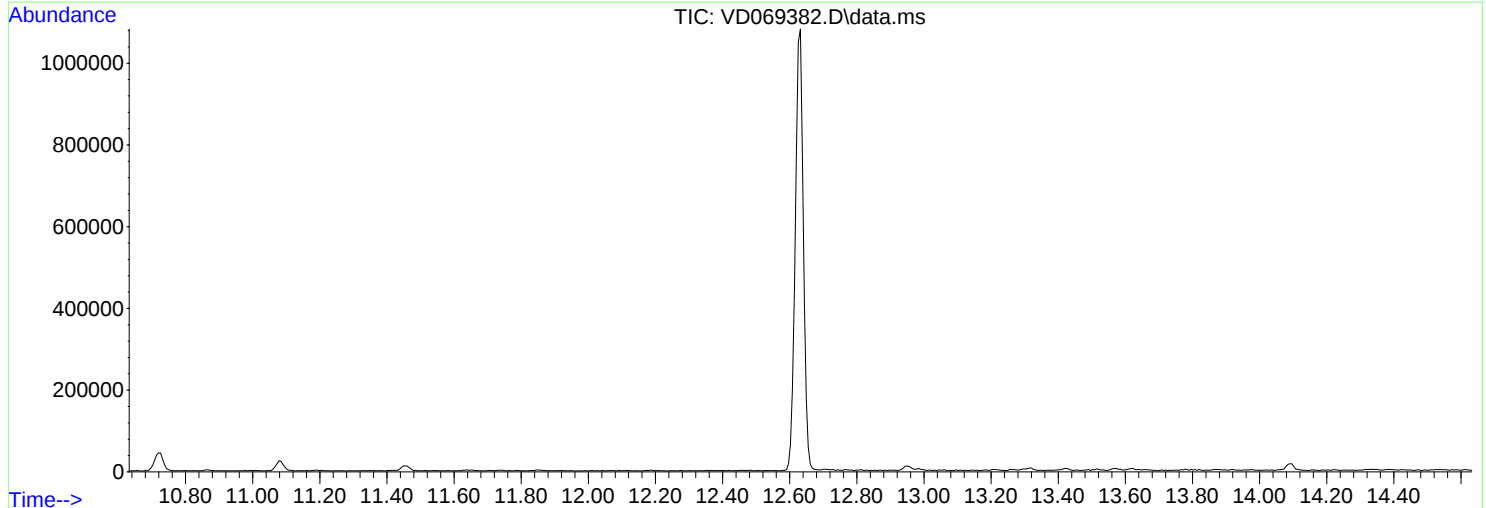

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	31141	PASS
75	95	30	60	48.0	89163	PASS
95	95	100	100	100.0	185579	PASS
96	95	5	9	6.6	12271	PASS
173	174	0.00	2	1.0	1608	PASS
174	95	50	100	88.5	164309	PASS
175	174	5	9	7.7	12641	PASS
176	174	95	101	97.3	159915	PASS
177	176	5	9	6.4	10285	PASS