
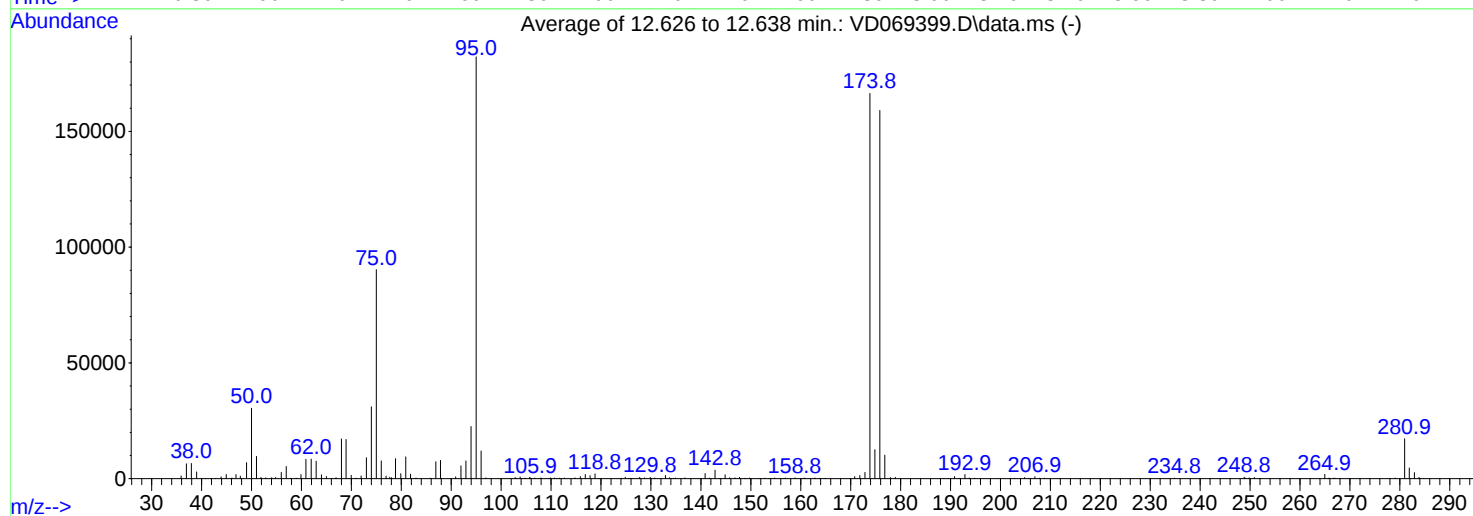


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060921\
 Data File : VD069399.D
 Acq On : 09 Jun 2021 11:07
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060121S.M
 Title : SW846 8260
 Last Update : Wed Jun 02 02:17:36 2021

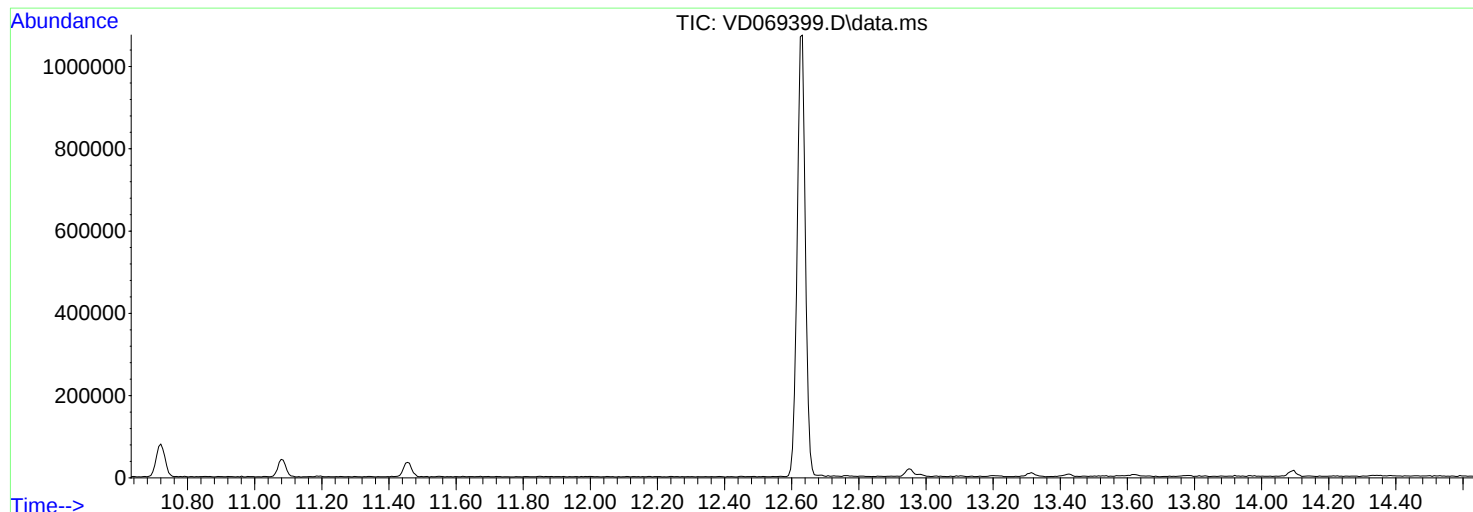

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	30408	PASS
75	95	30	60	49.5	90253	PASS
95	95	100	100	100.0	182208	PASS
96	95	5	9	6.6	11963	PASS
173	174	0.00	2	1.6	2674	PASS
174	95	50	100	91.4	166464	PASS
175	174	5	9	7.5	12497	PASS
176	174	95	101	95.5	159019	PASS
177	176	5	9	6.4	10187	PASS