


Methyl Iodide

Response Ratio

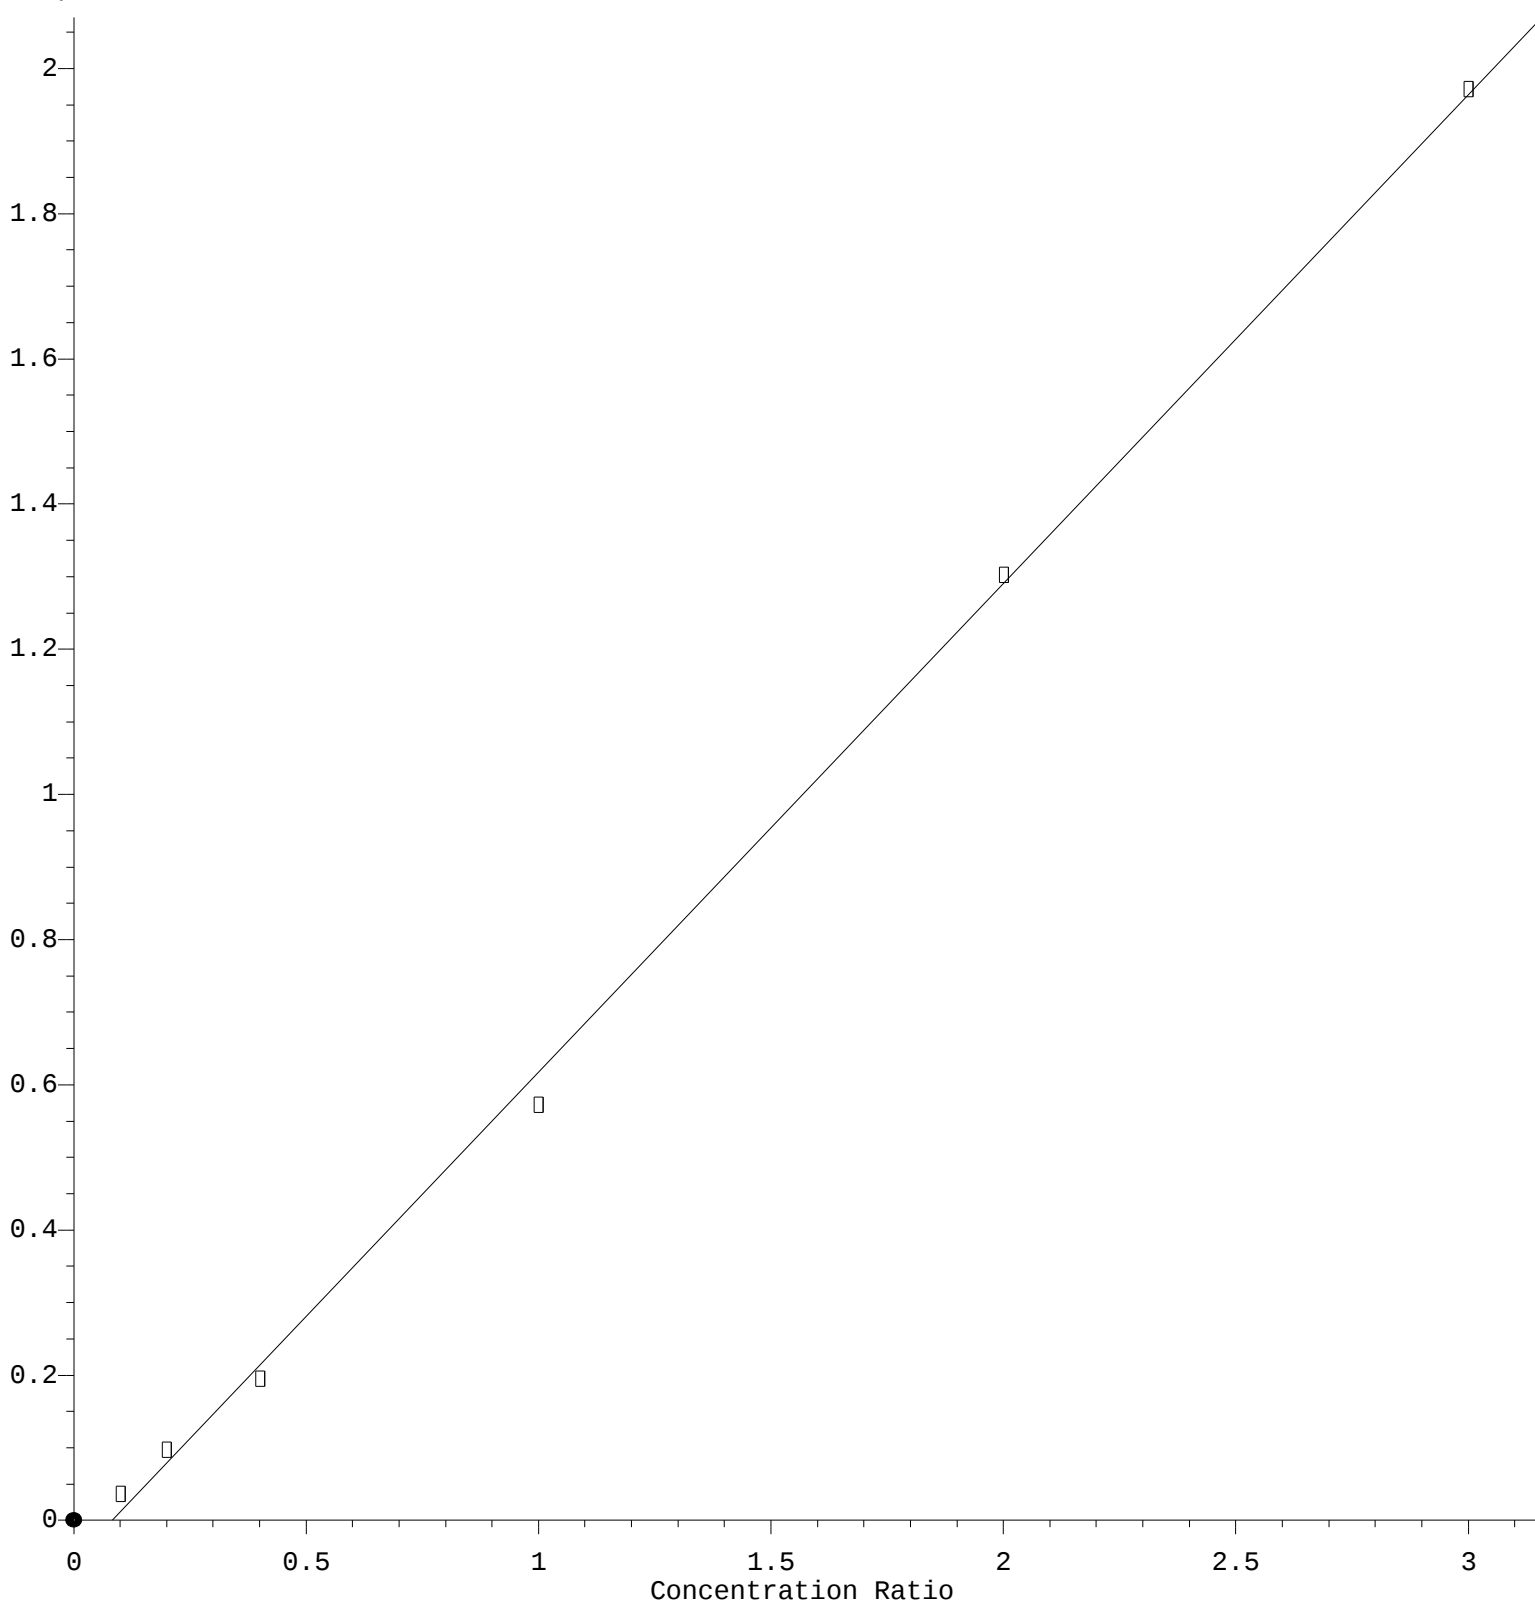


$$\text{Response} = 6.733\text{e-}001 * \text{Amt} - 5.619\text{e-}002$$

Coef of Det (r^2) = 0.998841 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M

Calibration Table Last Updated: Thu Jun 09 12:33:32 2022


Tert butylalcohol

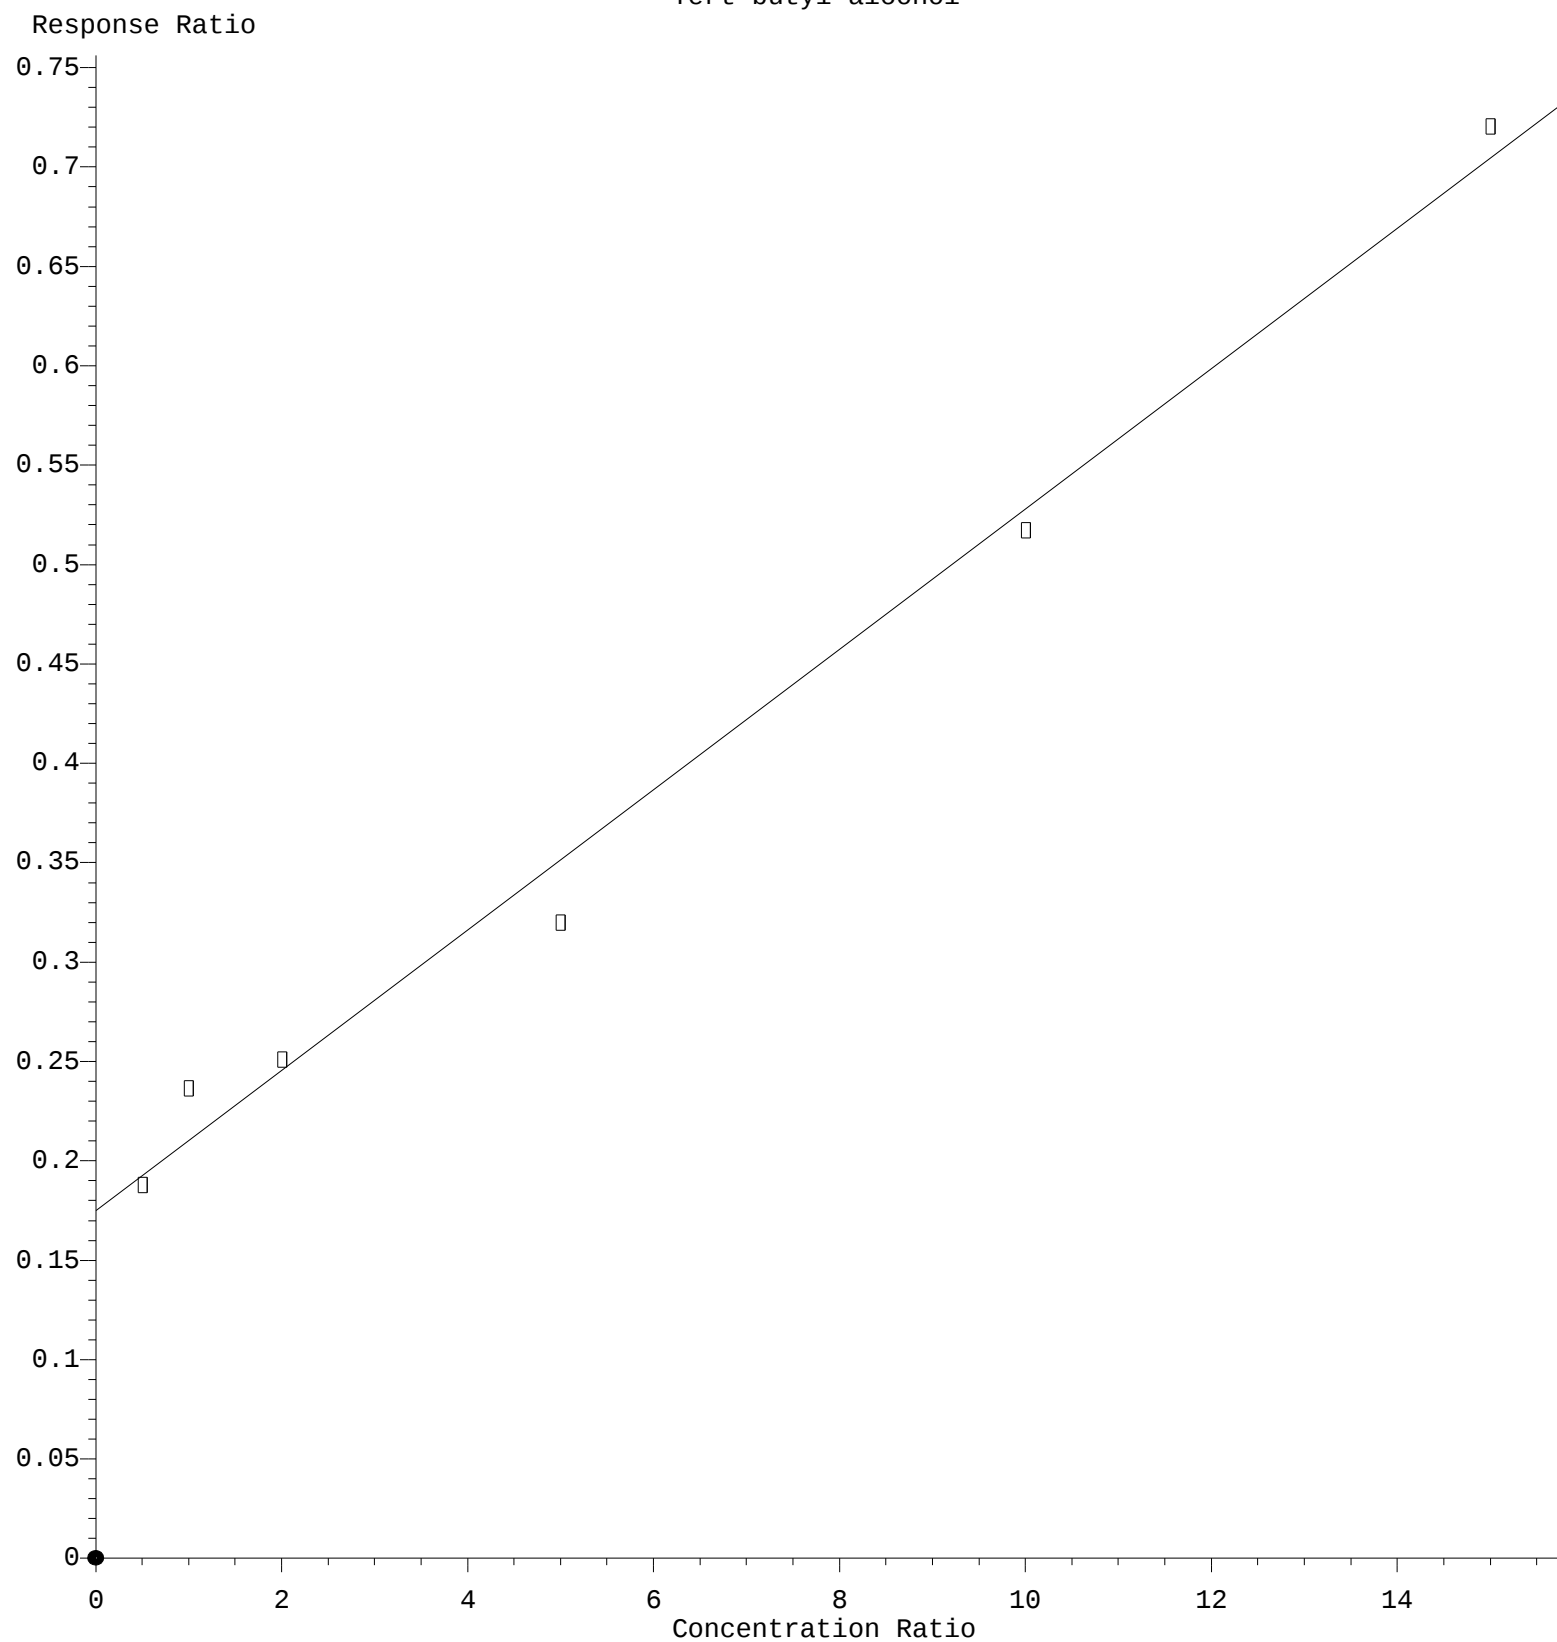

Response = $3.533\text{e-}002 \times \text{Amt} + 1.747\text{e-}001$
 Coef of Det (r^2) = 0.990123 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
 Calibration Table Last Updated: Thu Jun 09 12:33:32 2022

Methylene Chloride

Response Ratio

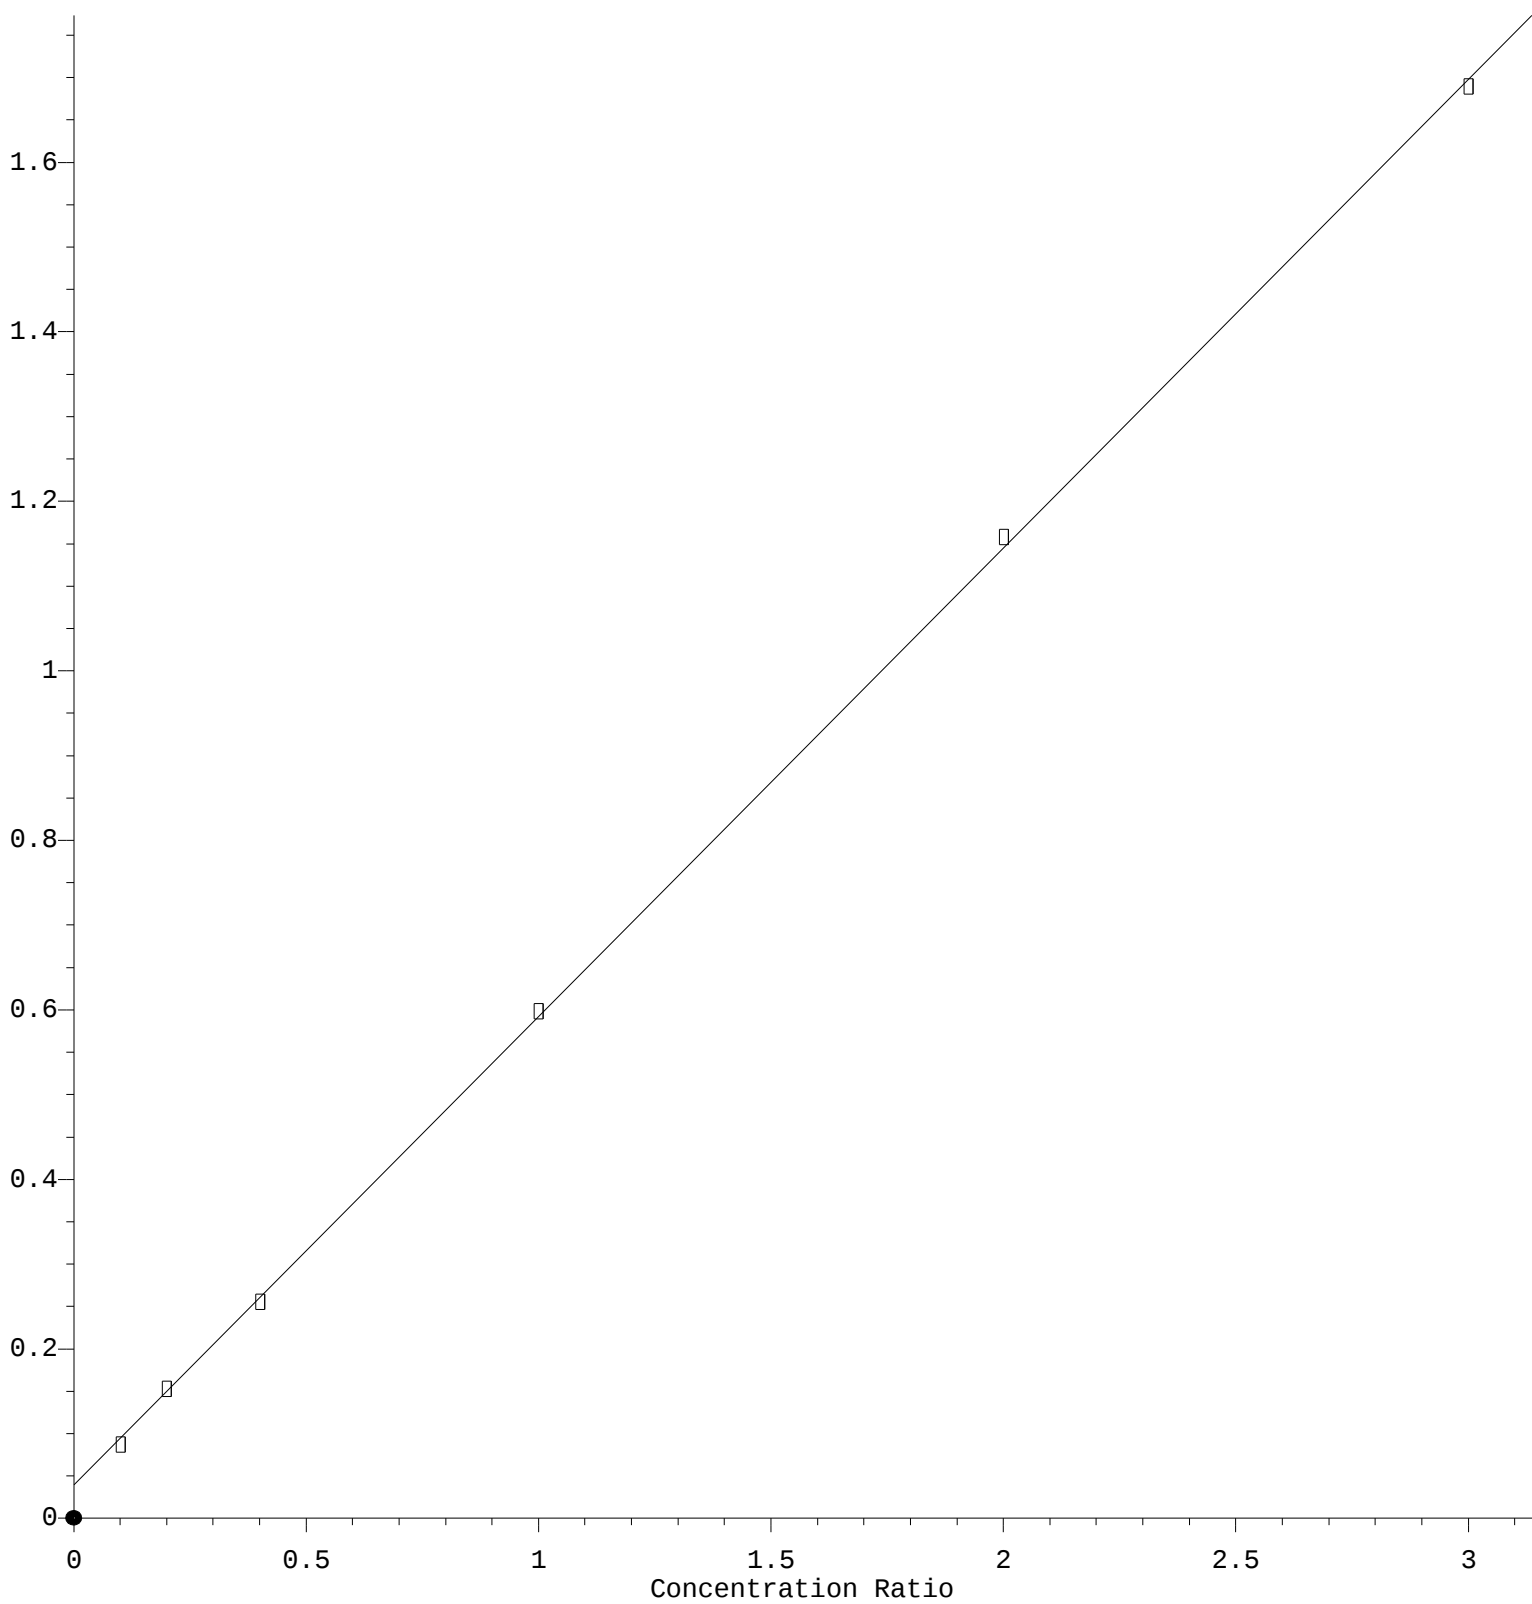

$$\text{Response} = 5.533\text{e-}001 * \text{Amt} + 3.868\text{e-}002$$


Coef of Det (r^2) = 0.999831 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M

Calibration Table Last Updated: Thu Jun 09 12:33:32 2022

Naphthalene

Response Ratio

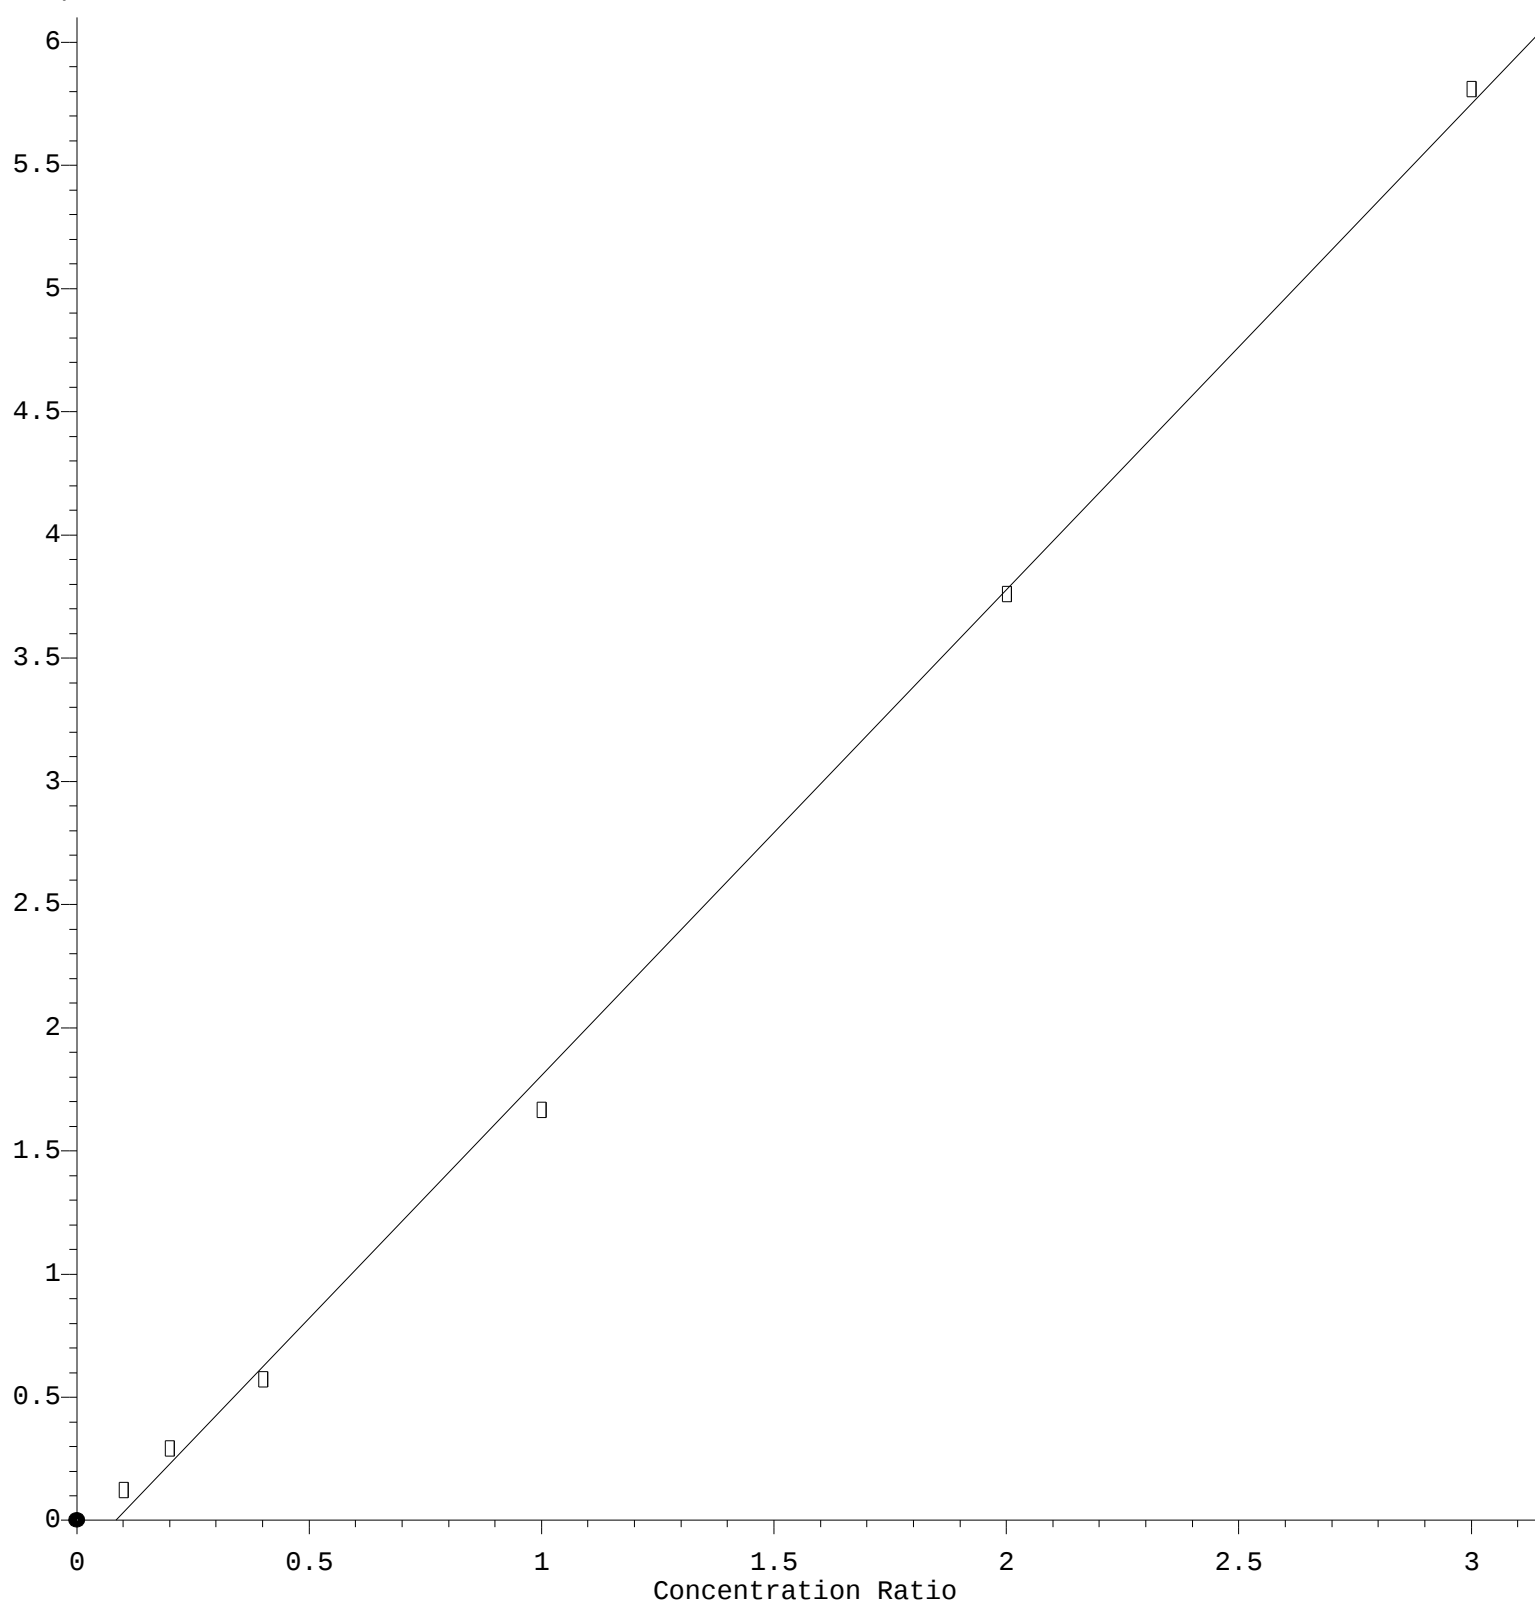

$$\text{Response} = 1.972\text{e}+000 * \text{Amt} - 1.658\text{e}-001$$


Coef of Det (r^2) = 0.998530 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M

Calibration Table Last Updated: Thu Jun 09 12:33:32 2022

Methyl Acetate

Response Ratio

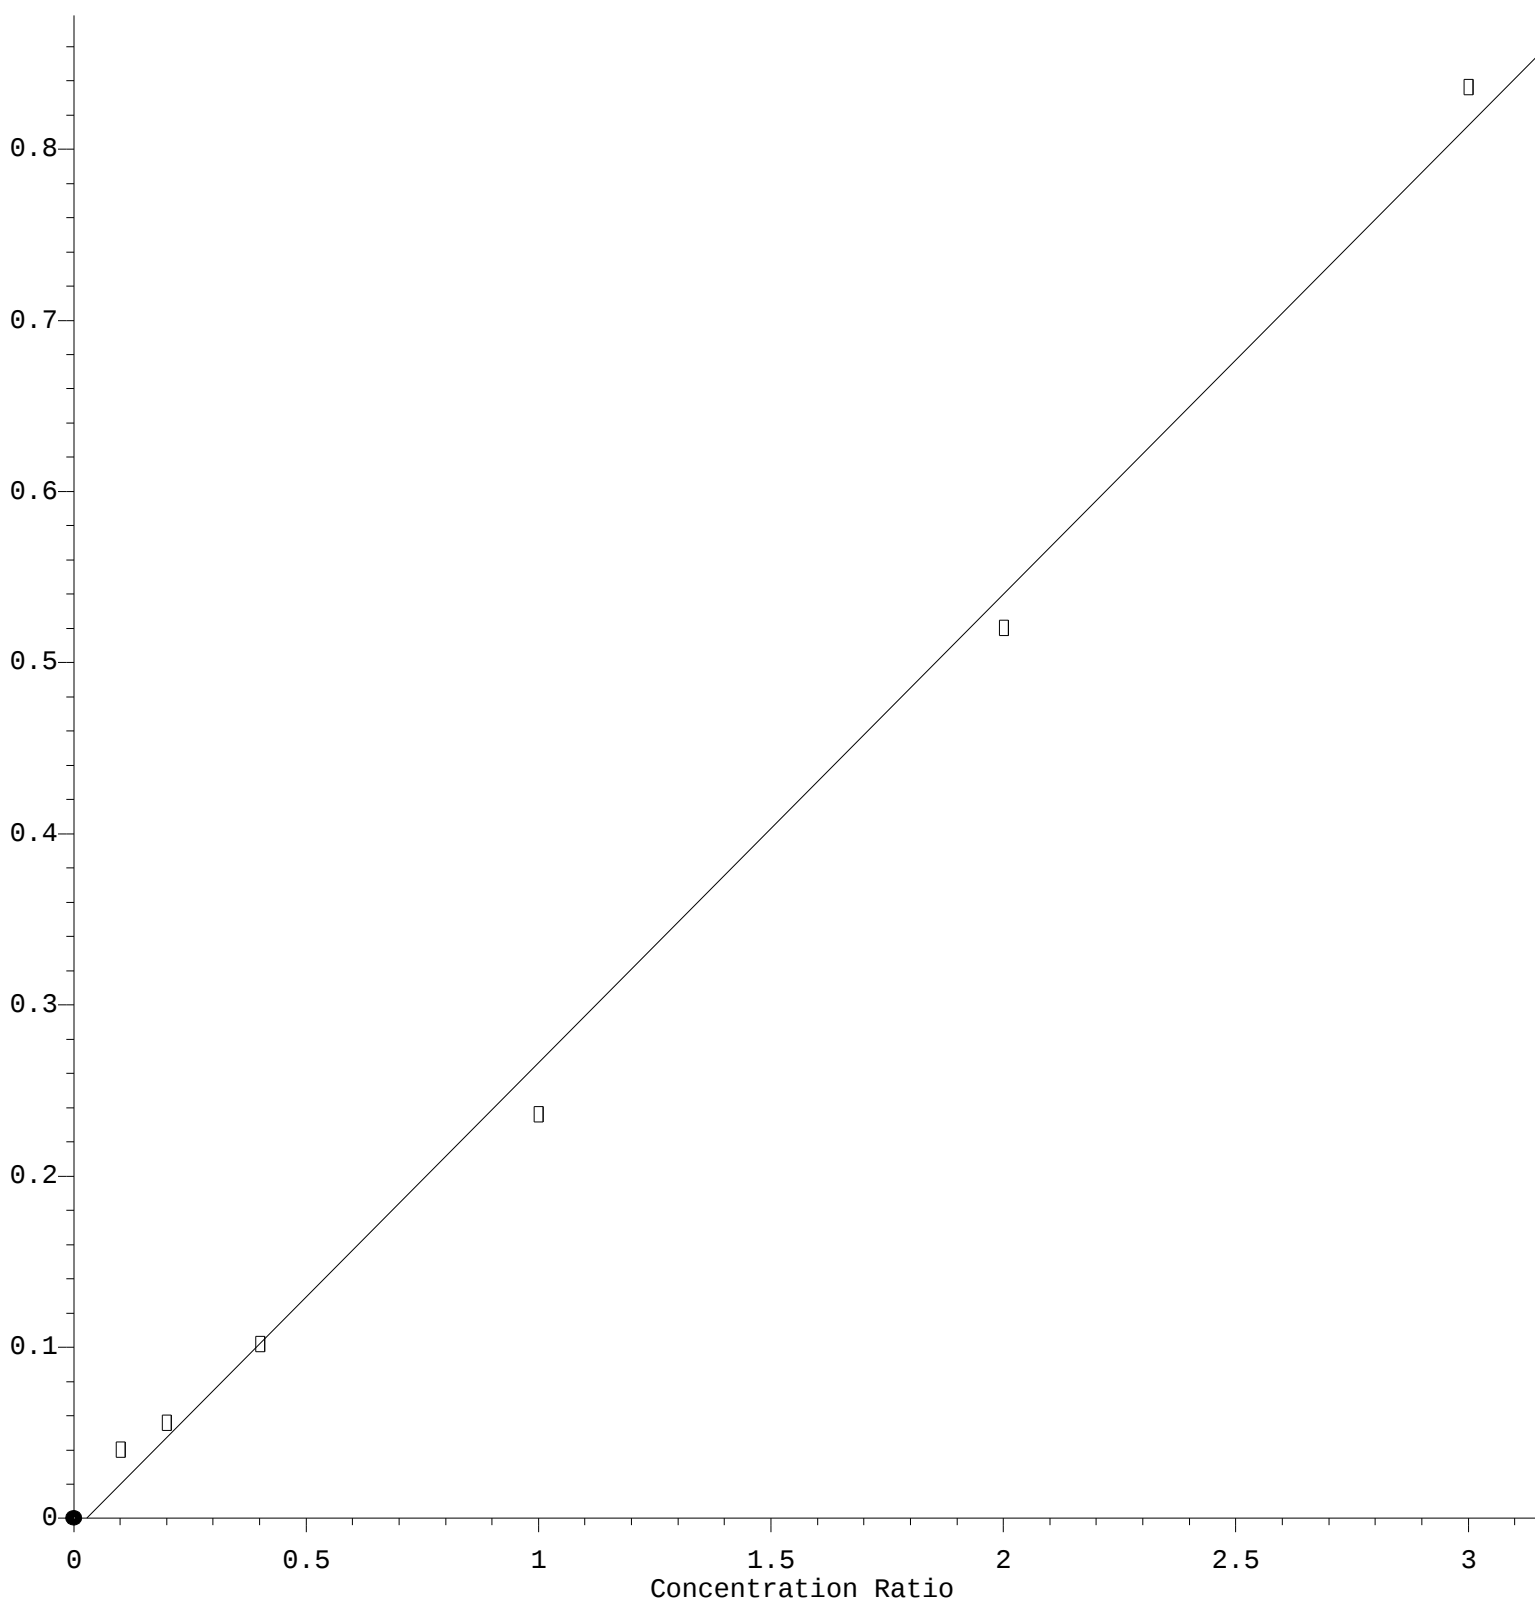

$$\text{Response} = 2.738\text{e-}001 * \text{Amt} - 7.498\text{e-}003$$

Coef of Det (r^2) = 0.995463 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M

Calibration Table Last Updated: Thu Jun 09 12:33:32 2022