


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD061019\
 Data File : VD062645.D
 Acq On : 10 Jun 2019 10:04
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
 Title : SW846 8260
 Last Update : Sat Jun 08 00:02:21 2019

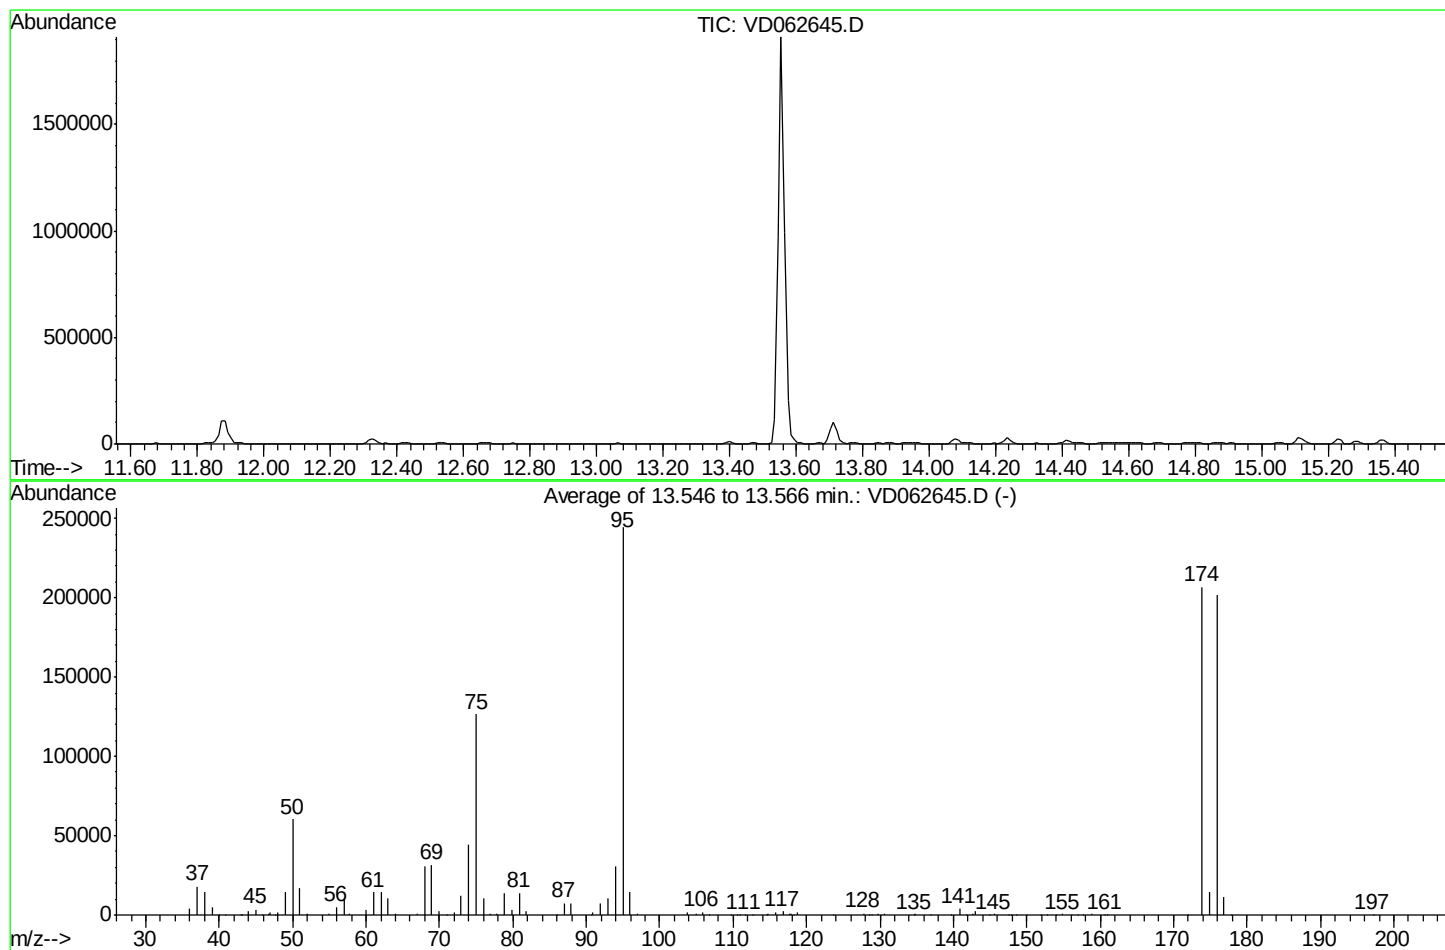

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	60173	PASS
75	95	30	60	51.8	126477	PASS
95	95	100	100	100.0	244352	PASS
96	95	5	9	6.0	14754	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.6	206768	PASS
175	174	5	9	7.0	14438	PASS
176	174	95	101	97.4	201330	PASS
177	176	5	9	5.6	11321	PASS