


Bromomethane

Response Ratio

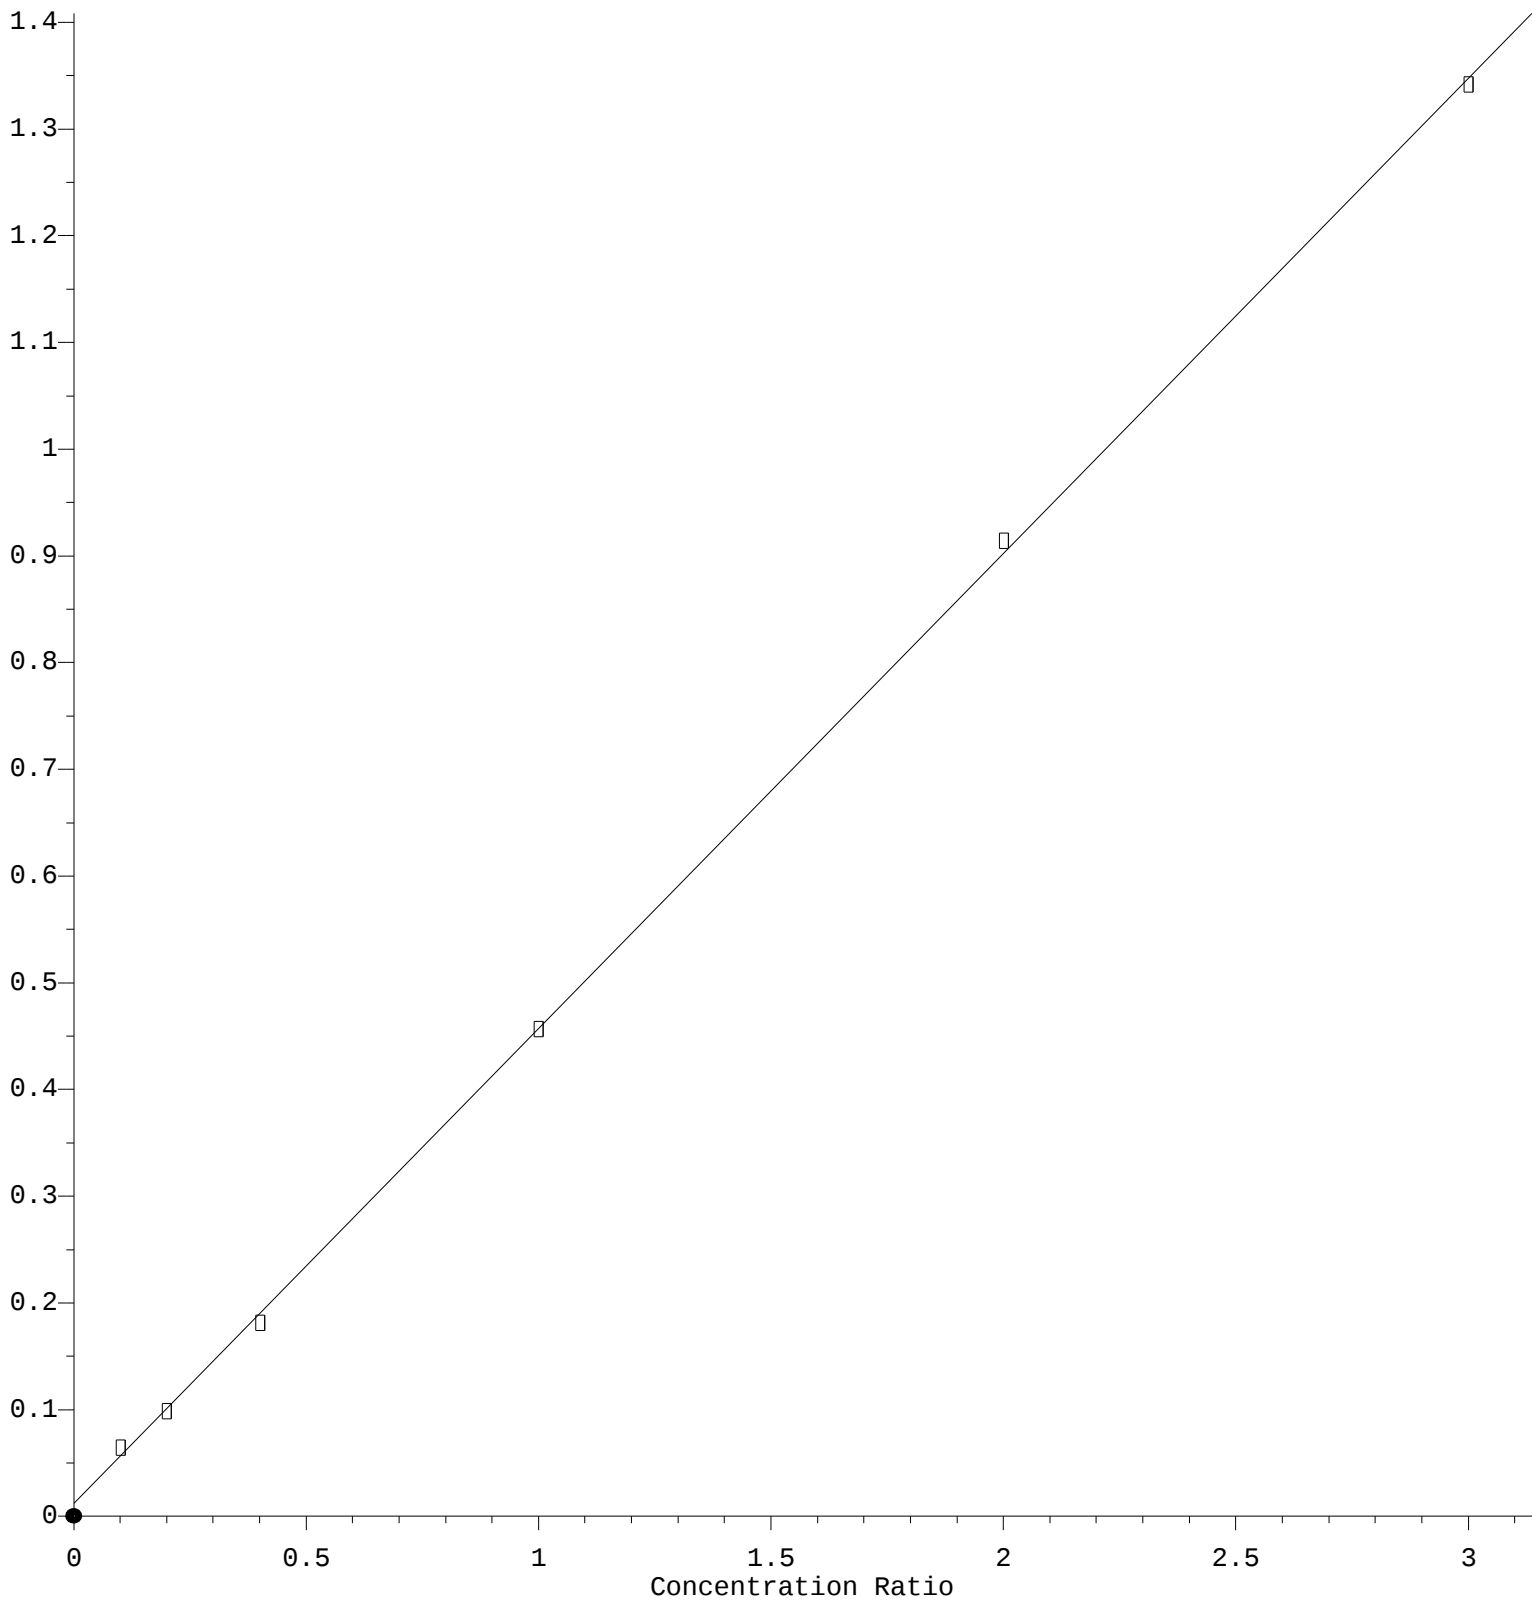

$$\text{Response} = 4.452\text{e-}001 * \text{Amt} + 1.204\text{e-}002$$


Coef of Det (r^2) = 0.999755 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

Methyl Iodide

Response Ratio

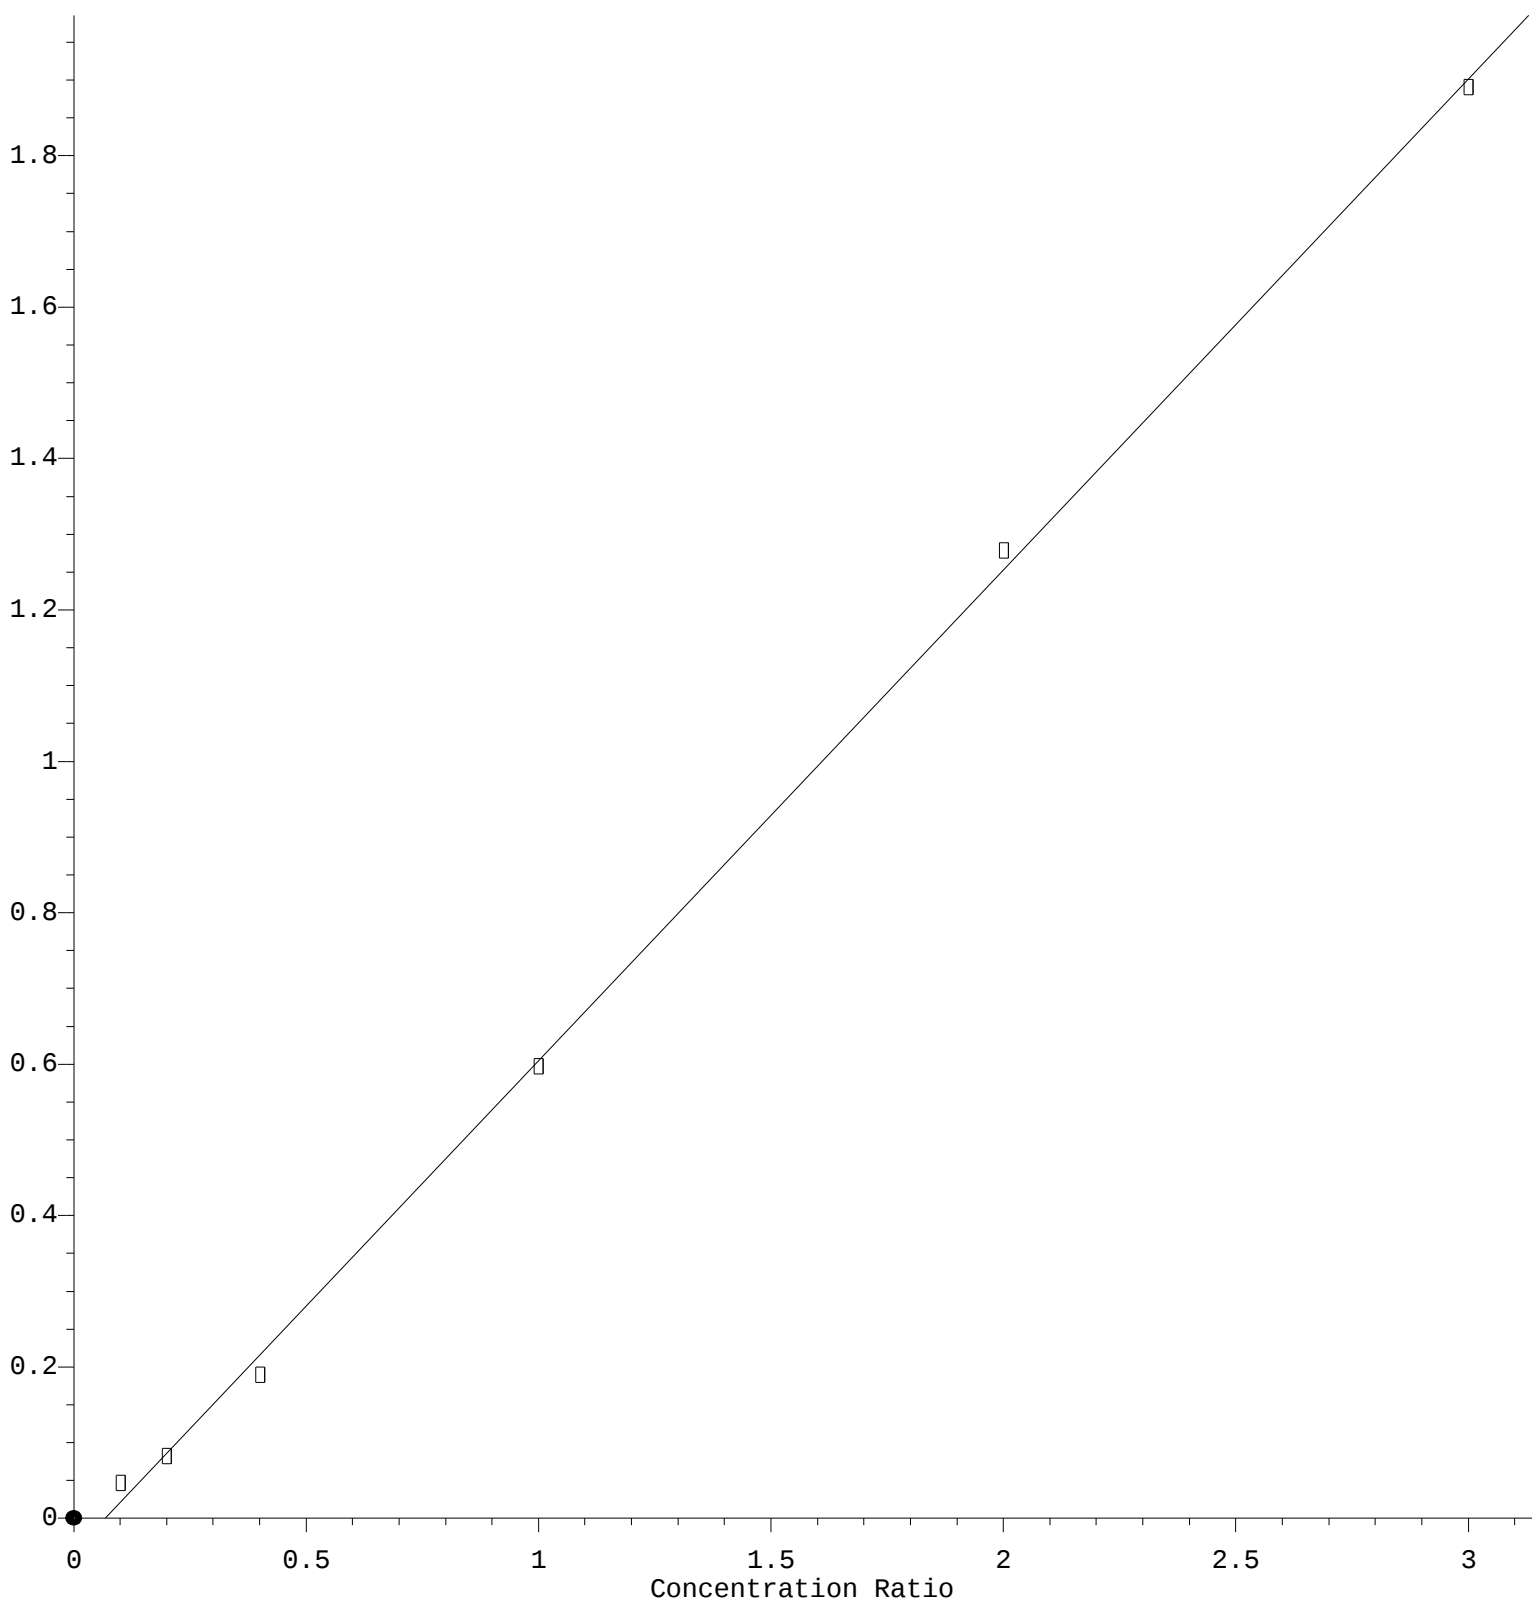


$$\text{Response} = 6.482\text{e-}001 * \text{Amt} - 4.324\text{e-}002$$

Coef of Det (r^2) = 0.999222 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021


Methyl Acetate

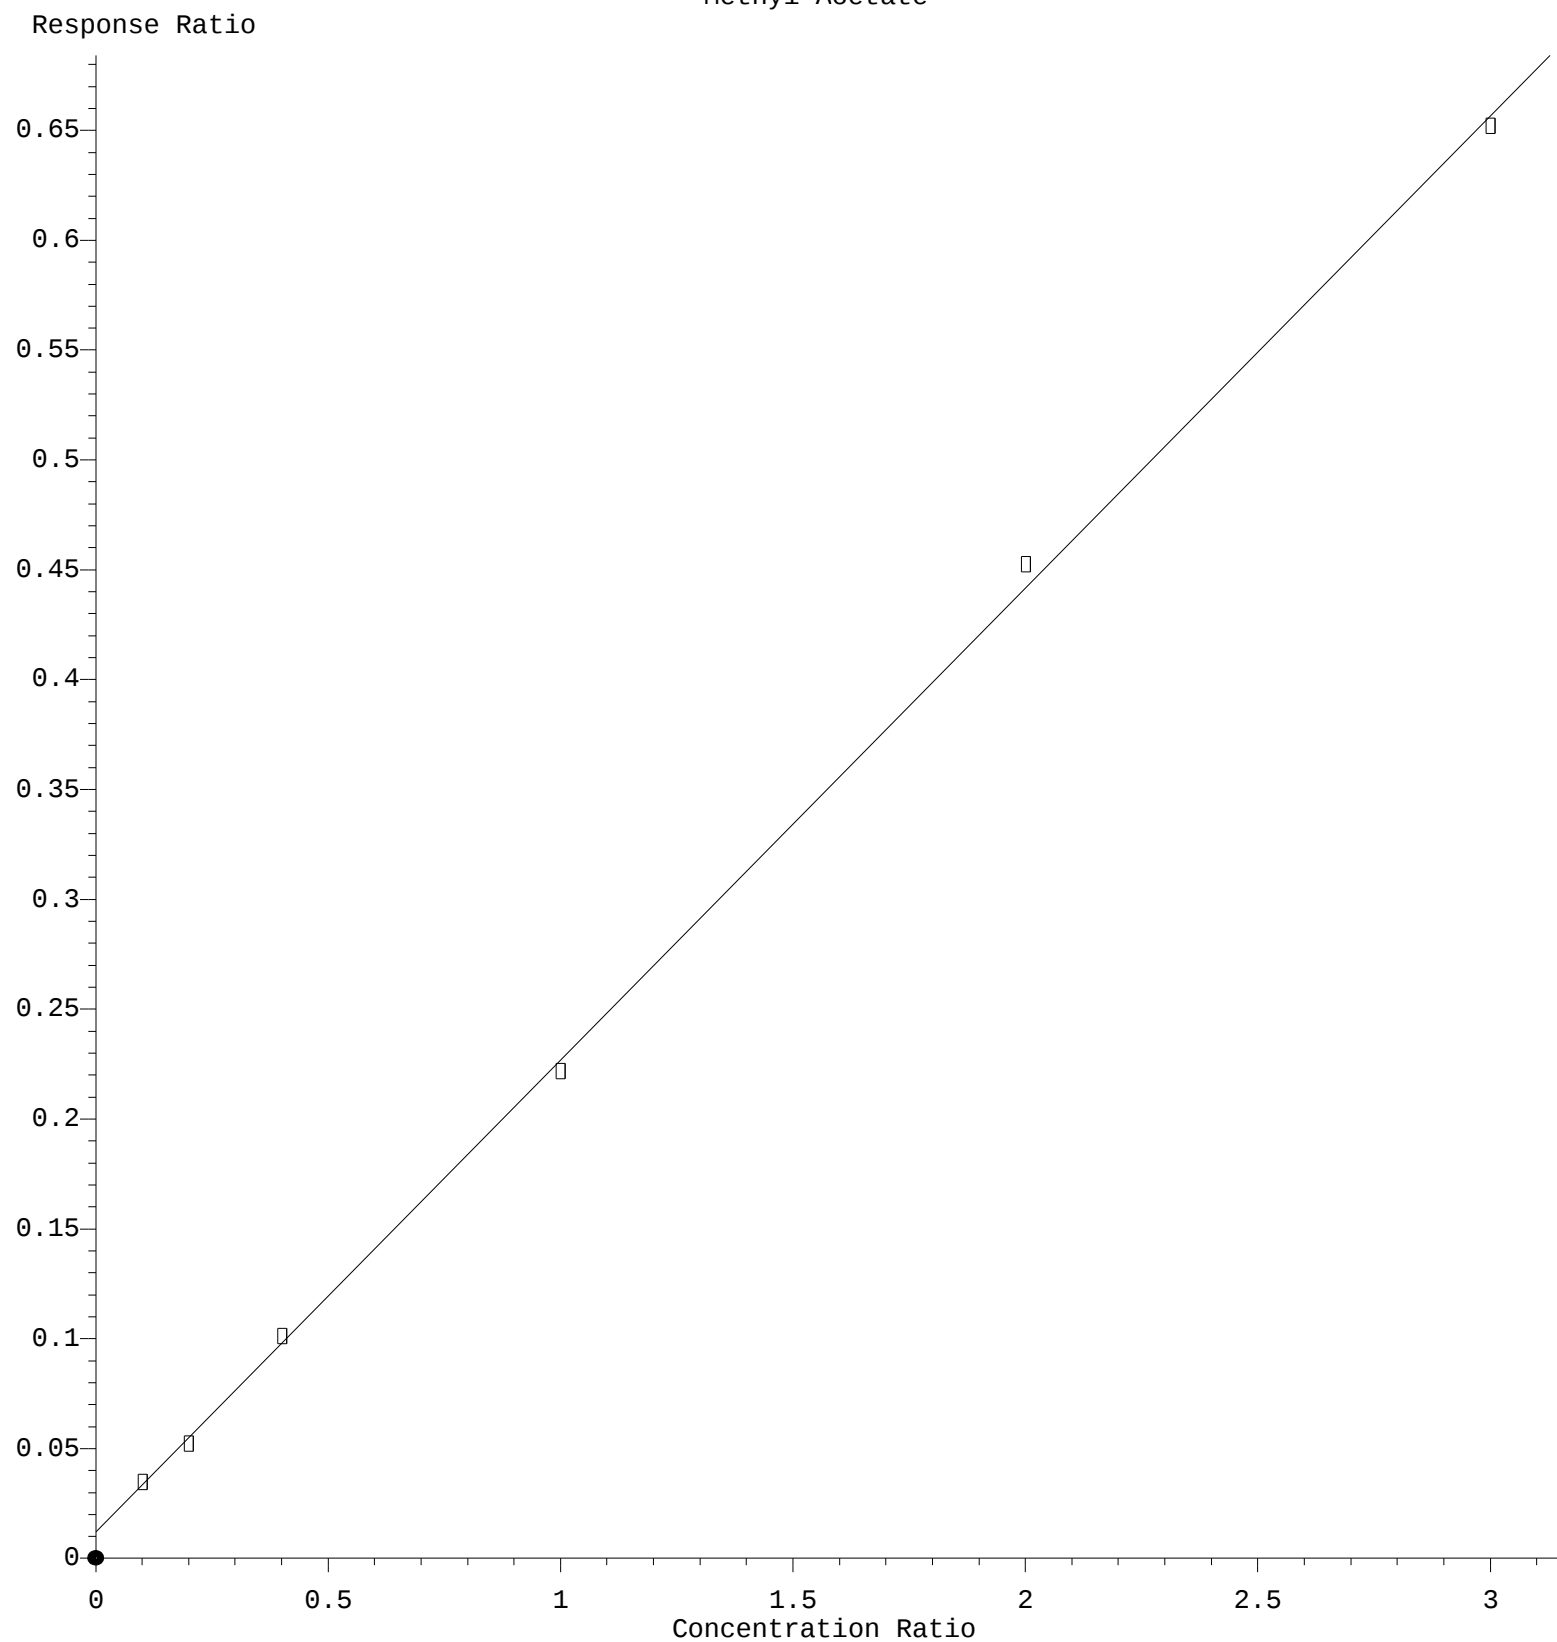

Response = 2.149e-001 * Amt + 1.231e-002
 Coef of Det (r^2) = 0.999420 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M
 Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

Methylene Chloride

Response Ratio

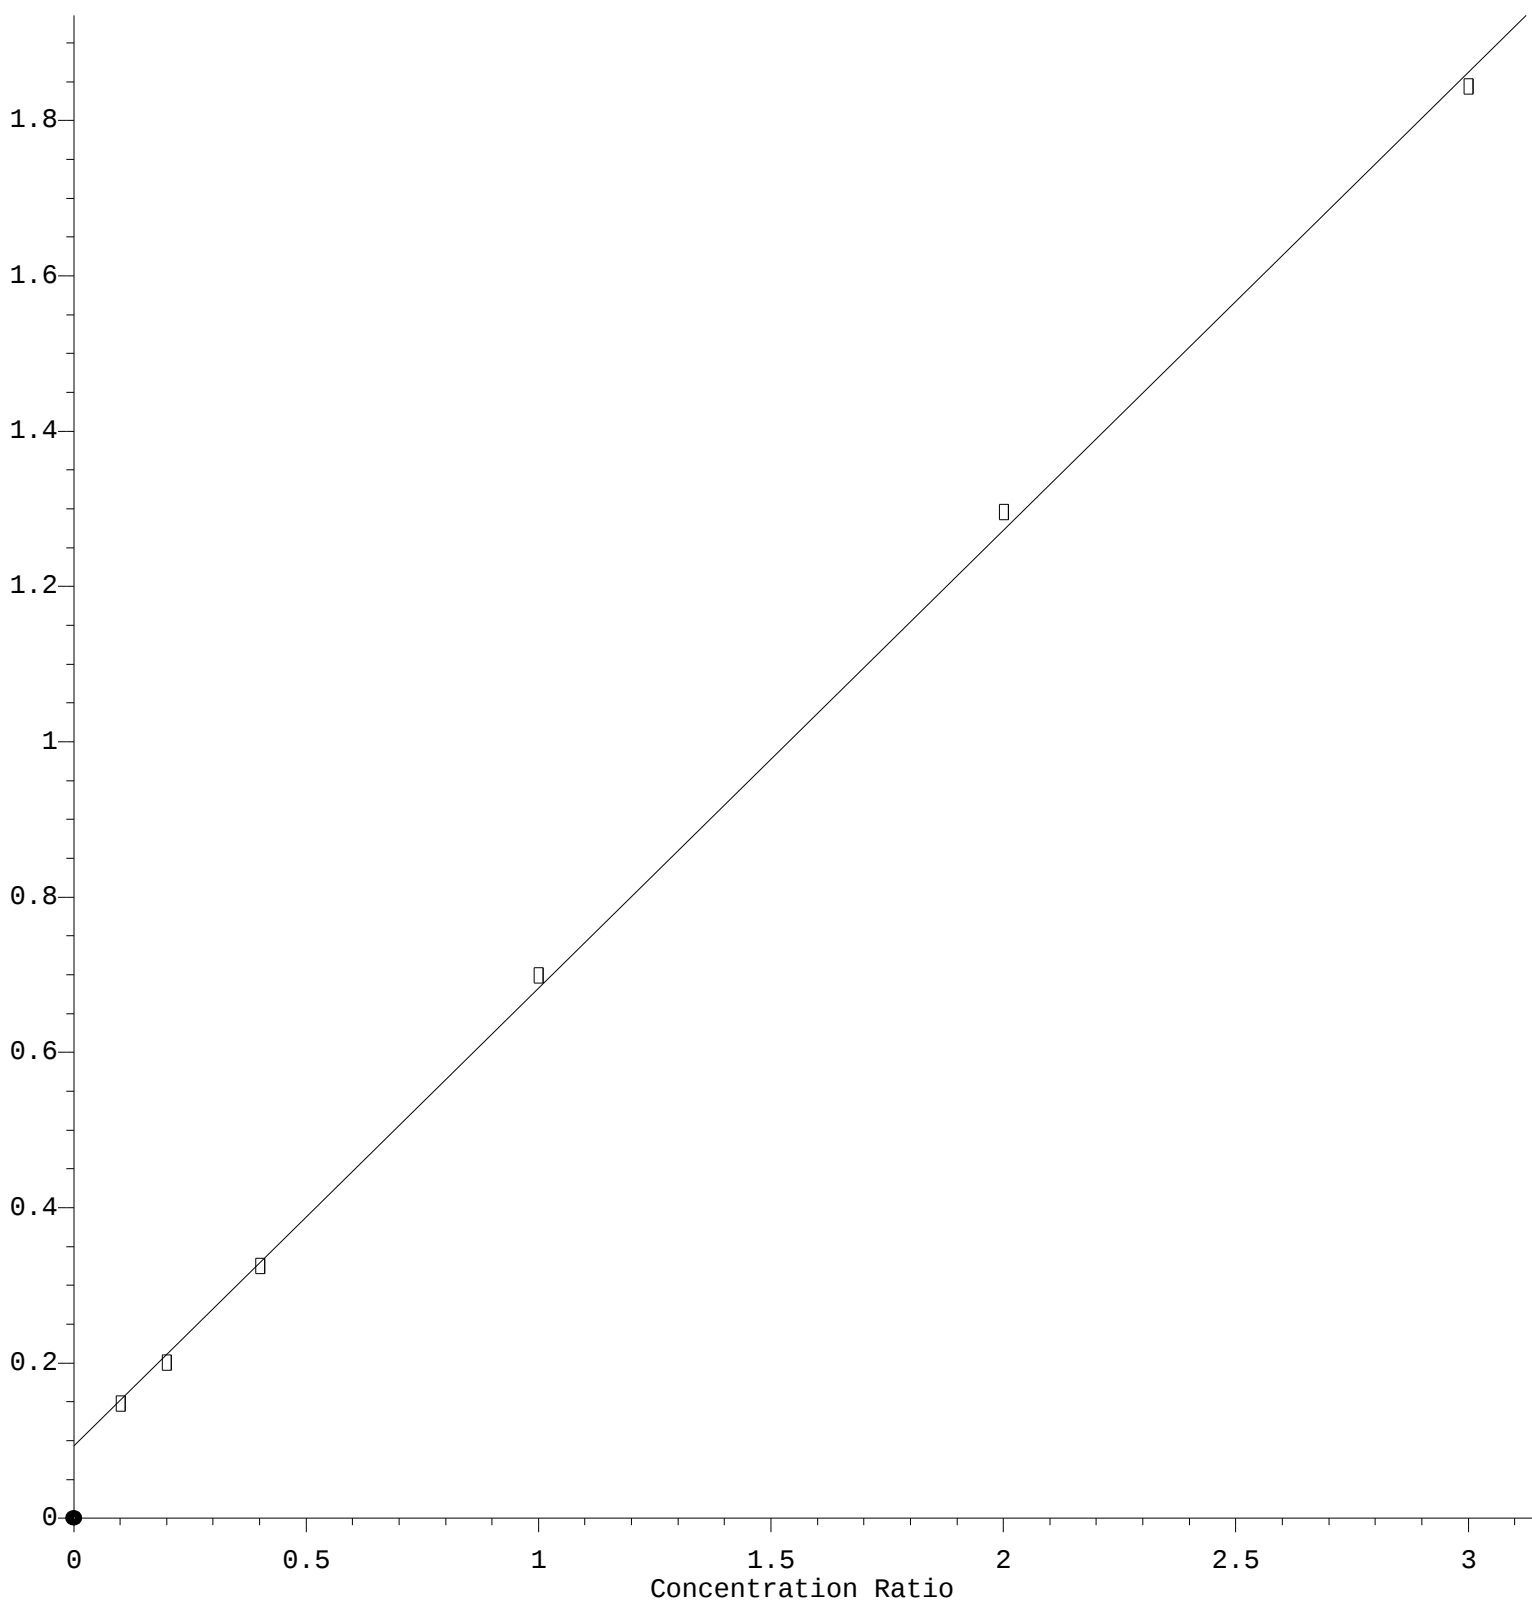

$$\text{Response} = 5.898\text{e-}001 * \text{Amt} + 9.295\text{e-}002$$


Coef of Det (r^2) = 0.999451 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

Vinyl Acetate

Response Ratio

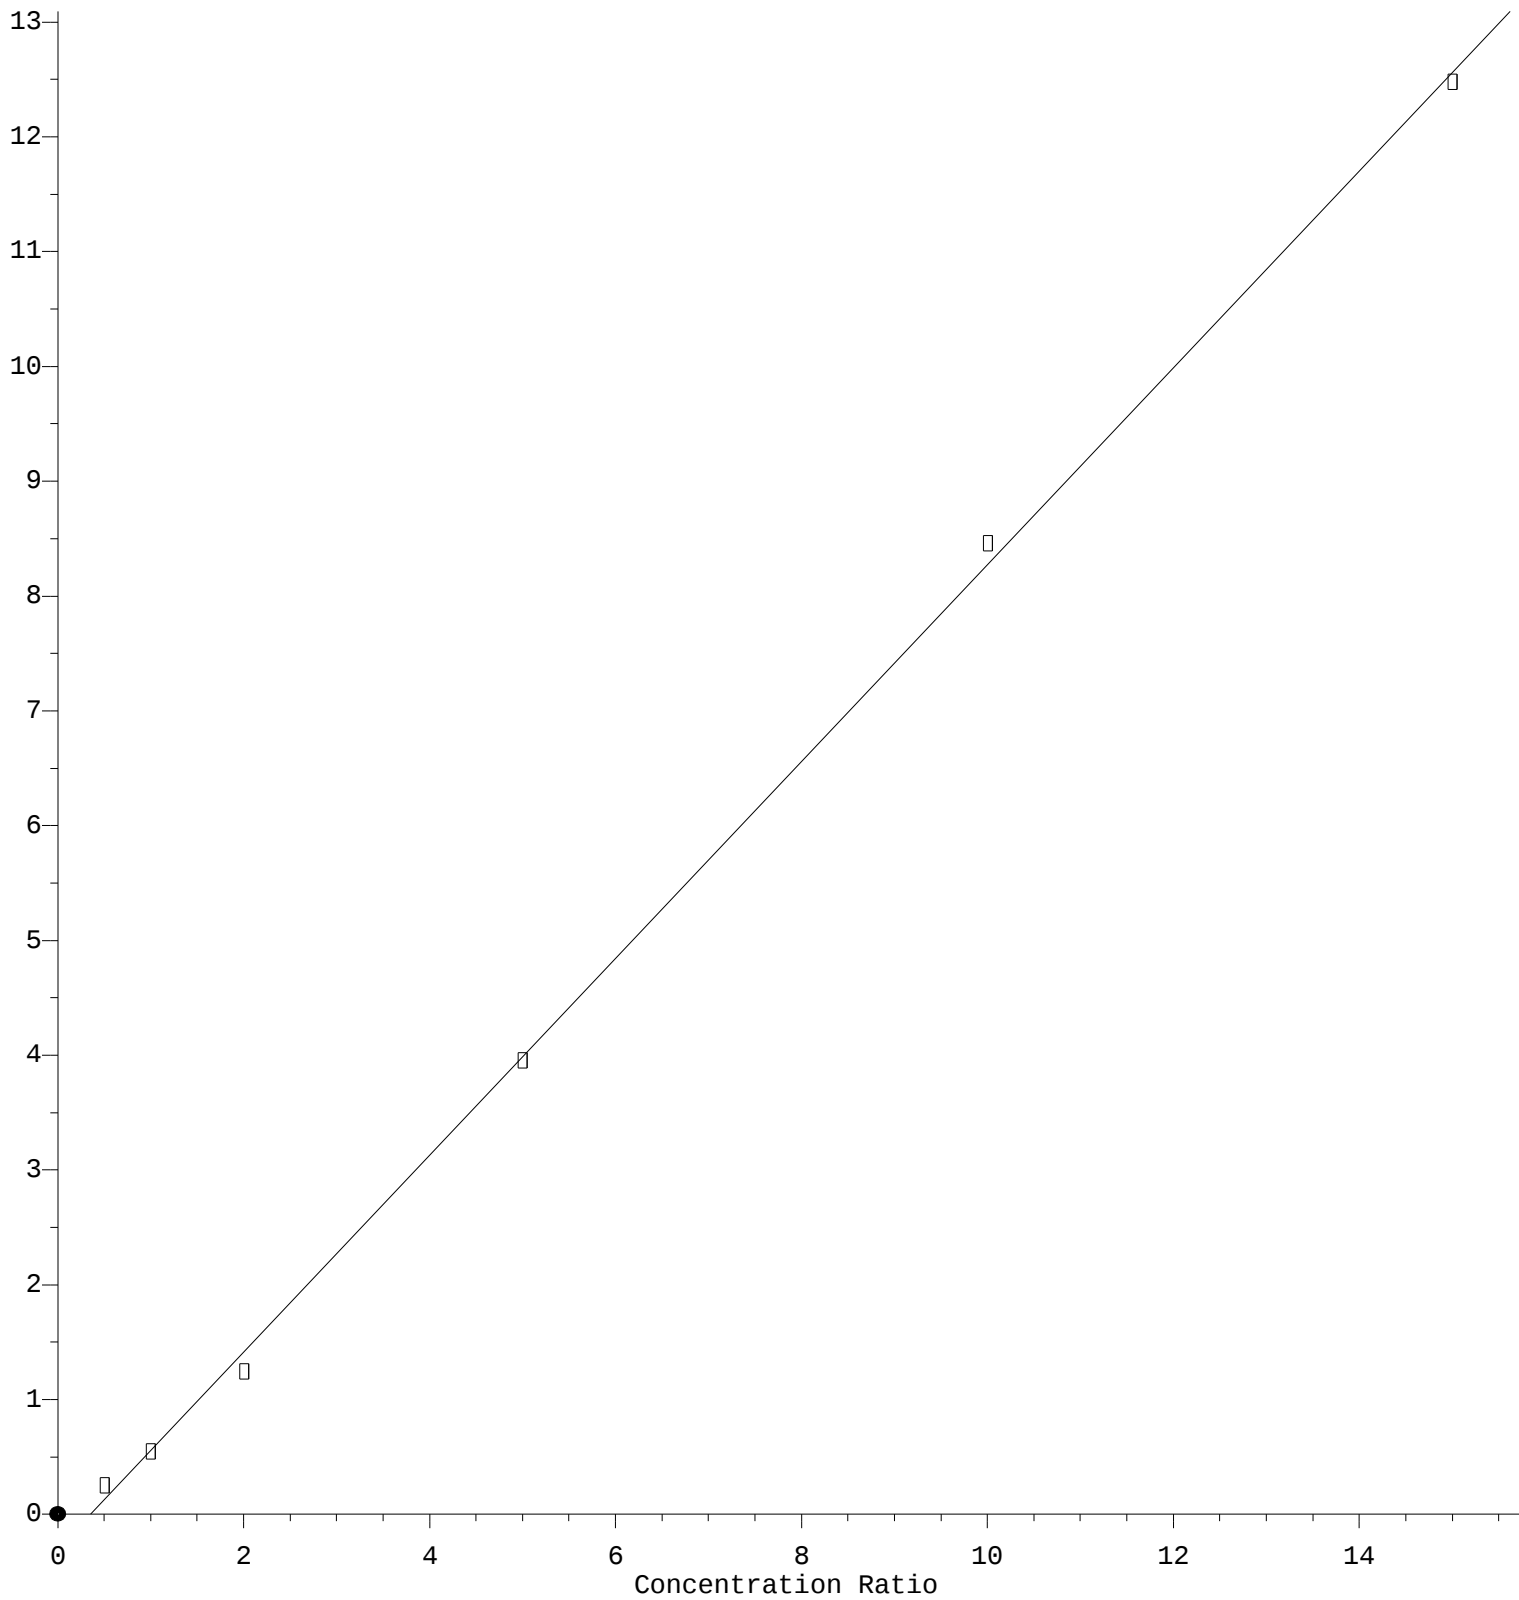

$$\text{Response} = 8.577\text{e-}001 * \text{Amt} - 3.015\text{e-}001$$


Coef of Det (r^2) = 0.999295 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

Ethyl methacrylate

Response Ratio

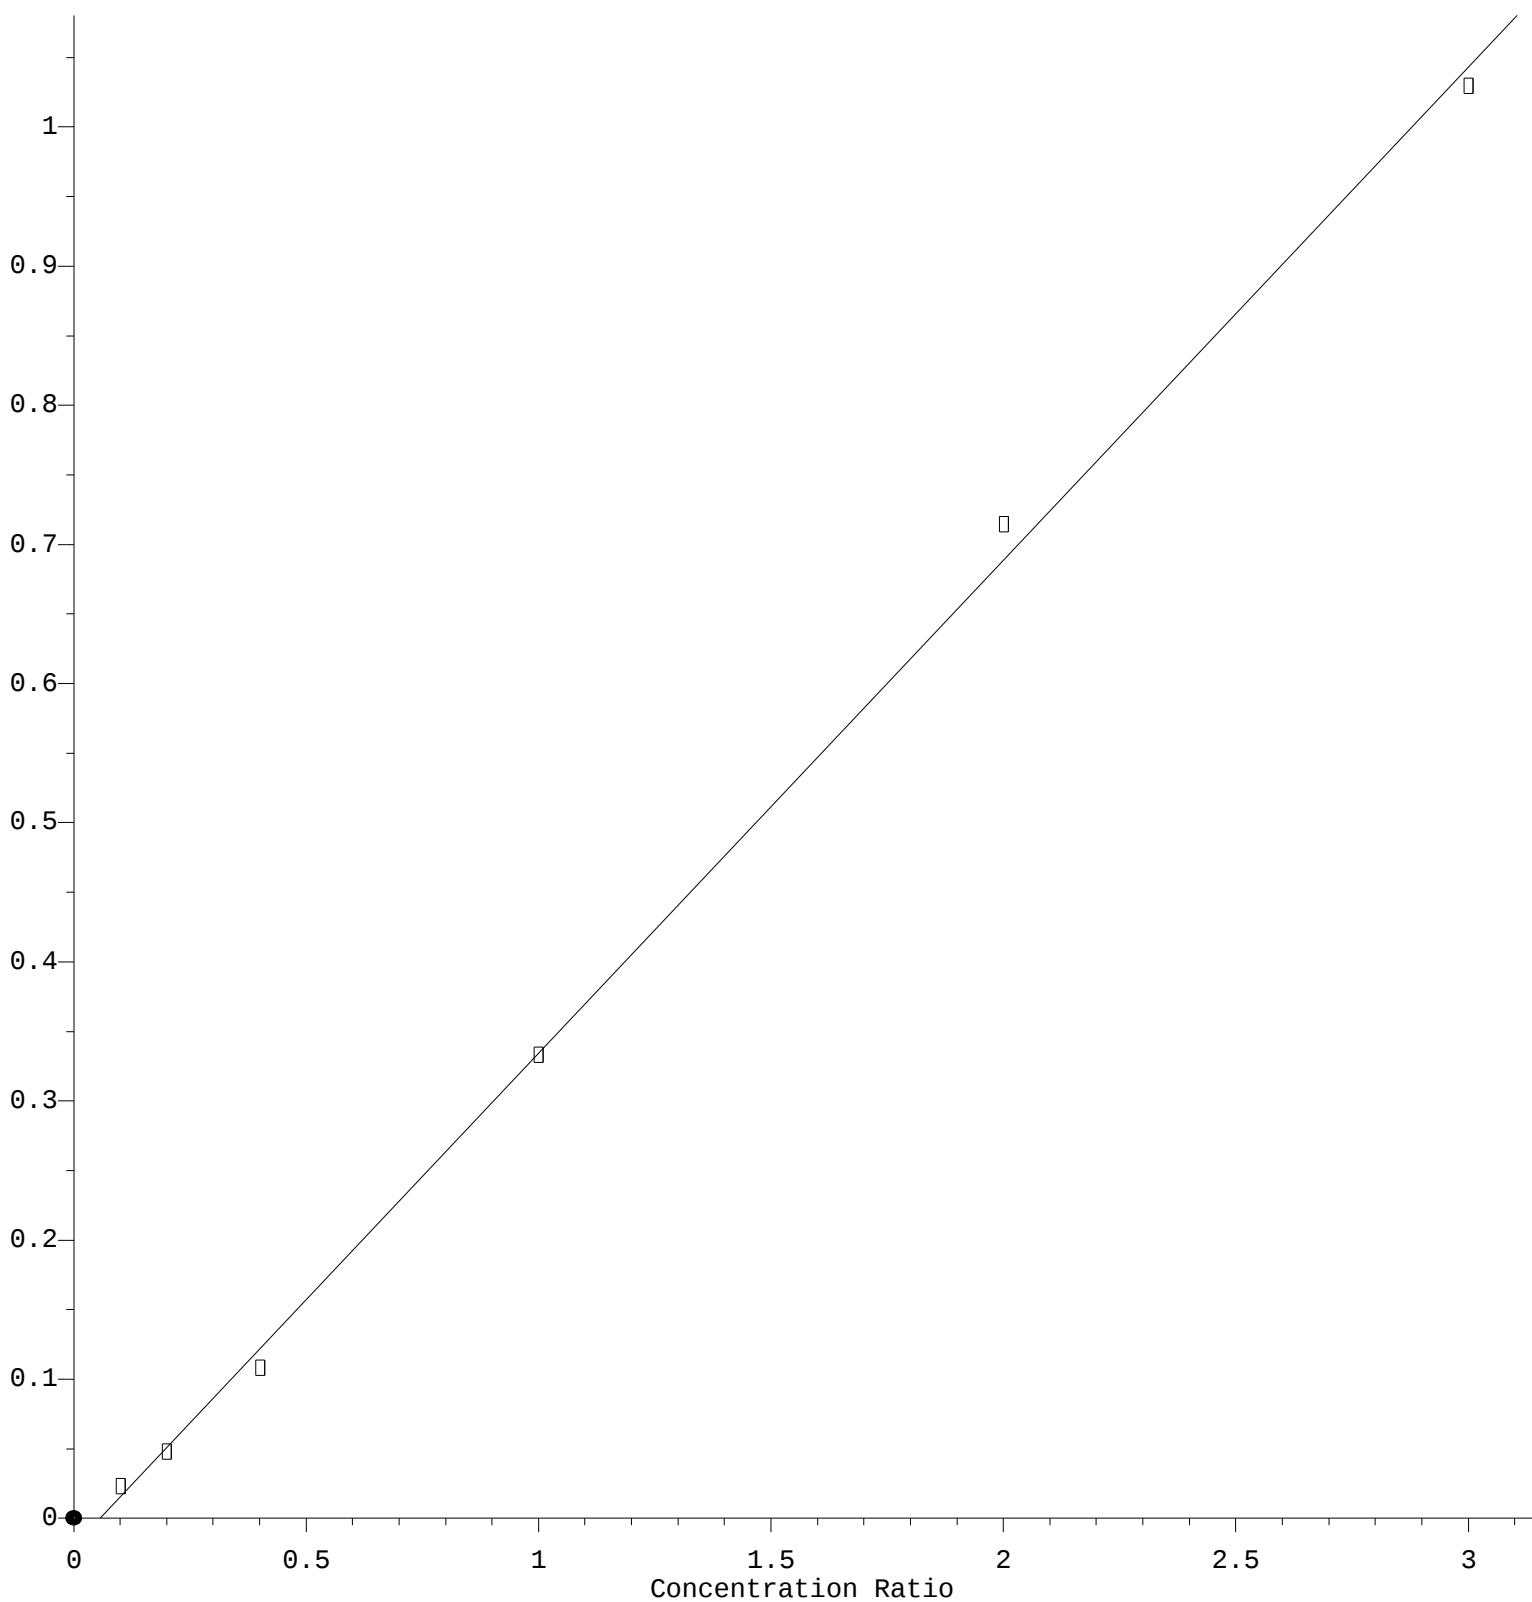

$$\text{Response} = 3.546\text{e-}001 * \text{Amt} - 2.002\text{e-}002$$


Coef of Det (r^2) = 0.998703 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

2-Chloroethyl Vinyl ether

Response Ratio

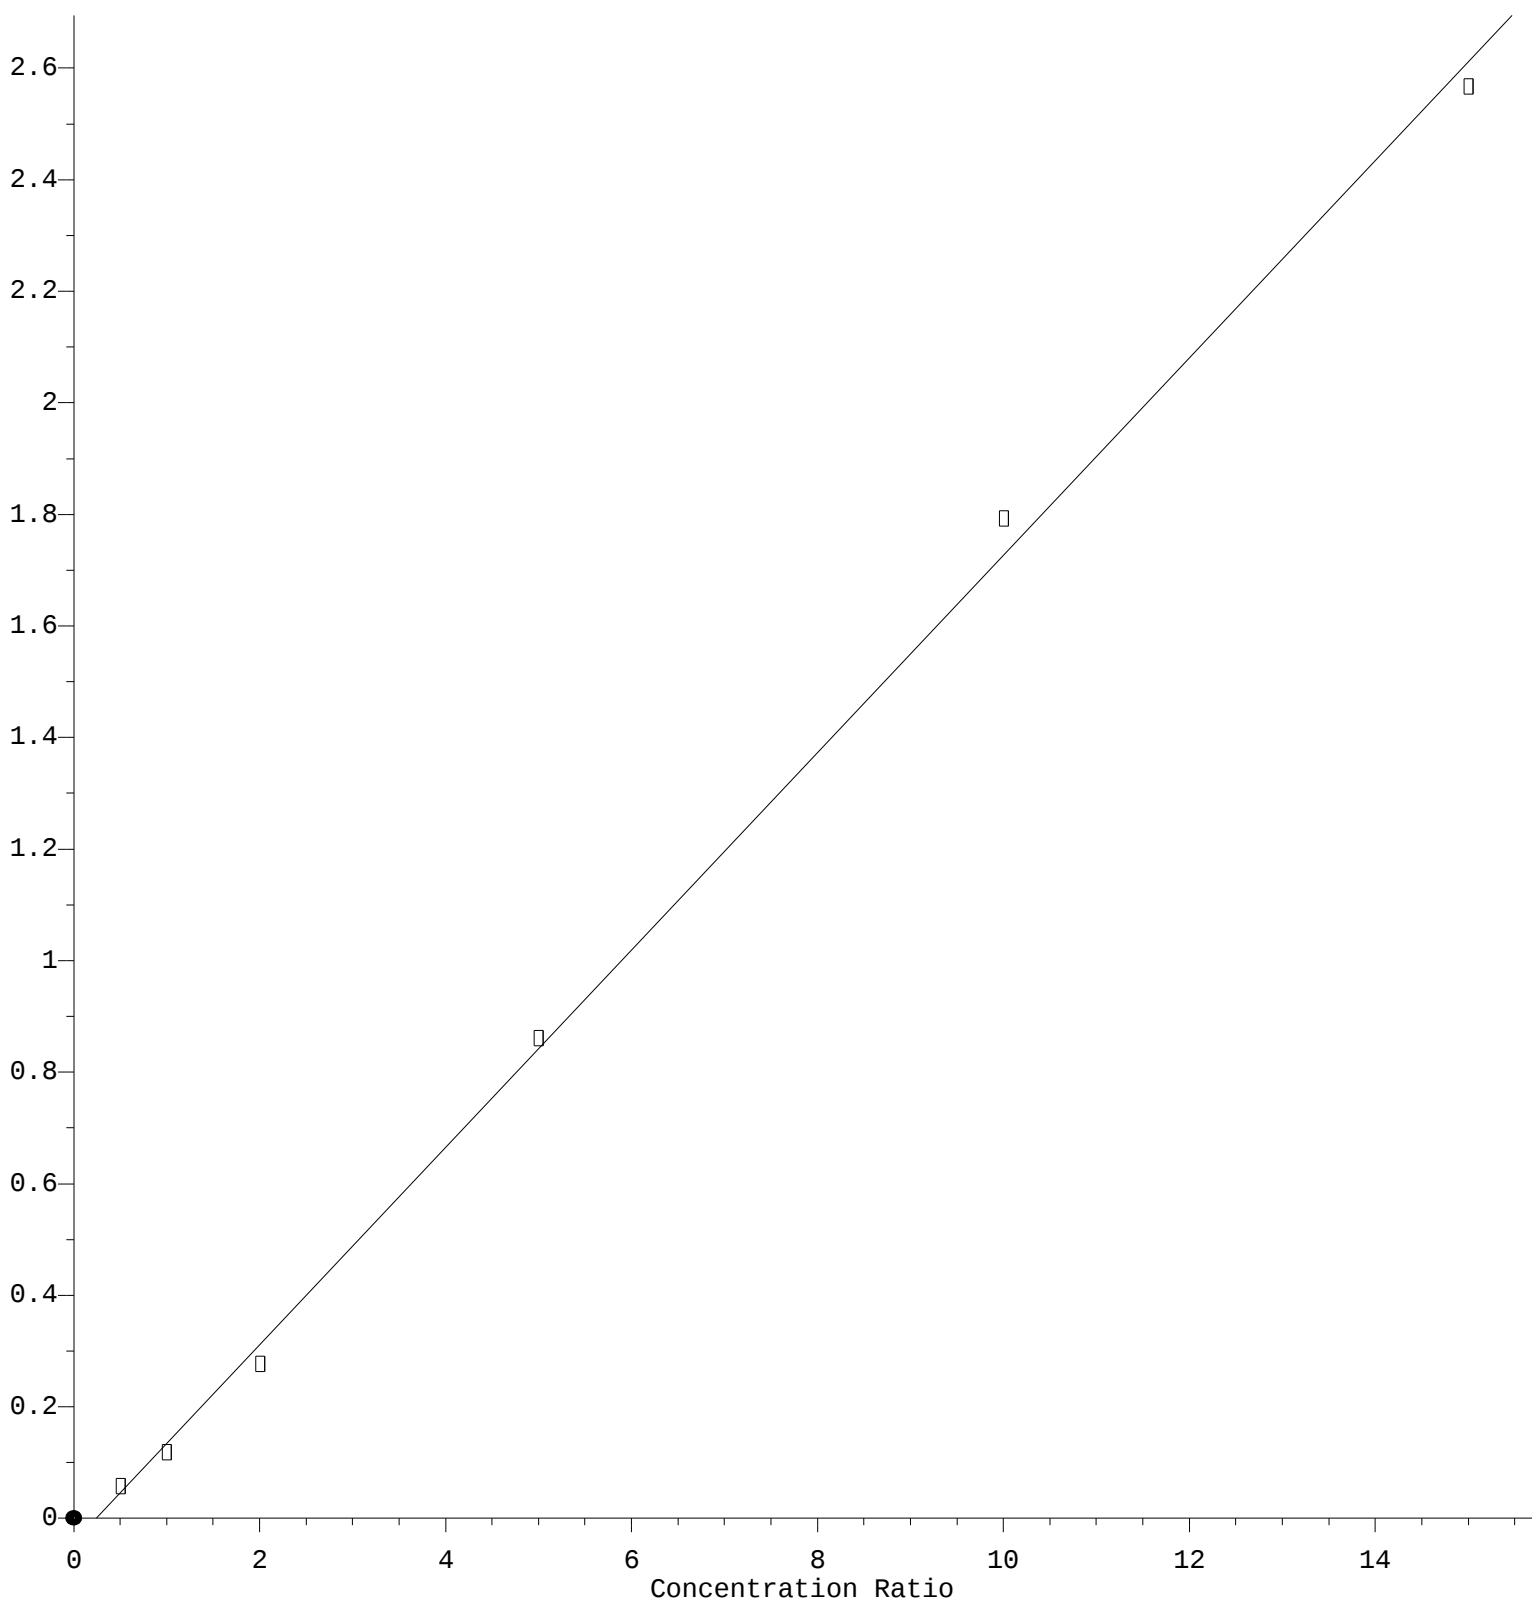

$$\text{Response} = 1.769\text{e-}001 * \text{Amt} - 4.224\text{e-}002$$


Coef of Det (r^2) = 0.998434 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021

Naphthalene

Response Ratio

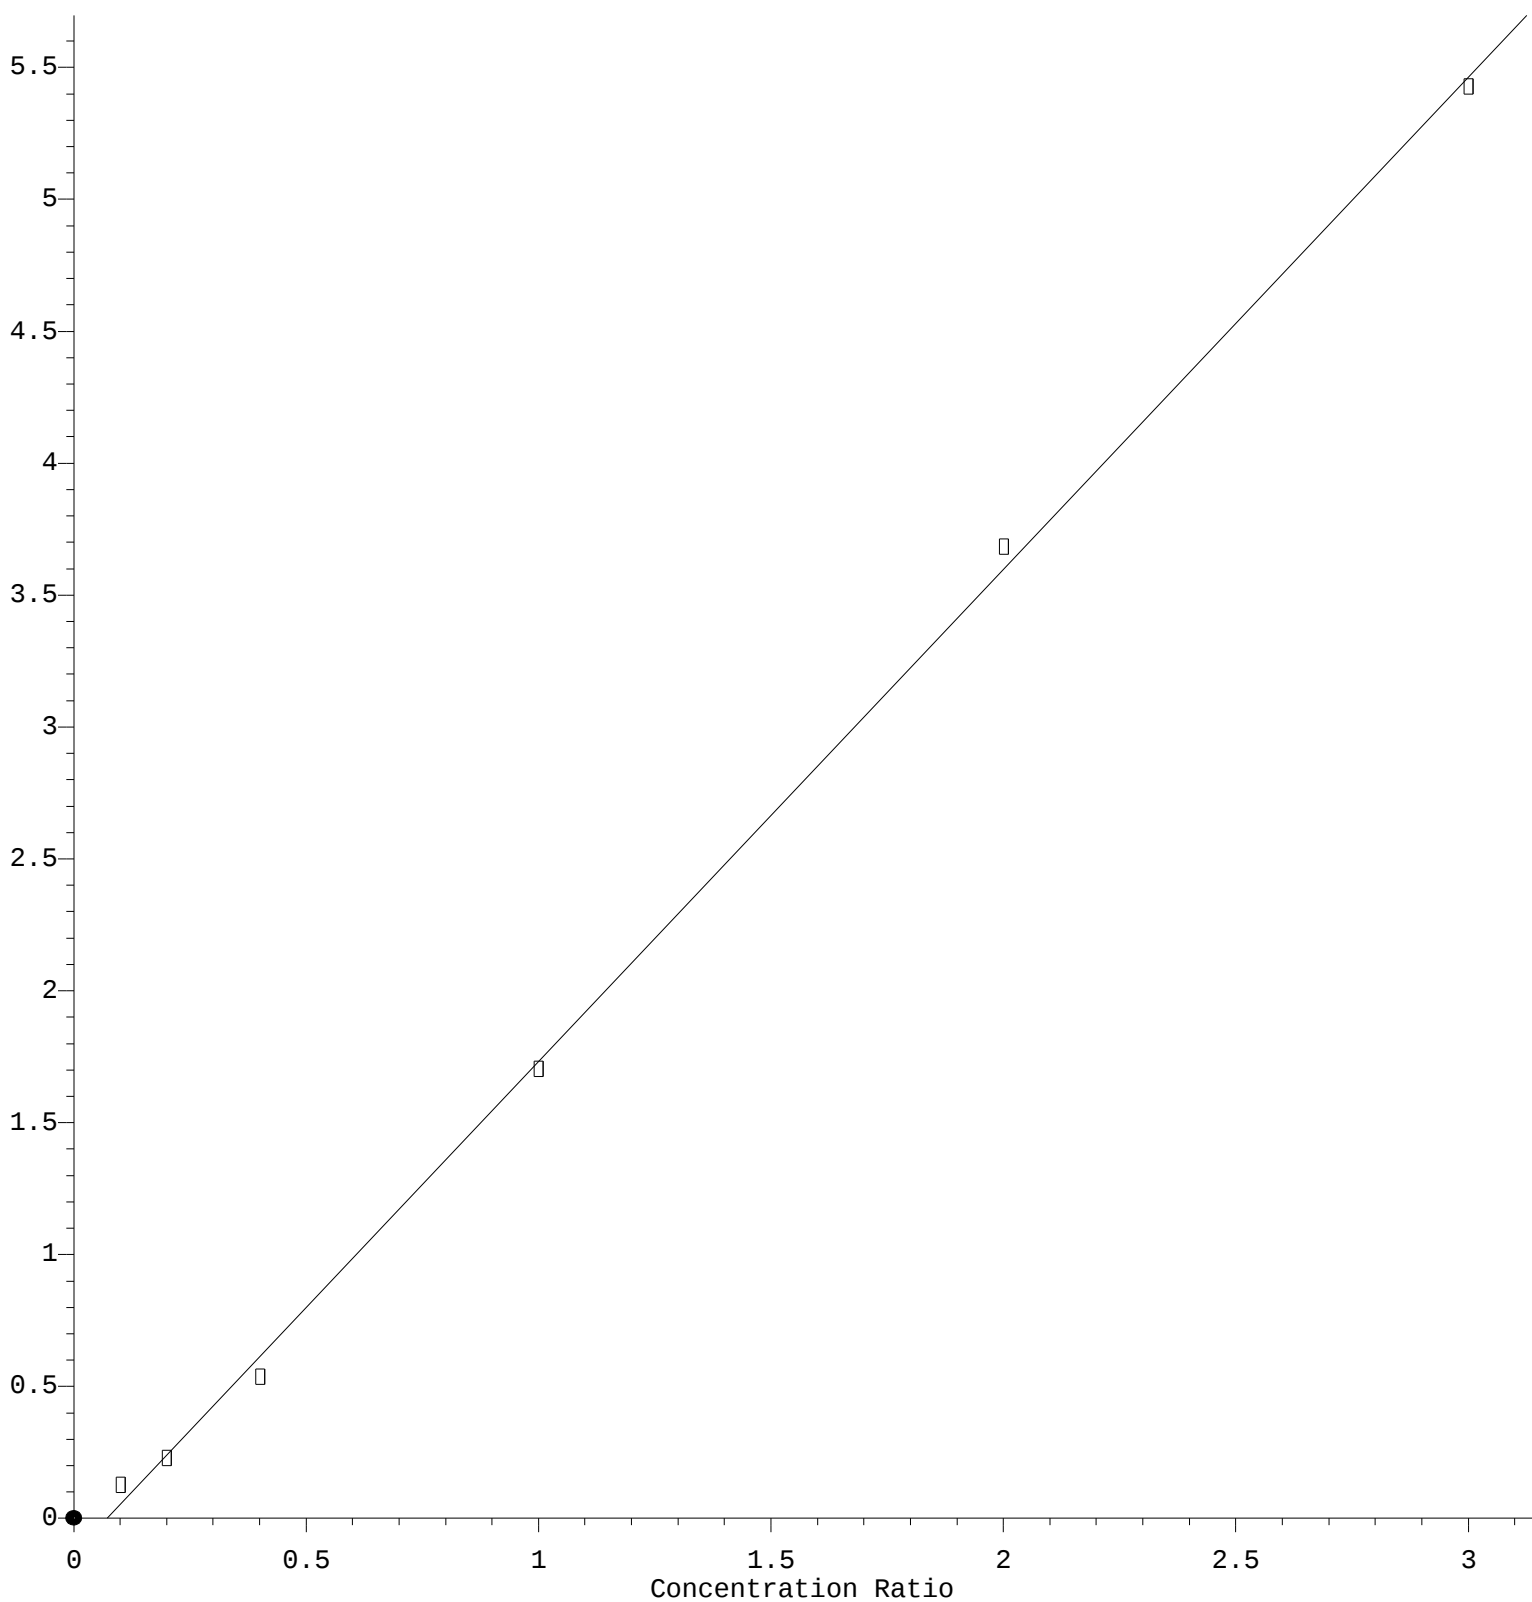

$$\text{Response} = 1.865e+000 * \text{Amt} - 1.332e-001$$

Coef of Det (r^2) = 0.999109 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M

Calibration Table Last Updated: Fri Jun 11 12:50:13 2021