
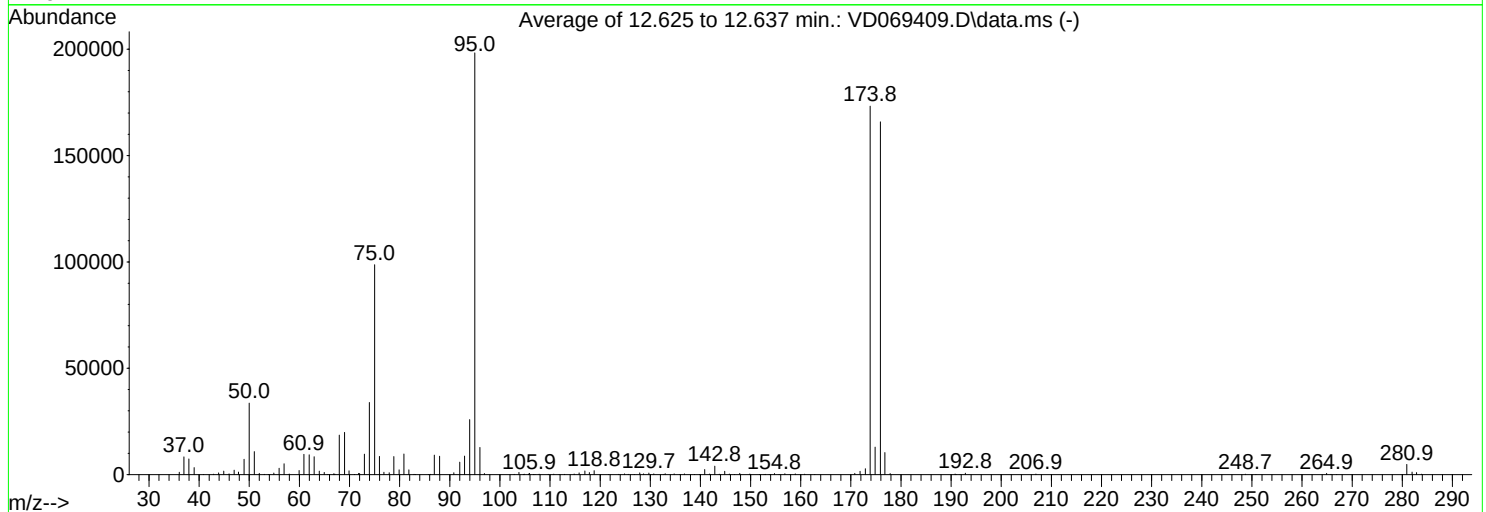


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061121\
Data File : VD069409.D
Acq On : 11 Jun 2021 09:01
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M
Title : SW846 8260
Last Update : Fri Jun 11 12:50:13 2021

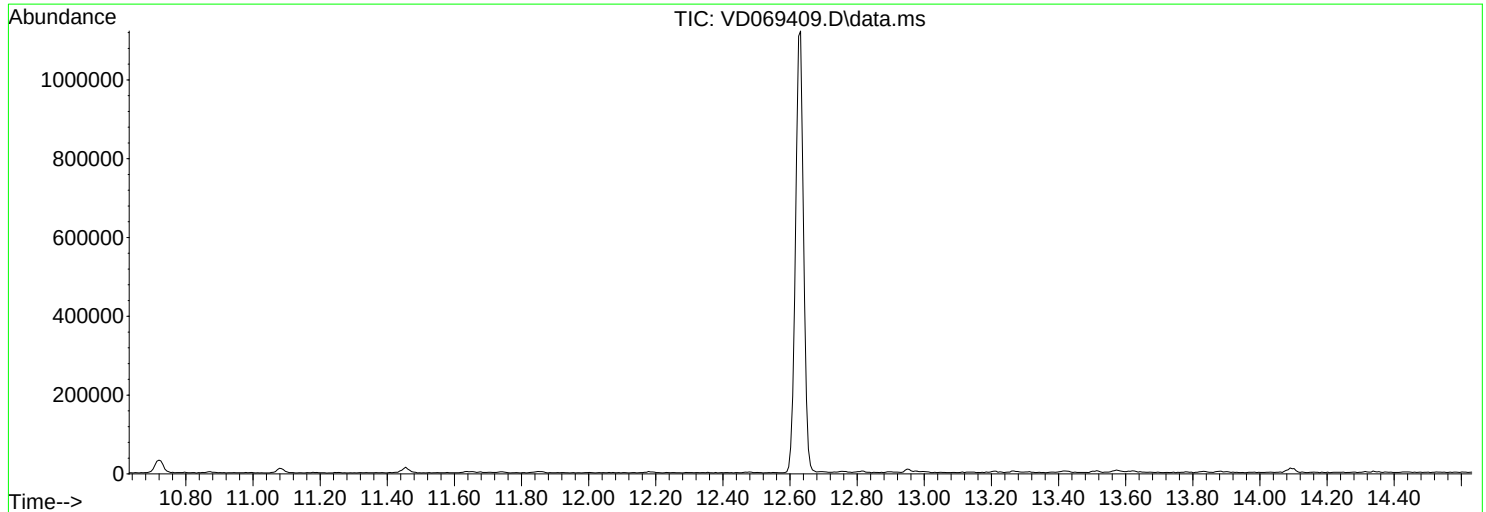

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	33600	PASS
75	95	30	60	49.8	98672	PASS
95	95	100	100	100.0	198293	PASS
96	95	5	9	6.5	12828	PASS
173	174	0.00	2	1.6	2755	PASS
174	95	50	100	87.4	173227	PASS
175	174	5	9	7.5	12957	PASS
176	174	95	101	95.7	165845	PASS
177	176	5	9	6.3	10400	PASS