


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD061220\
 Data File : VD065786.D
 Acq On : 12 Jun 2020 09:29
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060520S.M
 Title : SW846 8260
 Last Update : Fri Jun 05 13:07:30 2020

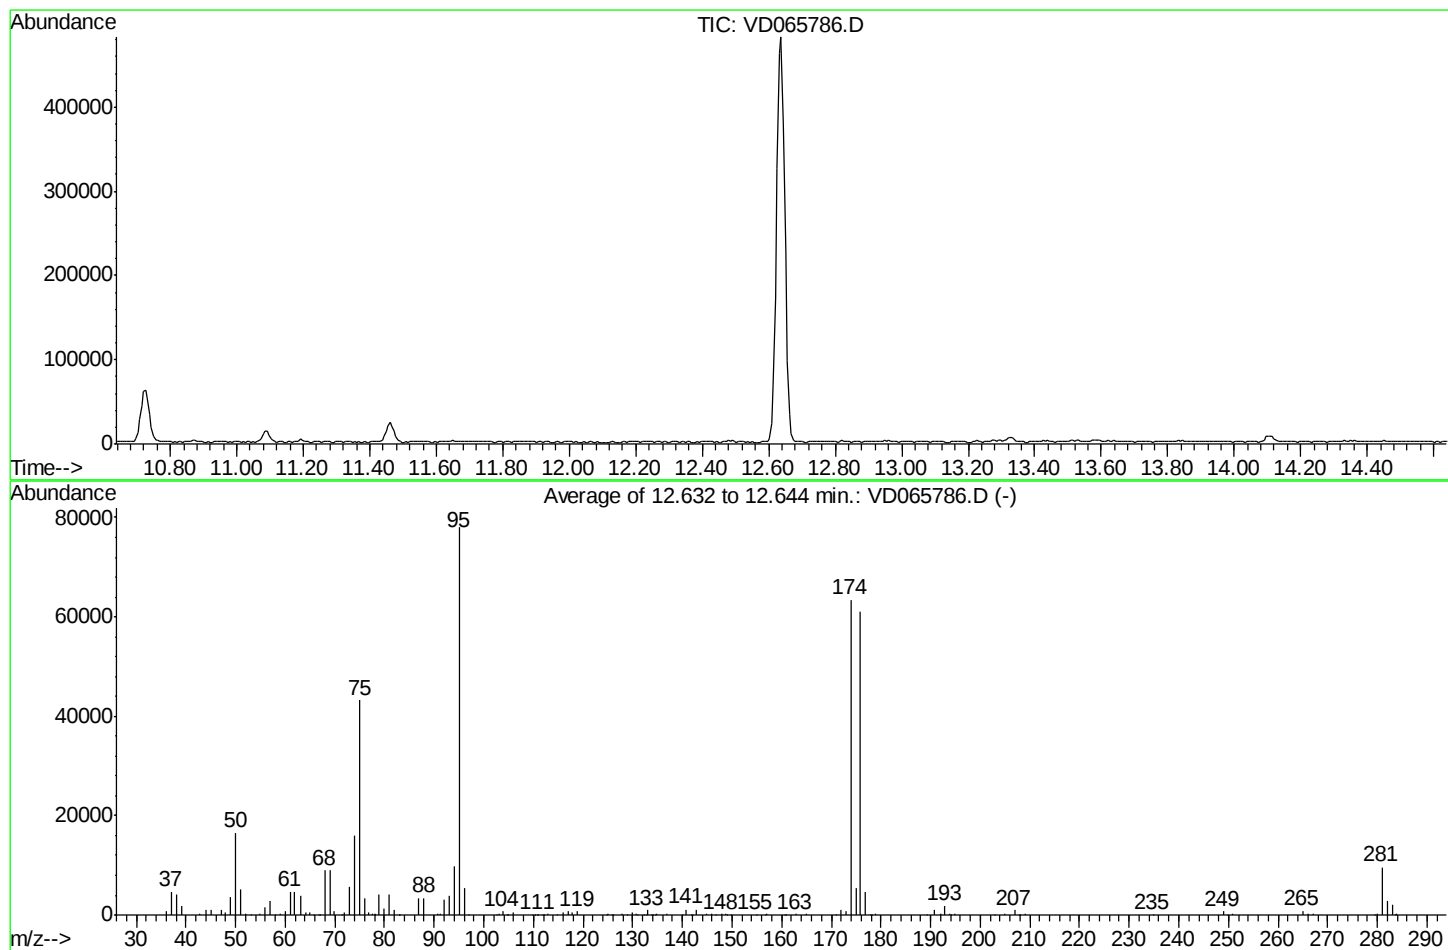

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	16488	PASS
75	95	30	60	55.4	43184	PASS
95	95	100	100	100.0	78013	PASS
96	95	5	9	6.8	5325	PASS
173	174	0.00	2	1.2	741	PASS
174	95	50	100	81.2	63378	PASS
175	174	5	9	8.7	5497	PASS
176	174	95	101	96.4	61088	PASS
177	176	5	9	7.6	4628	PASS