
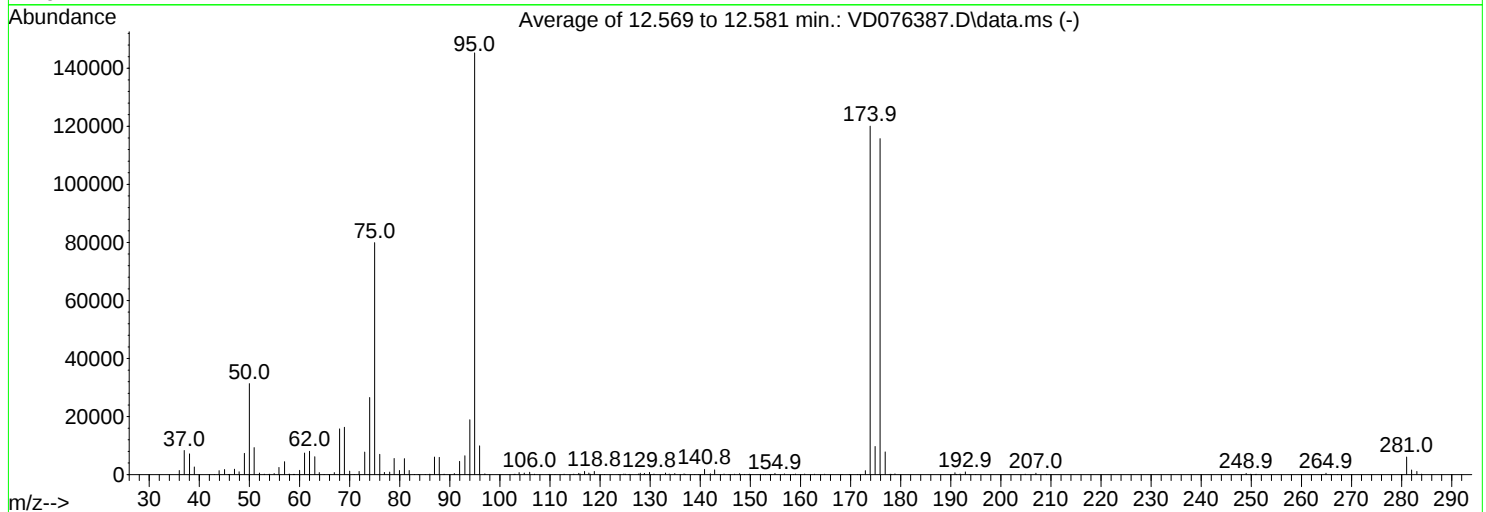


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061223\
Data File : VD076387.D
Acq On : 12 Jun 2023 11:17
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061223S.M
Title : SW846 8260
Last Update : Tue Jun 13 02:01:34 2023

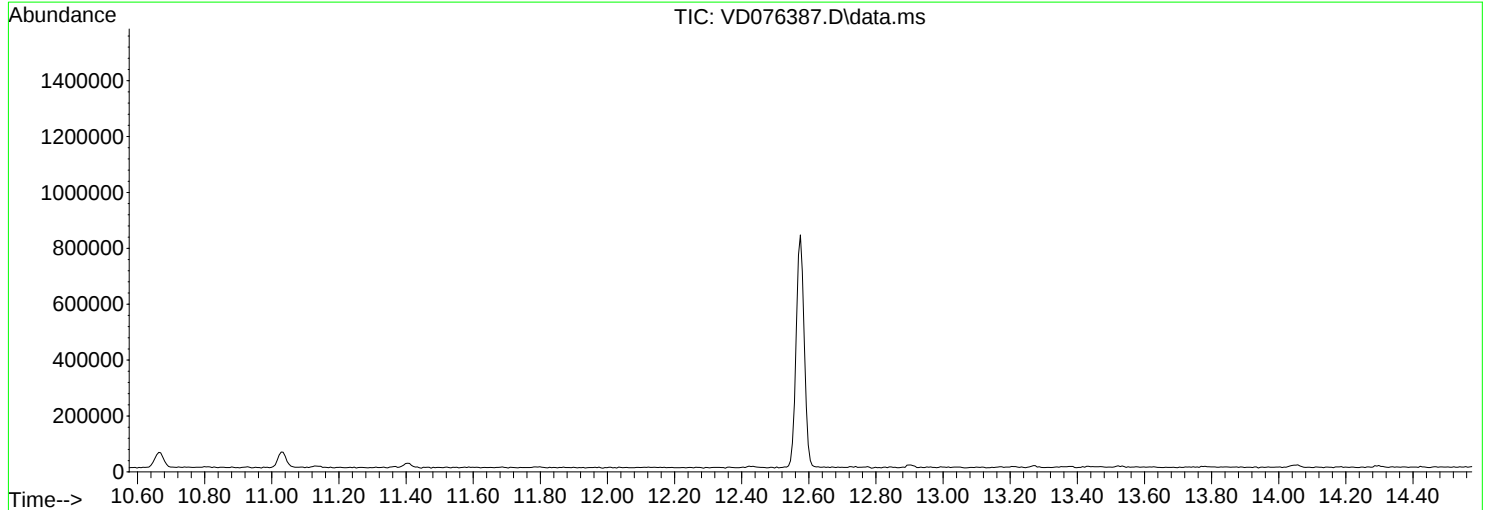

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	31397	PASS
75	95	30	60	55.0	79949	PASS
95	95	100	100	100.0	145314	PASS
96	95	5	9	6.8	9918	PASS
173	174	0.00	2	1.1	1377	PASS
174	95	50	100	82.6	120056	PASS
175	174	5	9	8.1	9680	PASS
176	174	95	101	96.4	115765	PASS
177	176	5	9	6.8	7822	PASS