

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061322\
 Data File : VD073546.D
 Acq On : 13 Jun 2022 15:13
 Operator : VA/SY
 Sample : N3234-01RE
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 RB-21499RE

Quant Time: Jun 14 01:28:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 09 12:33:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	30428	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	50667	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.637	117	68136	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	35526	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	24995	76.547	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	153.100%
35) Dibromofluoromethane	7.908	113	22518	69.114	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	138.220%
50) Toluene-d8	10.337	98	63748	51.750	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.500%
62) 4-Bromofluorobenzene	12.620	95	30271	67.691	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	135.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061322\
Data File : VD073546.D
Acq On : 13 Jun 2022 15:13
Operator : VA/SY
Sample : N3234-01RE
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
RB-21499RE

Quant Time: Jun 14 01:28:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 09 12:33:32 2022
Response via : Initial Calibration




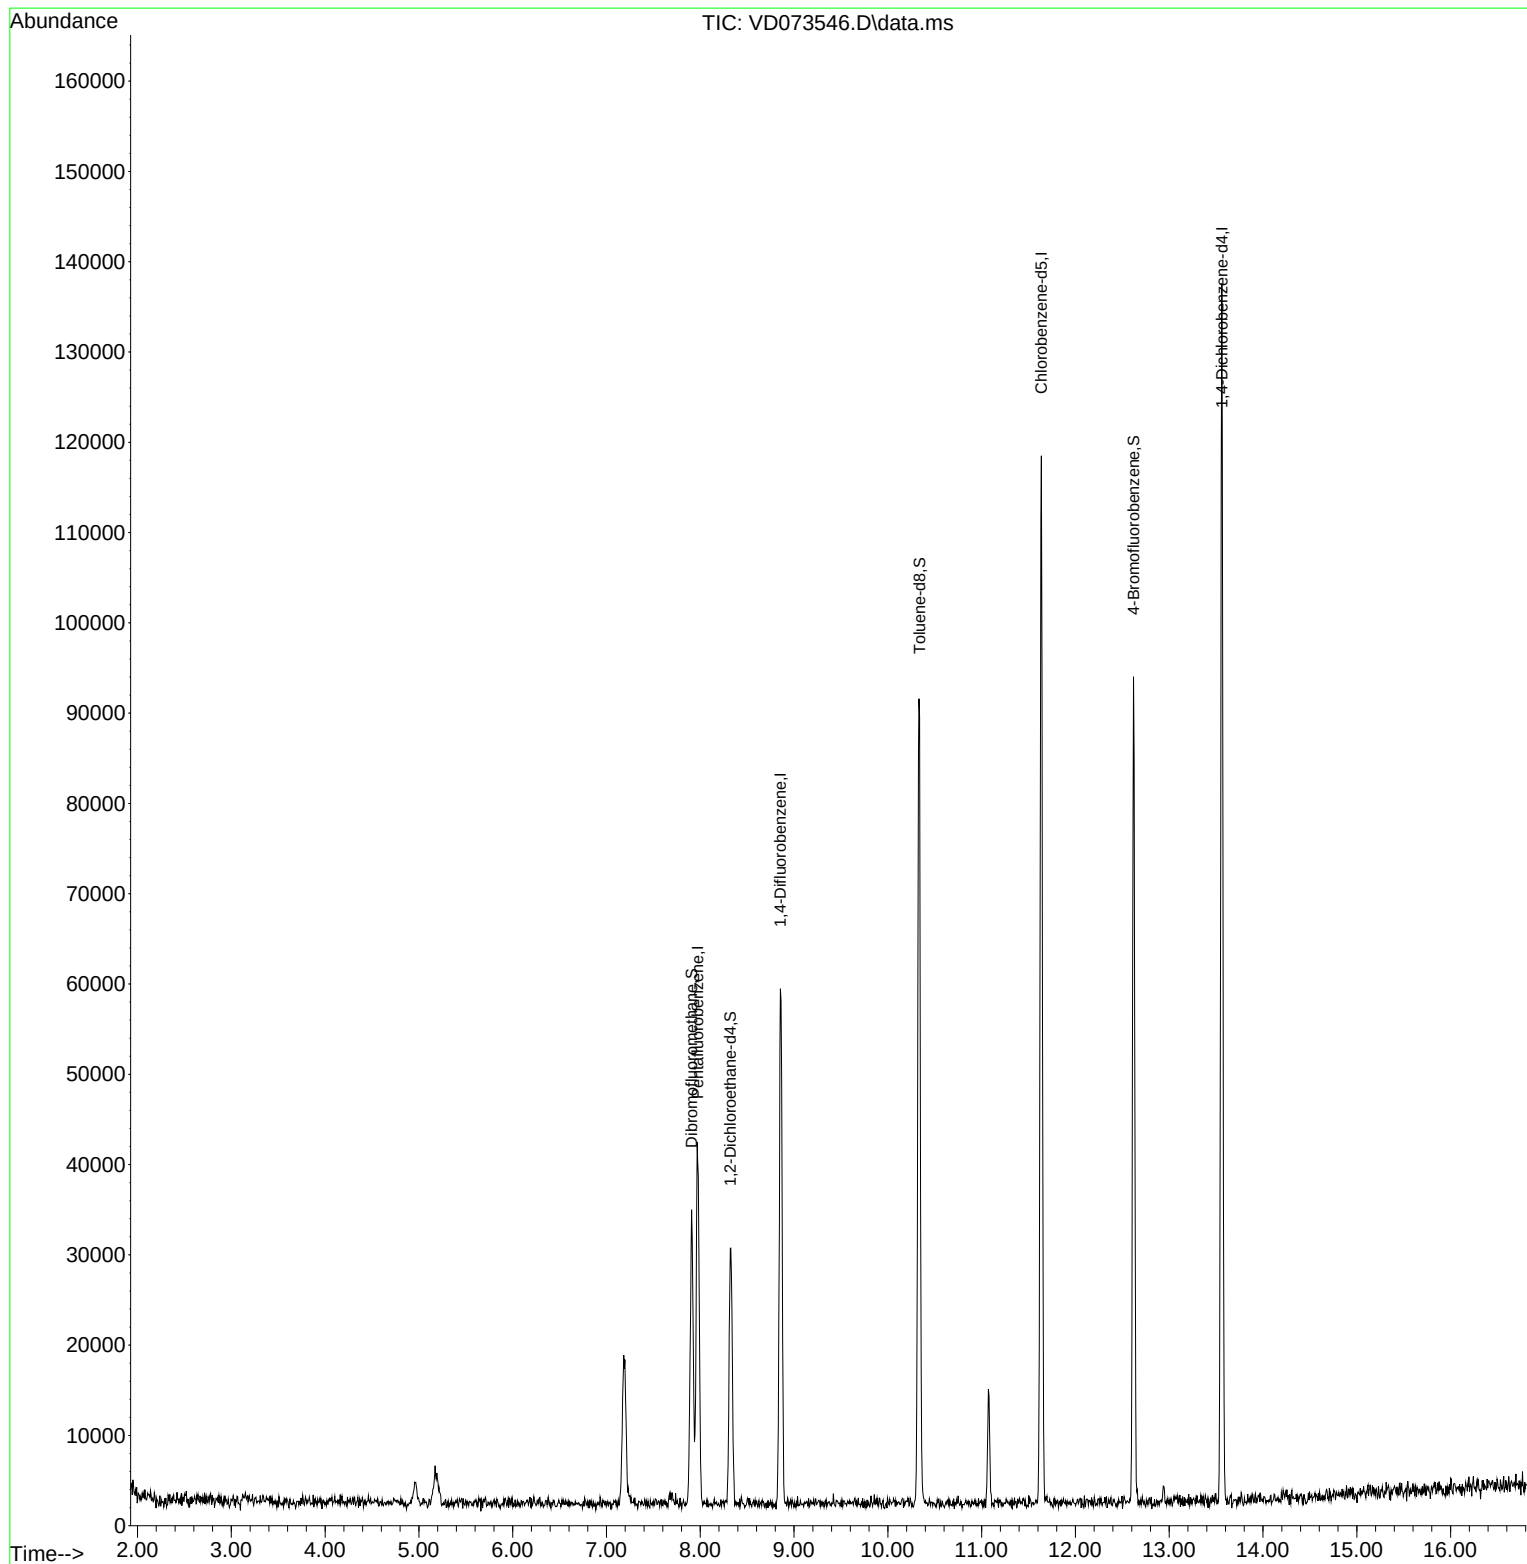


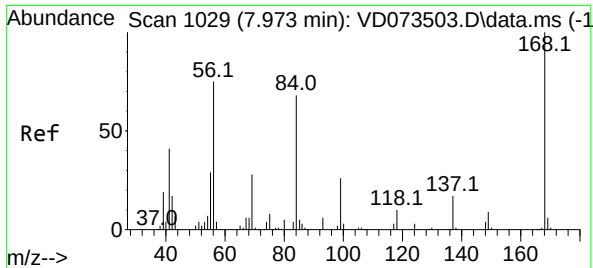

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.000 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13




Instrument :
MSVOA_D
ClientSampleId :
RB-21499RE


Tgt Ion:168 Resp: 30428
Ion Ratio Lower Upper
168 100
99 58.8 49.8 74.6

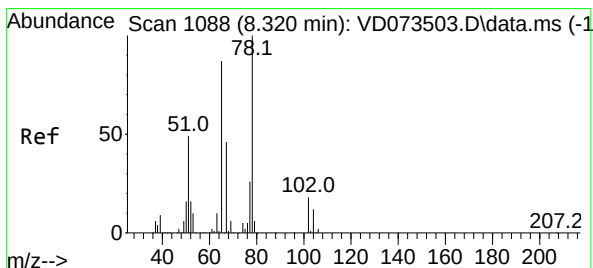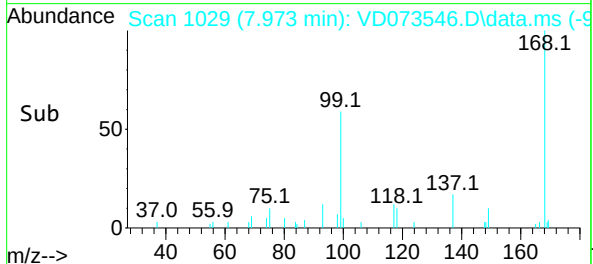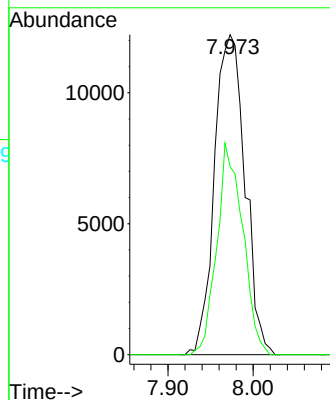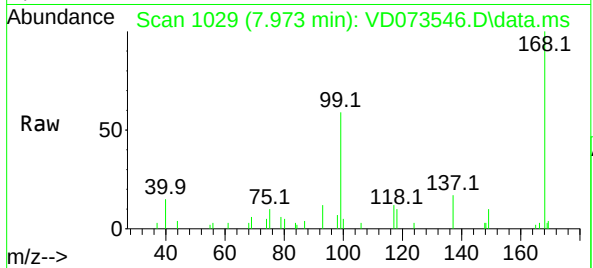

#33
1,2-Dichloroethane-d4
Concen: 76.547 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. -0.000 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13

Tgt Ion: 65 Resp: 24995
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.4

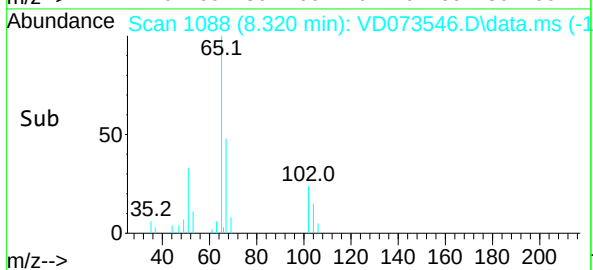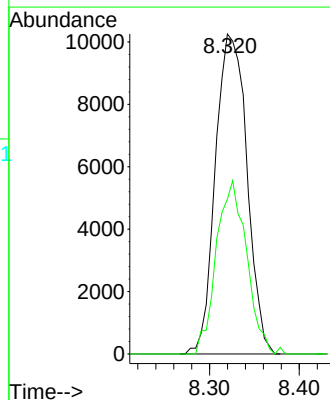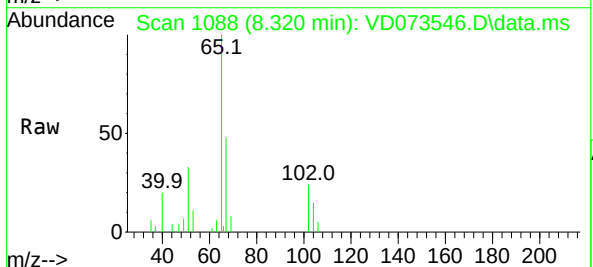

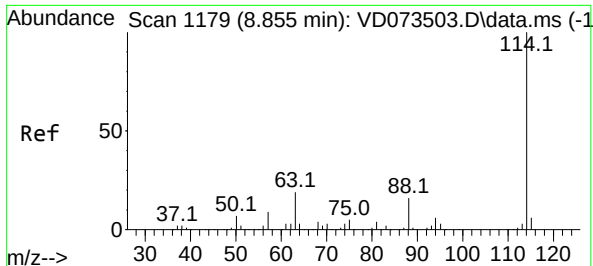

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VD073546.D

Acq: 13 Jun 2022 15:13

Instrument :

MSVOA_D

ClientSampleId :

RB-21499RE





Tgt Ion:114 Resp: 50667

Ion Ratio Lower Upper

114 100

63 18.7 0.0 46.6

88 16.9 0.0 33.2

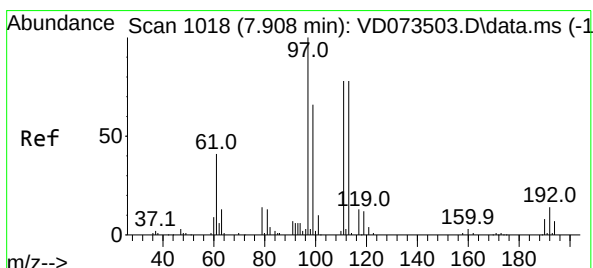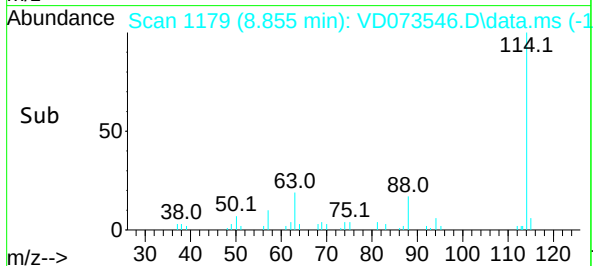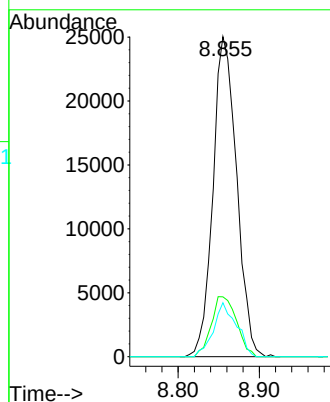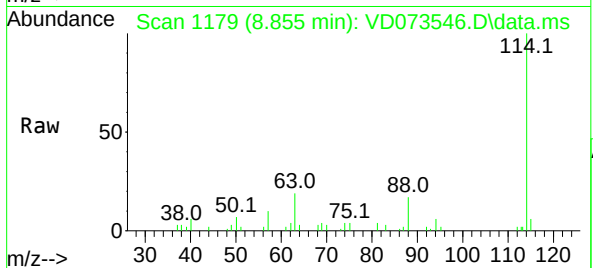

#35

Dibromofluoromethane

Concen: 69.114 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. 0.000 min

Lab File: VD073546.D

Acq: 13 Jun 2022 15:13




Tgt Ion:113 Resp: 22518


Ion Ratio Lower Upper

113 100

111 100.4 83.8 125.6

192 18.7 14.6 21.8


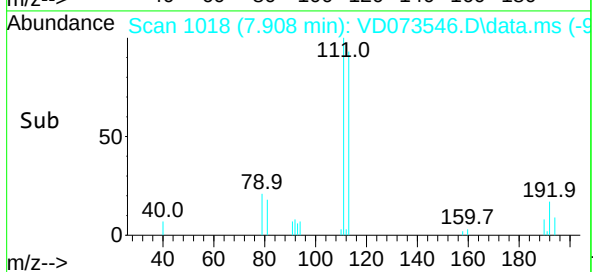
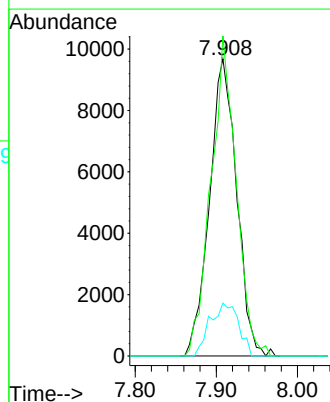
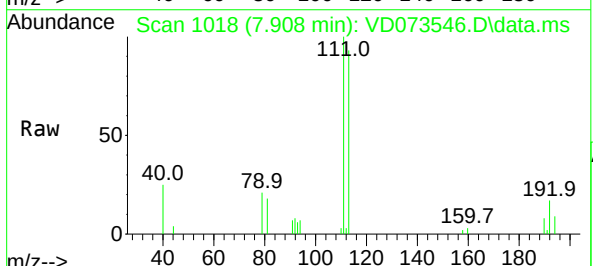


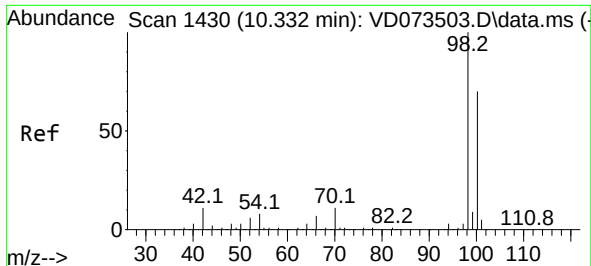

#50
Toluene-d8
Concen: 51.750 ug/l
RT: 10.337 min Scan# 1430
Delta R.T. 0.005 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13




Instrument :
MSVOA_D
ClientSampleId :
RB-21499RE


Tgt Ion: 98 Resp: 63748
Ion Ratio Lower Upper
98 100
100 67.2 52.4 78.6

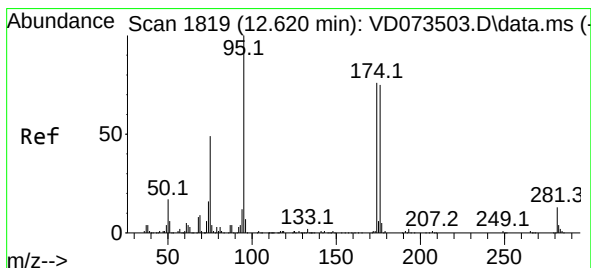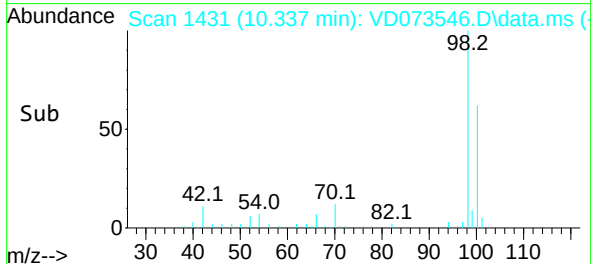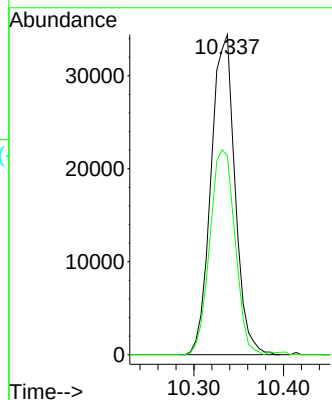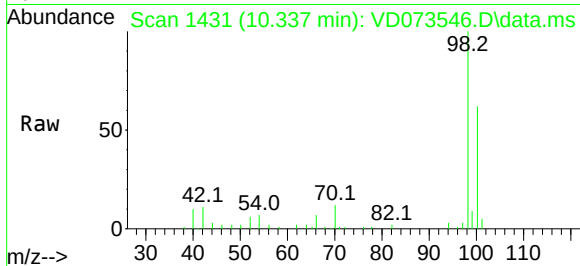

#62
4-Bromofluorobenzene
Concen: 67.691 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13

Tgt Ion: 95 Resp: 30271
Ion Ratio Lower Upper
95 100
174 82.7 0.0 152.8
176 77.5 0.0 145.4


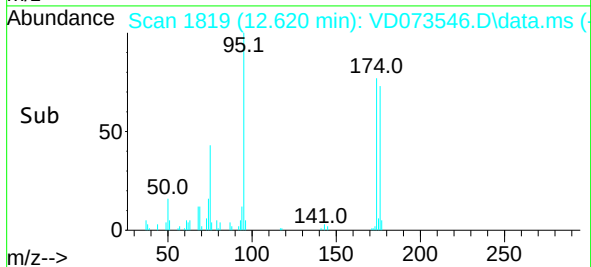
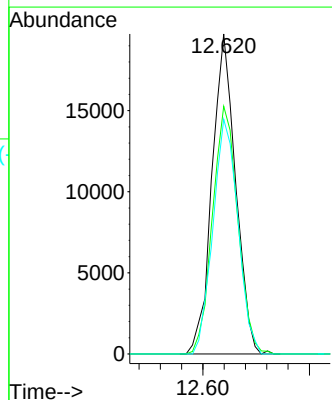
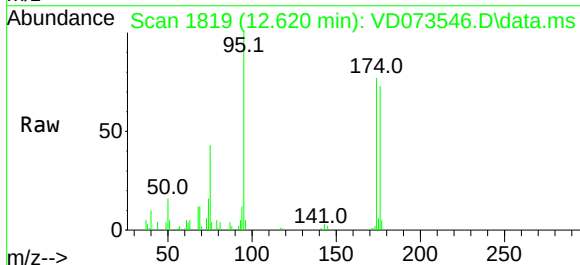


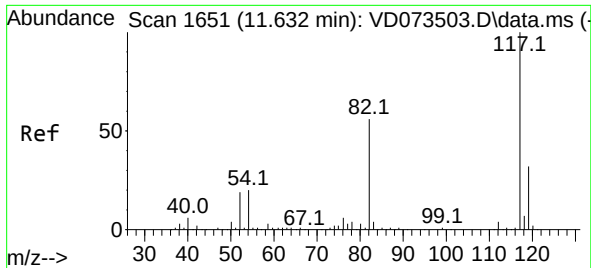

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.637 min Scan# 117
Delta R.T. 0.005 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13

Instrument :
MSVOA_D
ClientSampleId :
RB-21499RE

Tgt Ion:117 Resp: 68136
Ion Ratio Lower Upper
117 100
82 51.9 45.3 67.9
119 35.4 26.6 40.0

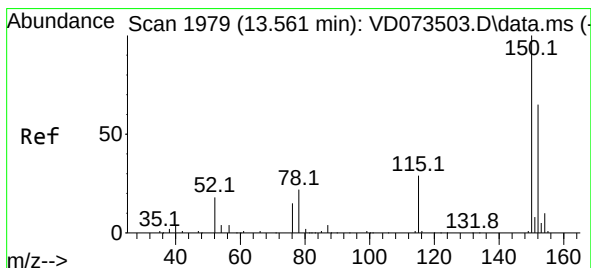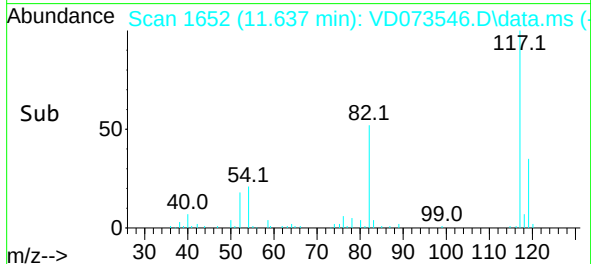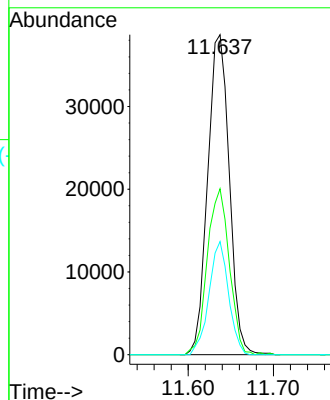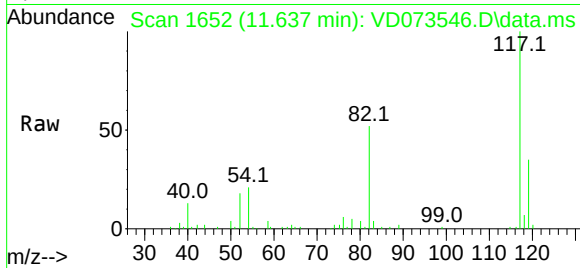

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.000 min
Lab File: VD073546.D
Acq: 13 Jun 2022 15:13

Tgt Ion:152 Resp: 35526
Ion Ratio Lower Upper
152 100
115 59.3 31.3 93.8
150 157.8 0.0 348.6

