
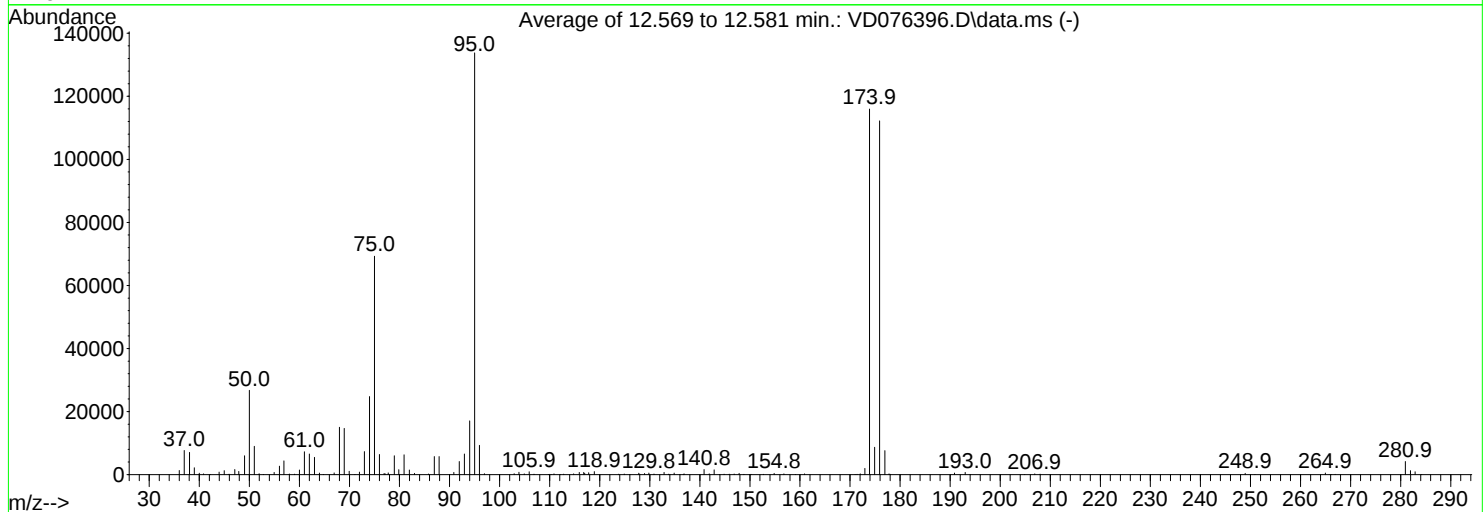


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061323\
Data File : VD076396.D
Acq On : 13 Jun 2023 09:35
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061223S.M
Title : SW846 8260
Last Update : Tue Jun 13 02:01:34 2023

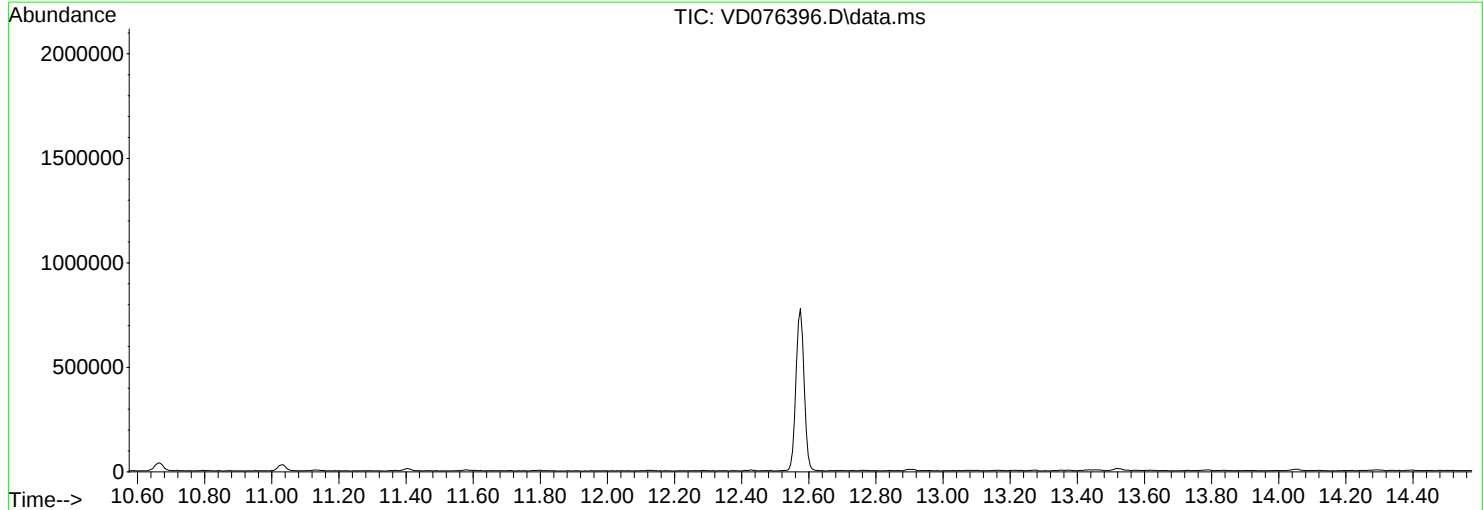

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	26733	PASS
75	95	30	60	51.8	69283	PASS
95	95	100	100	100.0	133784	PASS
96	95	5	9	6.9	9267	PASS
173	174	0.00	2	1.7	2006	PASS
174	95	50	100	86.7	115947	PASS
175	174	5	9	7.5	8661	PASS
176	174	95	101	96.8	112208	PASS
177	176	5	9	6.8	7624	PASS