
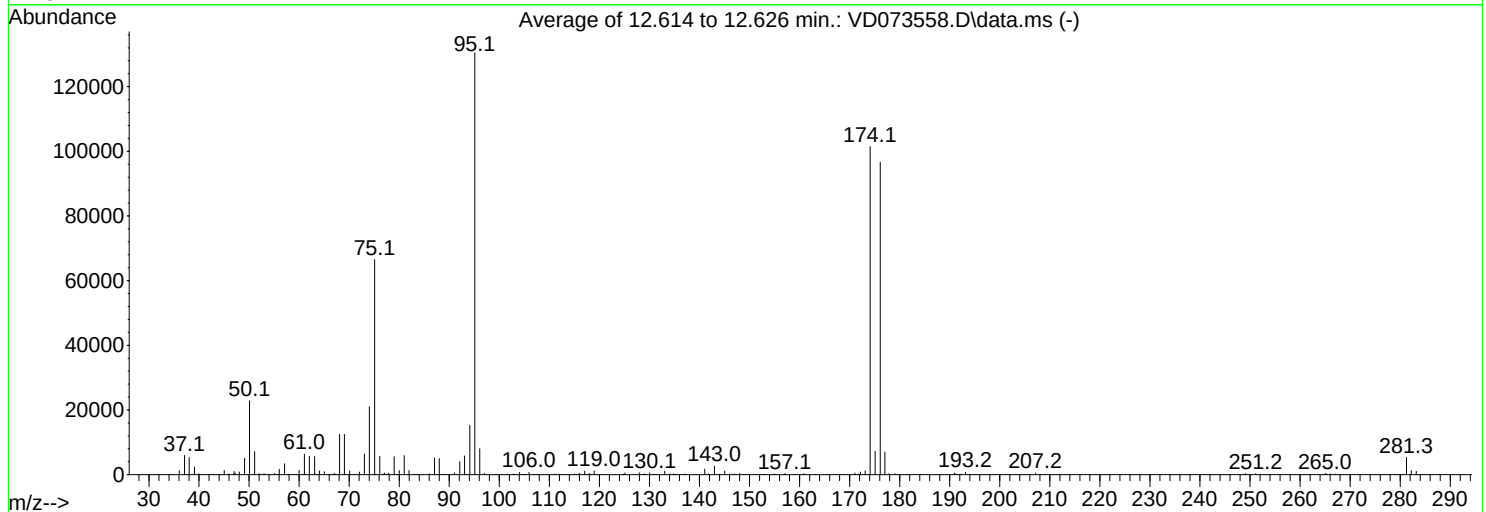


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061422\
Data File : VD073558.D
Acq On : 14 Jun 2022 09:07
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
Title : SW846 8260
Last Update : Thu Jun 09 12:33:32 2022

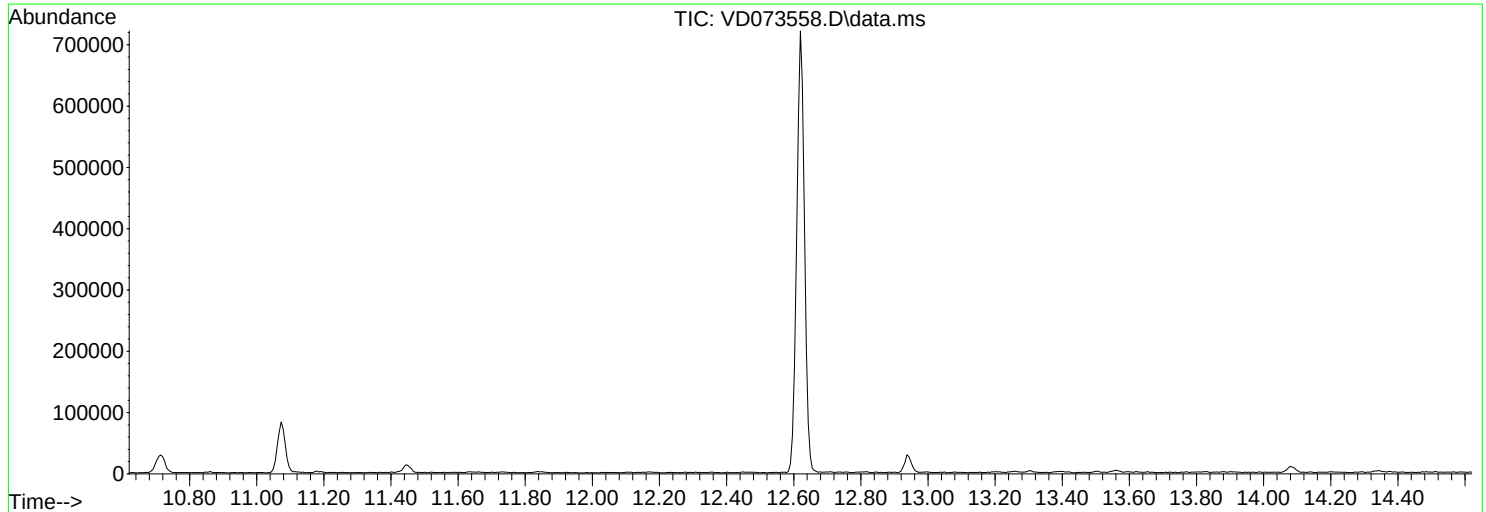

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	22835	PASS
75	95	30	60	51.0	66504	PASS
95	95	100	100	100.0	130459	PASS
96	95	5	9	6.1	8021	PASS
173	174	0.00	2	1.2	1185	PASS
174	95	50	100	77.7	101429	PASS
175	174	5	9	7.1	7210	PASS
176	174	95	101	95.3	96640	PASS
177	176	5	9	7.2	6977	PASS