
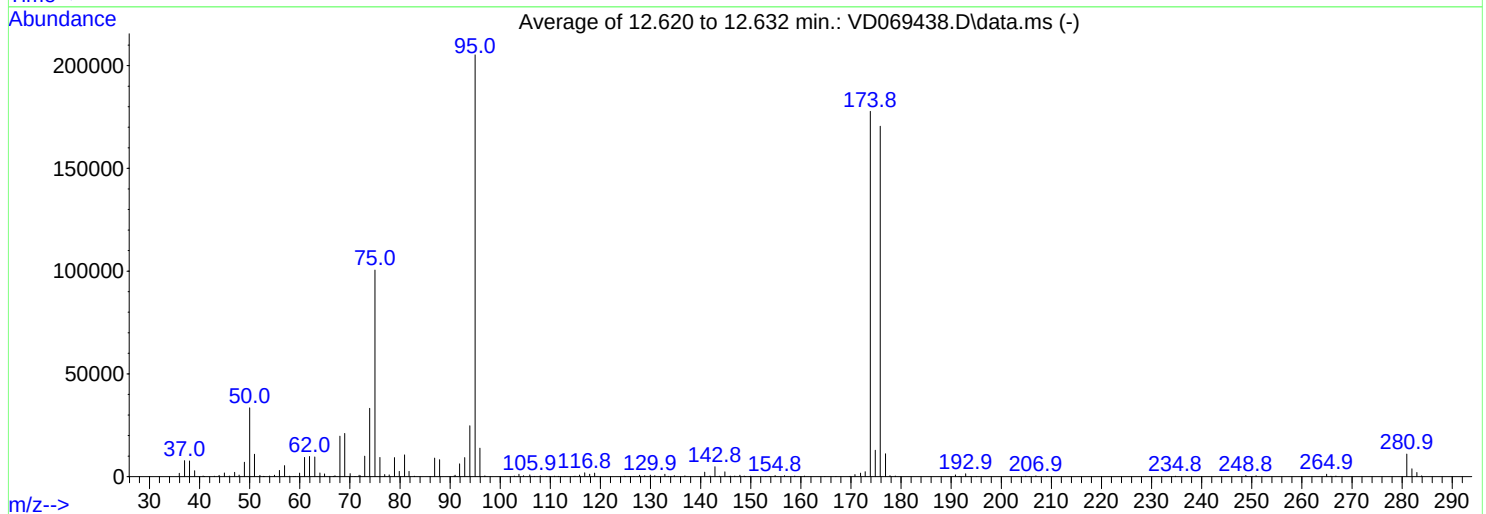


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061521\
Data File : VD069438.D
Acq On : 15 Jun 2021 10:17
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M
Title : SW846 8260
Last Update : Fri Jun 11 12:50:13 2021

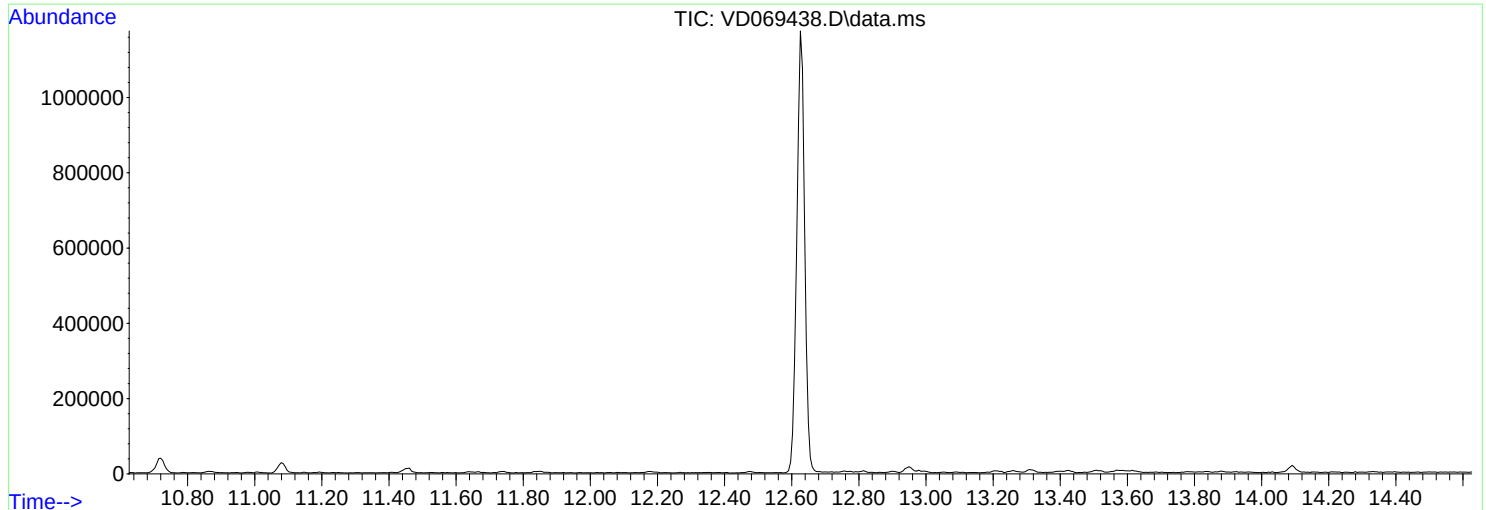

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	33461	PASS
75	95	30	60	49.0	100555	PASS
95	95	100	100	100.0	205248	PASS
96	95	5	9	6.8	13887	PASS
173	174	0.00	2	1.4	2406	PASS
174	95	50	100	86.6	177749	PASS
175	174	5	9	7.2	12853	PASS
176	174	95	101	95.9	170496	PASS
177	176	5	9	6.5	11144	PASS