

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD061522\  
 Data File : VD073583.D  
 Acq On : 15 Jun 2022 10:35  
 Operator : VA/SY  
 Sample : VD0615SBL01  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 VD0615SBL01

Quant Time: Jun 16 06:02:03 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D060922S.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Jun 09 12:33:32 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.973  | 168  | 325109   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.855  | 114  | 565632   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.638 | 117  | 535056   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.561 | 152  | 248117   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.320  | 65    | 176243   | 50.516   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 101.040% |
| 35) Dibromofluoromethane    | 7.902  | 113   | 182174   | 50.086   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 100.180% |
| 50) Toluene-d8              | 10.332 | 98    | 668851   | 48.637   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 97.280%  |
| 62) 4-Bromofluorobenzene    | 12.620 | 95    | 227500   | 45.570   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 91.140%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD061522\  
Data File : VD073583.D  
Acq On : 15 Jun 2022 10:35  
Operator : VA/SY  
Sample : VD0615SBL01  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0615SBL01

Quant Time: Jun 16 06:02:03 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D060922S.M  
Quant Title : SW846 8260  
QLast Update : Thu Jun 09 12:33:32 2022  
Response via : Initial Calibration




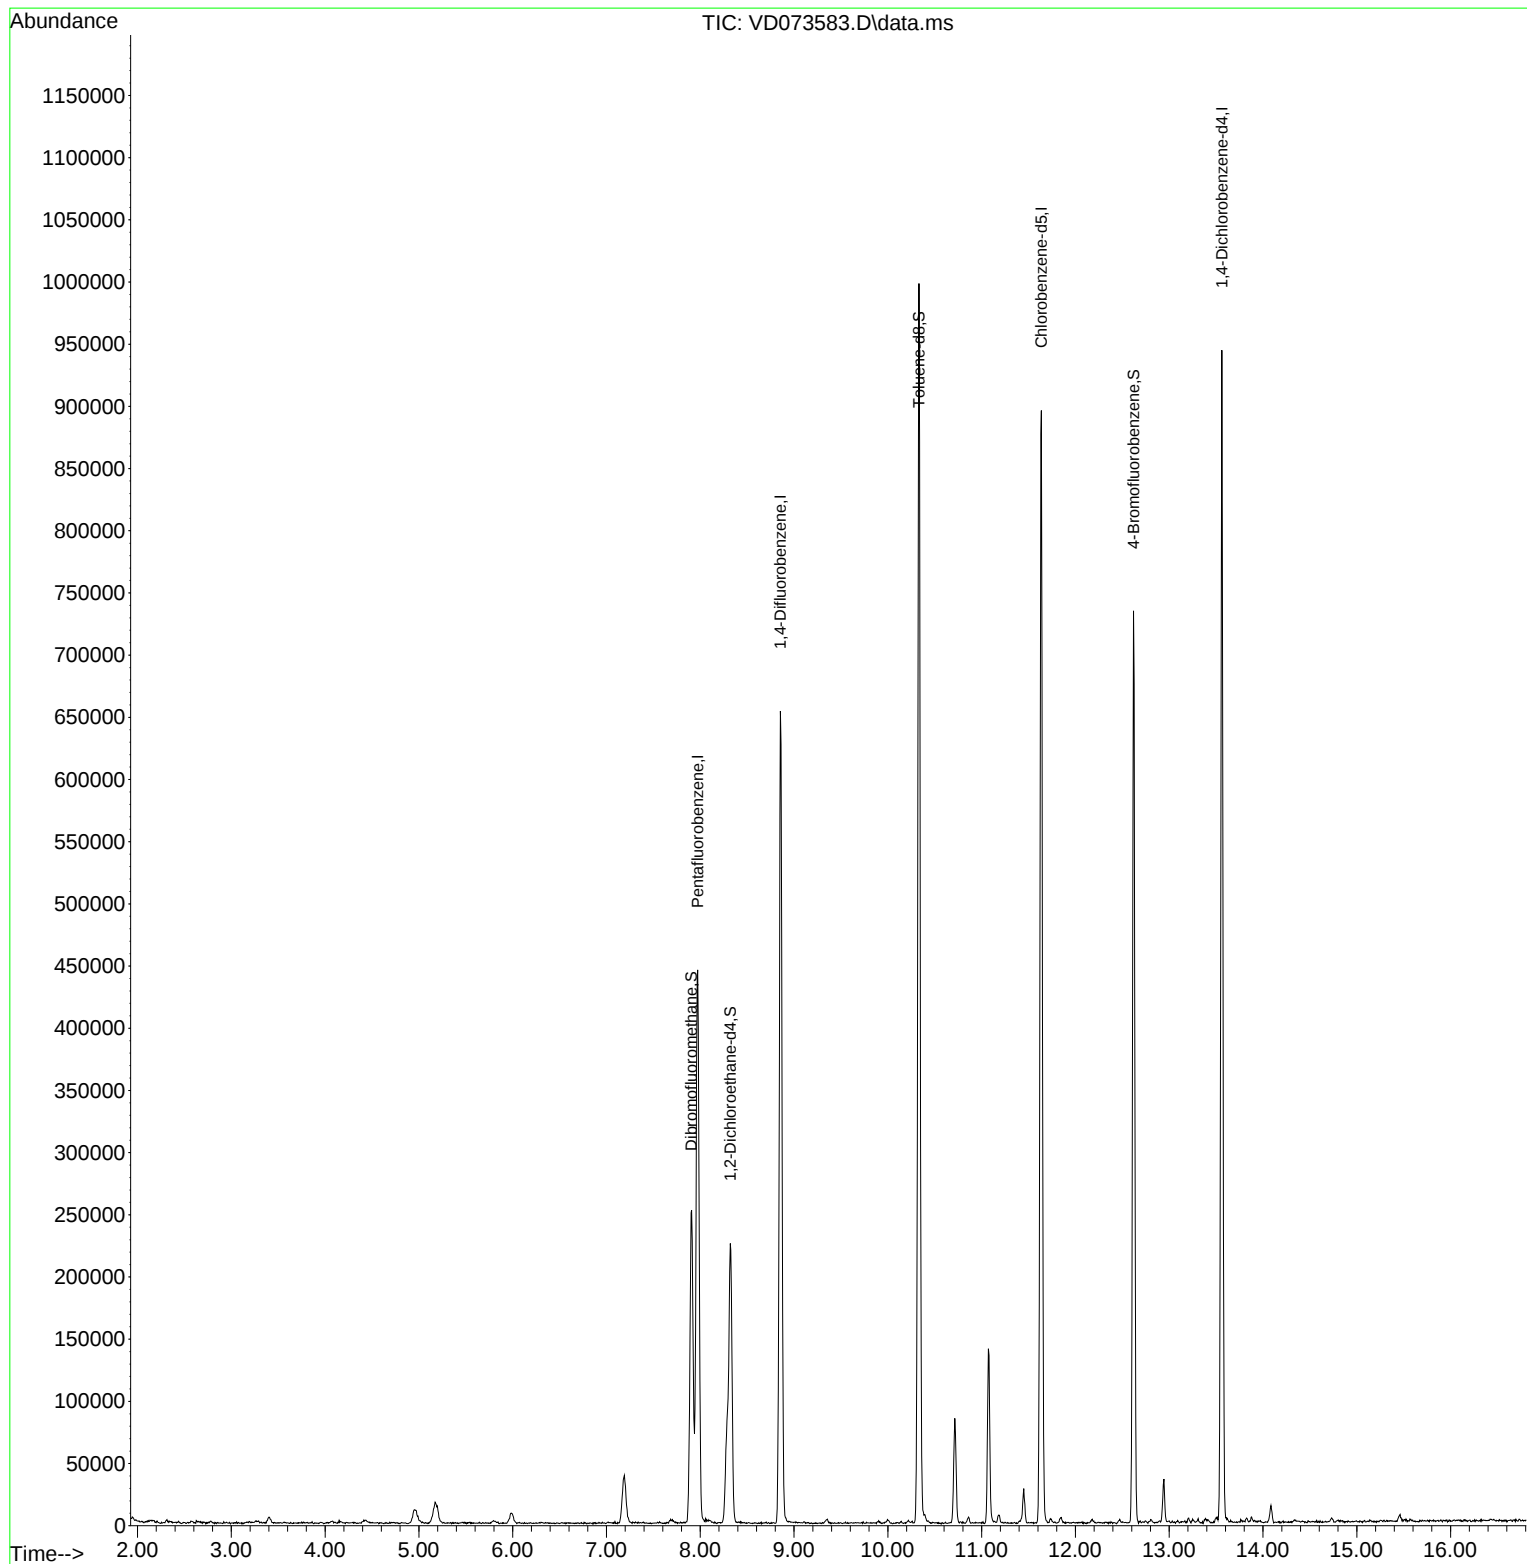


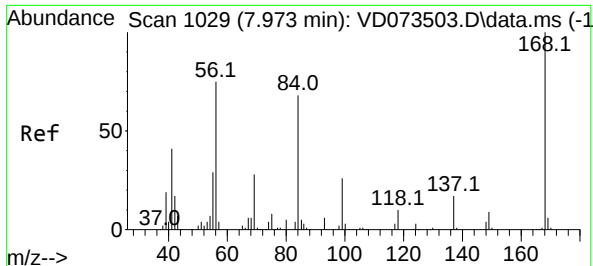

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.973 min Scan# 1029  
Delta R.T. 0.000 min  
Lab File: VD073583.D  
Acq: 15 Jun 2022 10:35




Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0615SBL01


Tgt Ion:168 Resp: 325109  
Ion Ratio Lower Upper  
168 100  
99 57.5 49.8 74.6

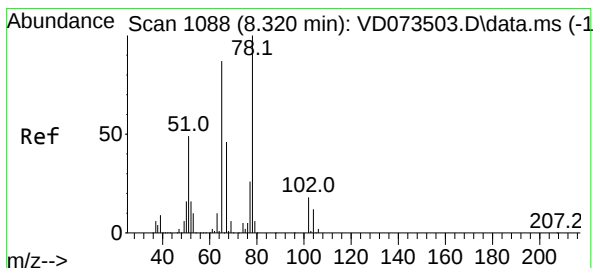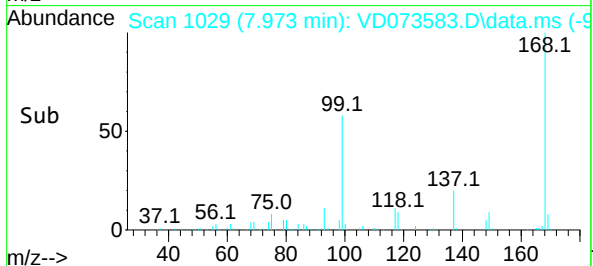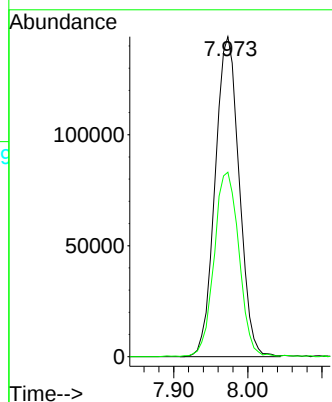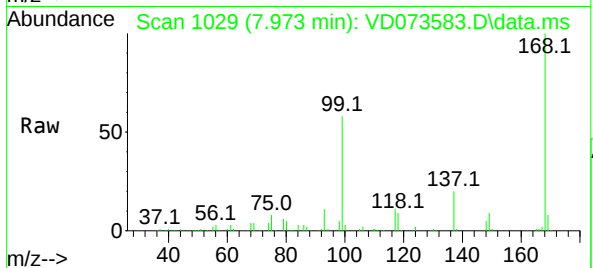

#33  
1,2-Dichloroethane-d4  
Concen: 50.516 ug/l  
RT: 8.320 min Scan# 1088  
Delta R.T. 0.000 min  
Lab File: VD073583.D  
Acq: 15 Jun 2022 10:35

Tgt Ion: 65 Resp: 176243  
Ion Ratio Lower Upper  
65 100  
67 52.3 0.0 101.4

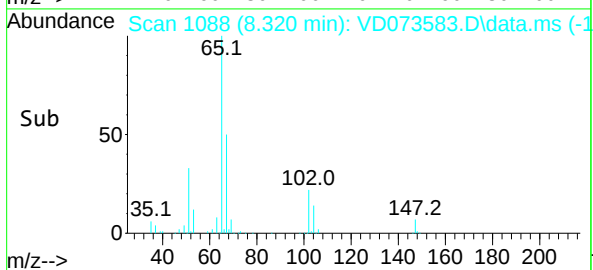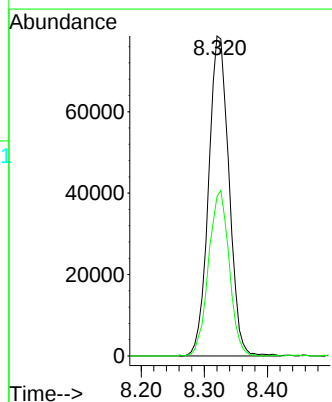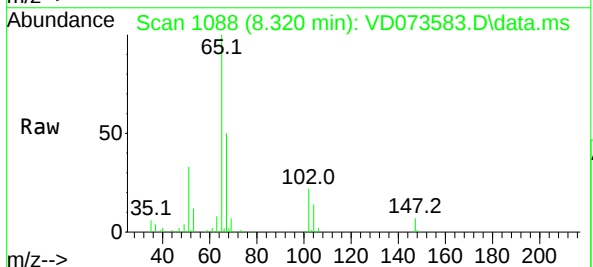

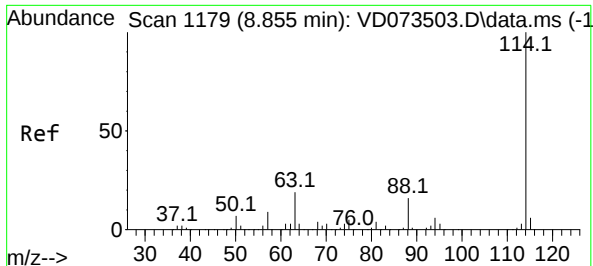

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VD073583.D

Acq: 15 Jun 2022 10:35

Instrument :

MSVOA\_D

ClientSampleId :

VD0615SBL01





Tgt Ion:114 Resp: 565632

Ion Ratio Lower Upper

114 100

63 19.9 0.0 46.6

88 14.3 0.0 33.2

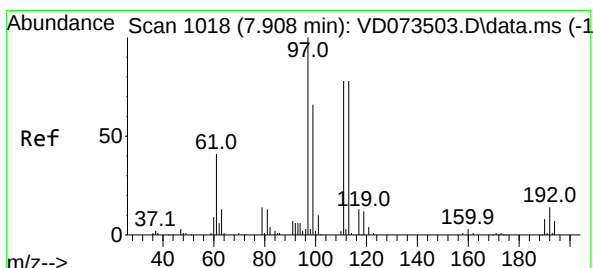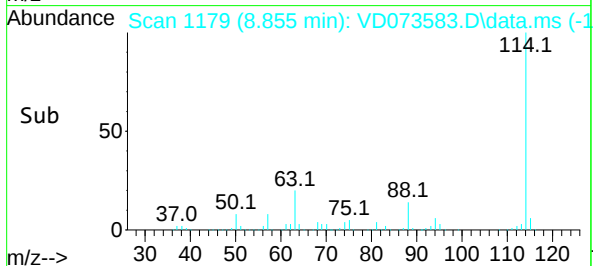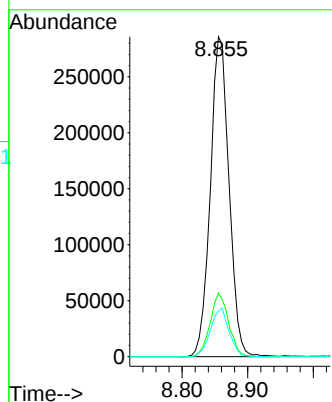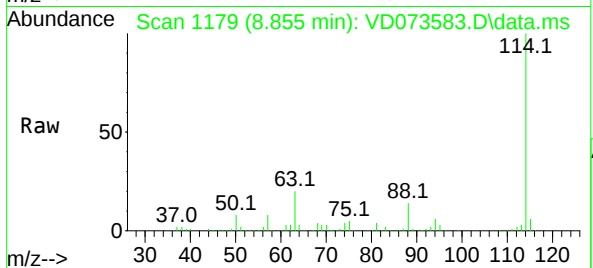

#35

Dibromofluoromethane

Concen: 50.086 ug/l

RT: 7.902 min Scan# 1017

Delta R.T. -0.006 min

Lab File: VD073583.D

Acq: 15 Jun 2022 10:35




Tgt Ion:113 Resp: 182174


Ion Ratio Lower Upper

113 100

111 103.6 83.8 125.6

192 19.0 14.6 21.8

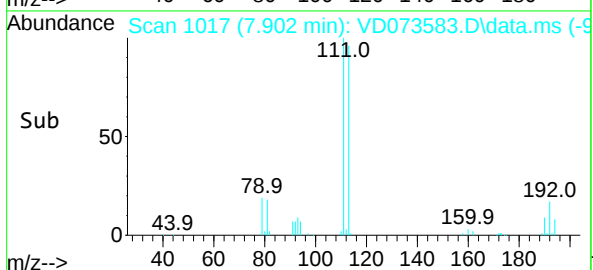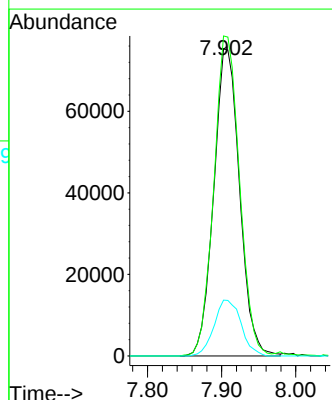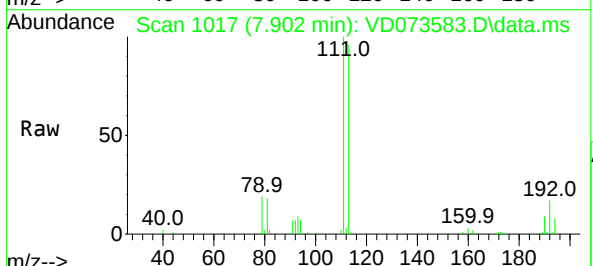

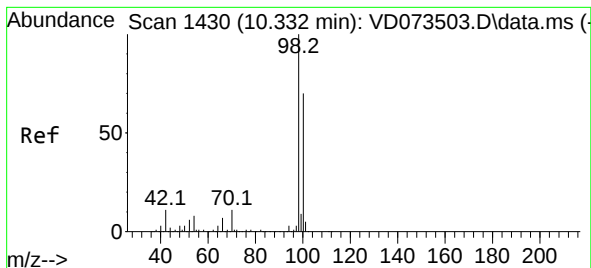

#50

Toluene-d8

Concen: 48.637 ug/l

RT: 10.332 min Scan# 1430

Delta R.T. -0.000 min

Lab File: VD073583.D

Acq: 15 Jun 2022 10:35

Instrument :

MSVOA\_D

ClientSampleId :





VD0615SBL01

Tgt Ion: 98 Resp: 668851

Ion Ratio Lower Upper

98 100

100 65.9 52.4 78.6

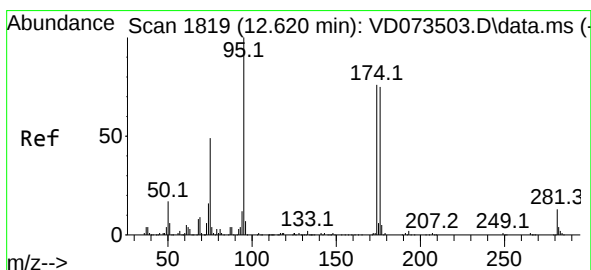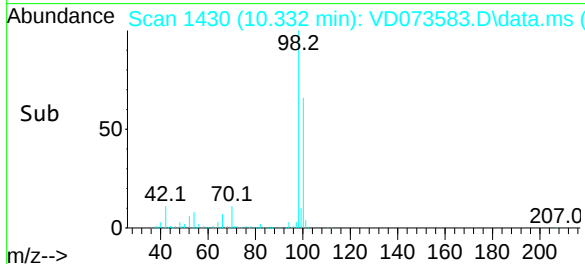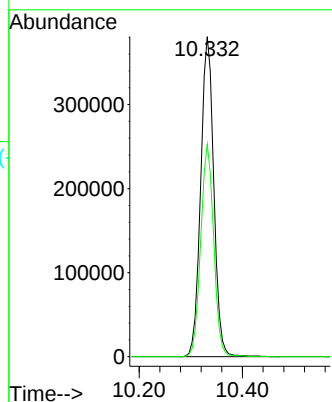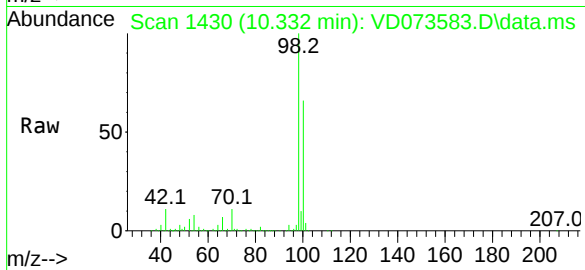

#62

4-Bromofluorobenzene

Concen: 45.570 ug/l

RT: 12.620 min Scan# 1819

Delta R.T. -0.000 min

Lab File: VD073583.D

Acq: 15 Jun 2022 10:35




Tgt Ion: 95 Resp: 227500


Ion Ratio Lower Upper

95 100

174 81.1 0.0 152.8

176 75.6 0.0 145.4


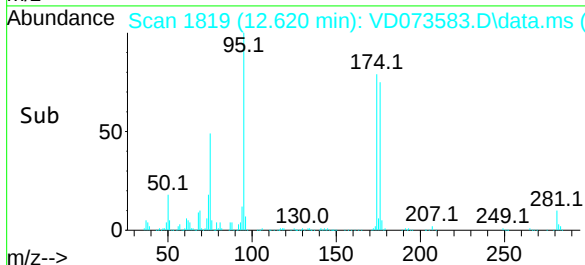
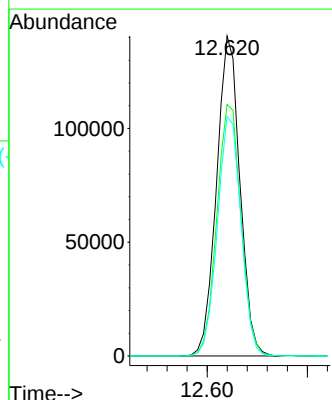
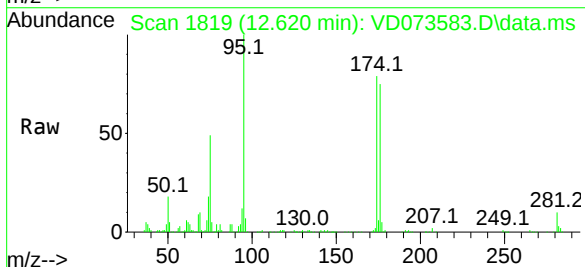


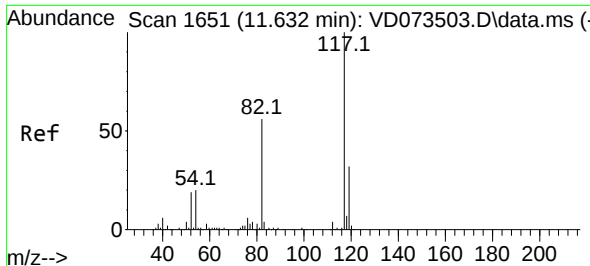

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.638 min Scan# 117  
Delta R.T. 0.006 min  
Lab File: VD073583.D  
Acq: 15 Jun 2022 10:35

Instrument :  
MSVOA\_D  
ClientSampleId :  
VD0615SBL01

Tgt Ion:117 Resp: 535056  
Ion Ratio Lower Upper  
117 100  
82 53.2 45.3 67.9  
119 33.5 26.6 40.0

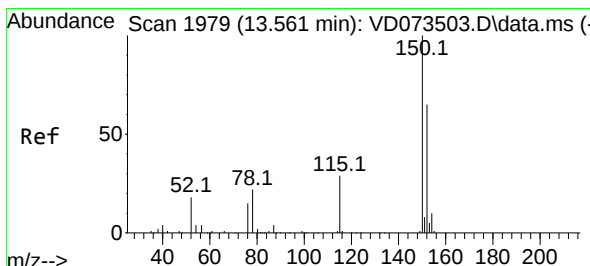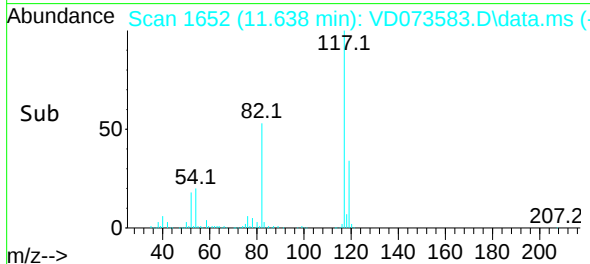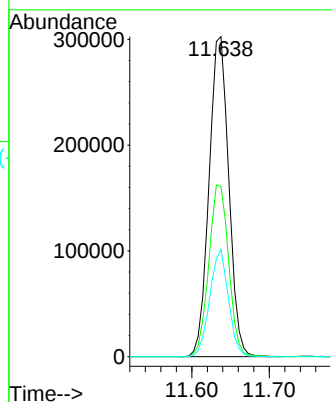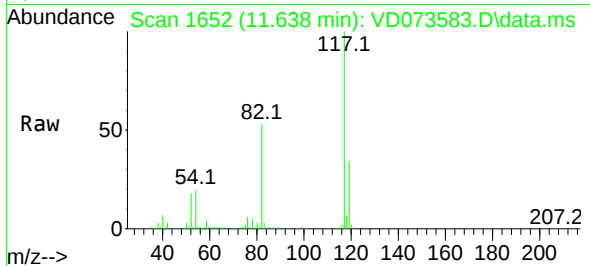

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.561 min Scan# 1979  
Delta R.T. 0.000 min  
Lab File: VD073583.D  
Acq: 15 Jun 2022 10:35

Tgt Ion:152 Resp: 248117  
Ion Ratio Lower Upper  
152 100  
115 59.2 31.3 93.8  
150 155.5 0.0 348.6

