
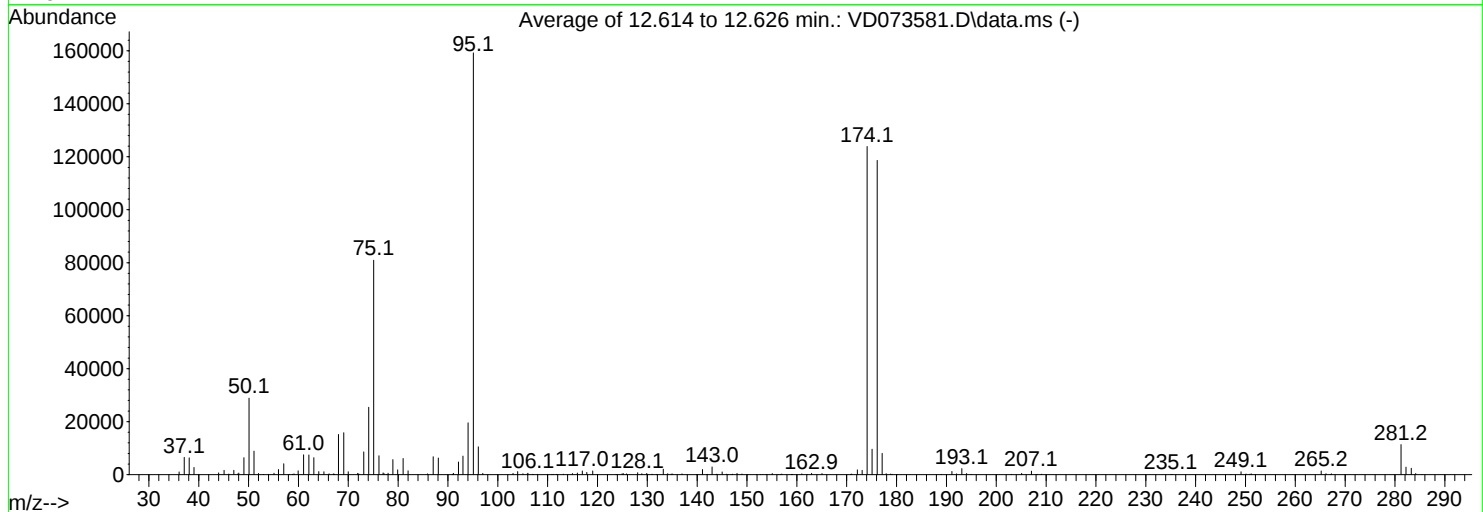


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061522\
Data File : VD073581.D
Acq On : 15 Jun 2022 08:55
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
Title : SW846 8260
Last Update : Thu Jun 09 12:33:32 2022

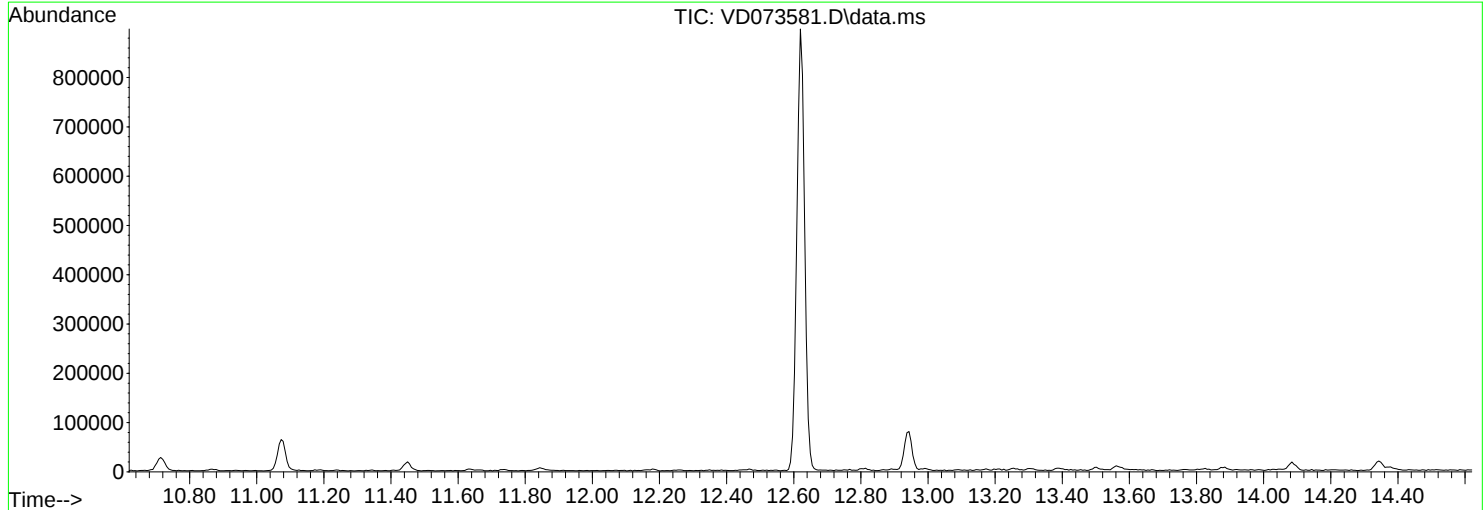

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	28877	PASS
75	95	30	60	50.8	80939	PASS
95	95	100	100	100.0	159232	PASS
96	95	5	9	6.6	10517	PASS
173	174	0.00	2	1.3	1660	PASS
174	95	50	100	77.8	123901	PASS
175	174	5	9	7.8	9611	PASS
176	174	95	101	95.8	118661	PASS
177	176	5	9	6.8	8044	PASS