

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
 Data File : VD076447.D
 Acq On : 15 Jun 2023 19:36
 Operator : KP/SY
 Sample : 03236-17
 Misc : 5.28G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 YBW25

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 06/16/2023
 Supervised By :Mahesh Dadoda 06/16/2023

Quant Time: Jun 16 02:01:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	211689	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	178664	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	68276	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.270	65	75158	14.579	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.320%		
7) Chloroethane-d5	2.793	69	74820	17.949	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.800%		
11) 1,1-Dichloroethene-d2	3.911	65	22199	16.497	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.000%		
21) 2-Butanone-d5	6.981	46	55631	71.253	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	142.500%#		
24) Chloroform-d	7.563	84	122949	22.045	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.200%		
26) 1,2-Dichloroethane-d4	8.228	65	68632	24.945	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.760%		
32) Benzene-d6	8.199	84	237093	21.693	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.760%		
36) 1,2-Dichloropropane-d6	9.210	67	88906	25.485	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.920%		
41) Toluene-d8	10.269	98	208194	20.573	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.280%		
43) trans-1,3-Dichloroprop...	10.522	79	34806	23.987	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.960%		
47) 2-Hexanone-d5	10.875	63	39850	73.588	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	147.180%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	76471	30.811	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	123.240%#		
66) 1,2-Dichlorobenzene-d4	13.816	152	56919	22.744	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.960%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	3.934	96	5667	2.063	ug/L #	1
16) Methylene chloride	4.799	84	9522m	2.588	ug/L	
30) 1,1,1-Trichloroethane	7.787	97	5433m	1.309	ug/L	
34) Trichloroethene	9.028	95	37719	12.418	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
Data File : VD076447.D
Acq On : 15 Jun 2023 19:36
Operator : KP/SY
Sample : 03236-17
Misc : 5.28G/10.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_D
ClientSampleId :
YBW25

Quant Time: Jun 16 02:01:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 06/16/2023
Supervised By :Mahesh Dadoda 06/16/2023

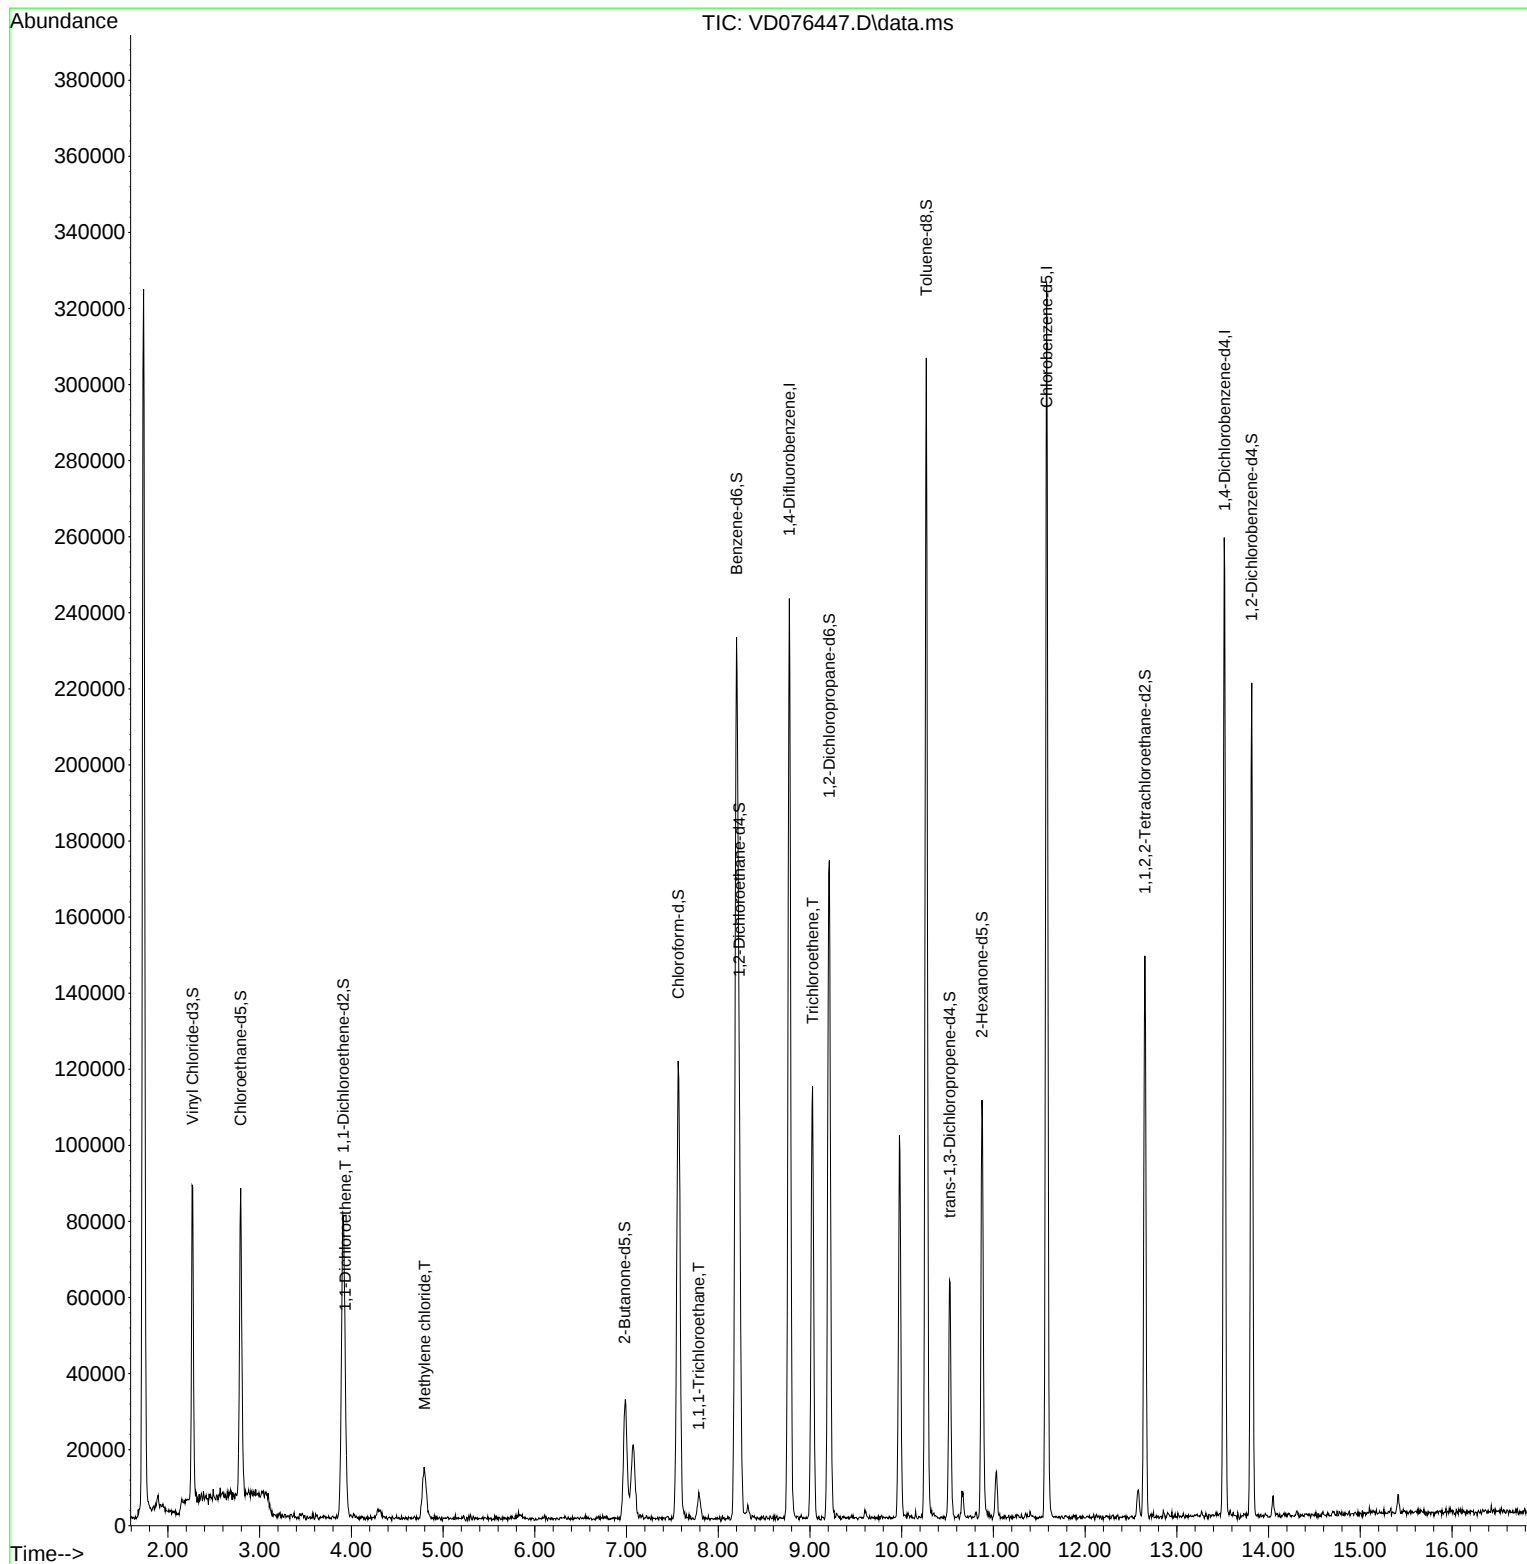

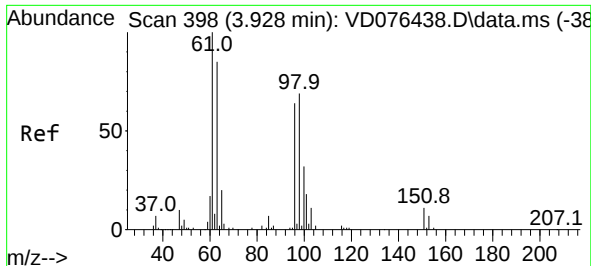

#12

1,1-Dichloroethene

Concen: 2.063 ug/L

RT: 3.934 min Scan# 399

Delta R.T. 0.006 min

Lab File: VD076447.D

Acq: 15 Jun 2023 19:36

Instrument :

MSVOA_D

ClientSampleId :

YBW25





Tgt Ion:	96	Resp:	566
Ion	Ratio	Lower	Upper
96	100		
61	194.9	113.0	209.8
63	468.5	83.6	155.2

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 06/16/2023

Supervised By :Mahesh Dadoda 06/16/2023

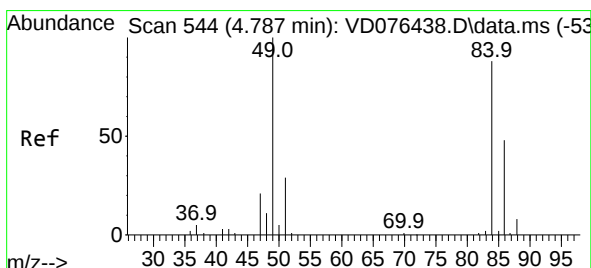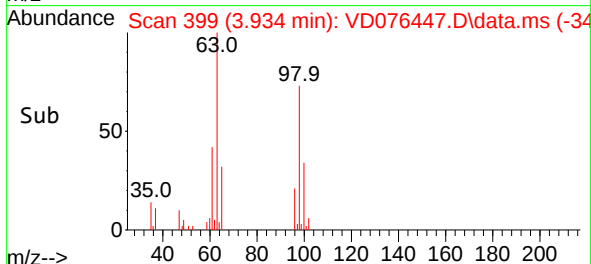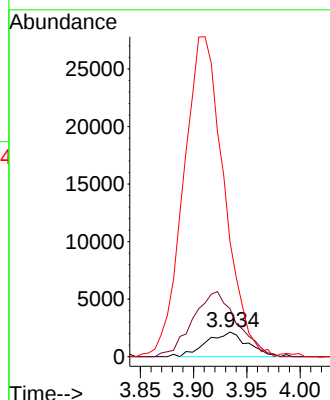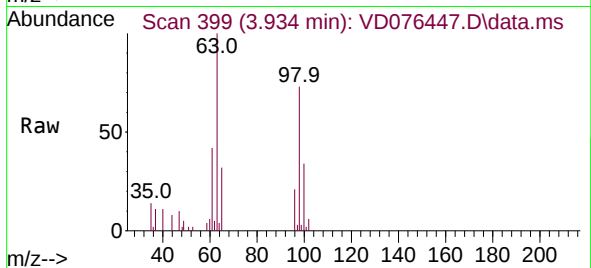

#16

Methylene chloride

Concen: 2.588 ug/L m




RT: 4.799 min Scan# 546


Delta R.T. 0.012 min

Lab File: VD076447.D

Acq: 15 Jun 2023 19:36


Tgt Ion:	84	Resp:	9522
Ion	Ratio	Lower	Upper
84	100		
86	40.3	45.1	83.9#
49	127.0	97.2	180.6

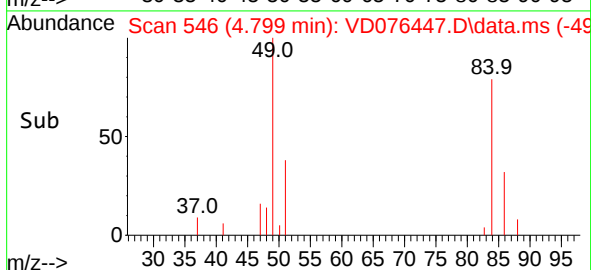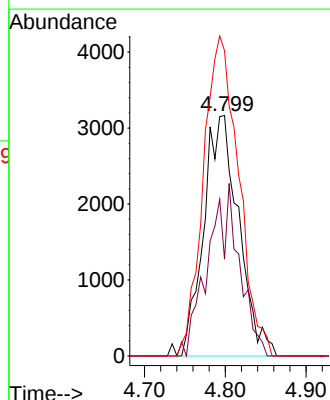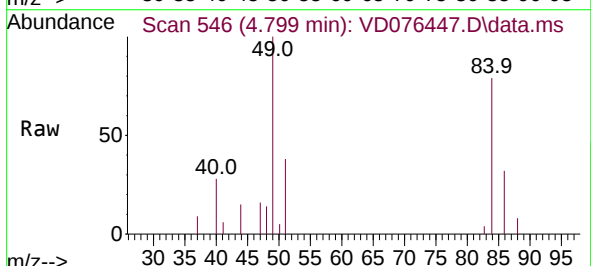

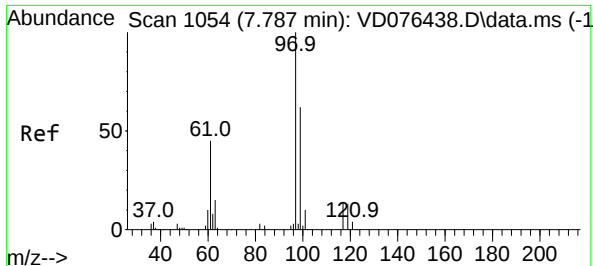

#30
1,1,1-Trichloroethane
Concen: 1.309 ug/L m
RT: 7.787 min Scan# 1054
Delta R.T. -0.000 min
Lab File: VD076447.D
Acq: 15 Jun 2023 19:36




Instrument :
MSVOA_D
ClientSampleId :
YBW25

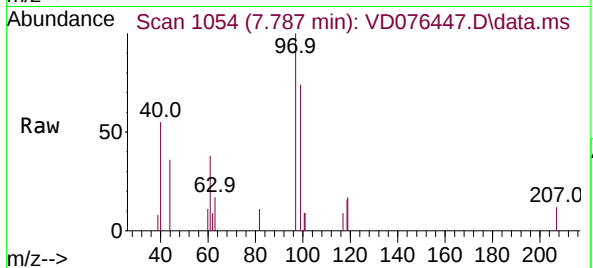

Tgt Ion: 97 Resp: 543
Ion Ratio Lower Upper
97 100
99 67.4 51.0 76.6
61 16.9 36.4 54.6

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 06/16/2023
Supervised By :Mahesh Dadoda 06/16/2023

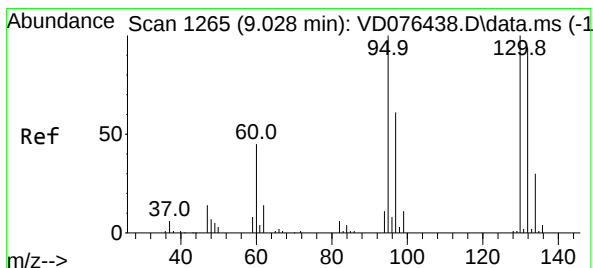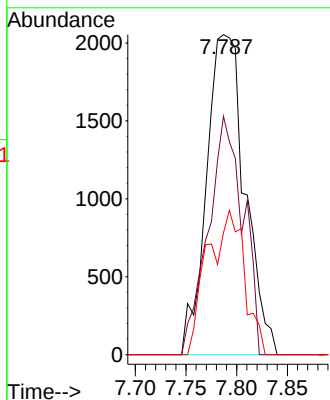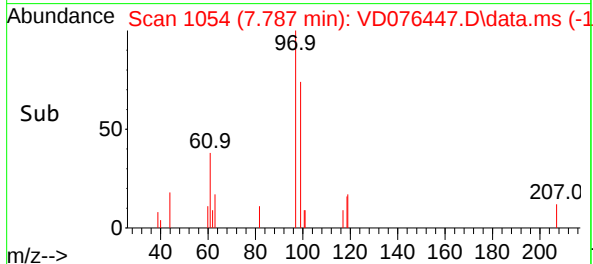

#34
Trichloroethene
Concen: 12.418 ug/L
RT: 9.028 min Scan# 1265
Delta R.T. -0.000 min
Lab File: VD076447.D
Acq: 15 Jun 2023 19:36

Tgt Ion: 95 Resp: 37719
Ion Ratio Lower Upper
95 100
97 61.9 43.1 80.1
132 104.6 71.8 133.4
130 104.2 71.9 133.5

