

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
 Data File : VD076436.D
 Acq On : 15 Jun 2023 13:20
 Operator : KP/SY
 Sample : VIBLK120
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDL061523SMA.M
 Title : SFAM01.0

Signal : TIC: VD076436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.740	15	26	38	rBV	743902	1379056	100.00%	14.291%
2	2.152	92	96	97	rBV3	3768	4433	0.32%	0.046%
3	2.270	111	116	125	rVB	194774	286310	20.76%	2.967%
4	2.799	199	206	215	rBV	140860	257360	18.66%	2.667%
5	3.228	278	279	284	rBV3	1273	1603	0.12%	0.017%
6	3.299	287	291	293	rBV3	3163	3863	0.28%	0.040%
7	3.534	329	331	335	rVB2	1340	1519	0.11%	0.016%
8	3.564	335	336	340	rVB3	1273	838	0.06%	0.009%
9	3.911	385	395	408	rVV2	152404	408219	29.60%	4.230%
10	4.169	438	439	443	rVB2	802	853	0.06%	0.009%
11	4.228	447	449	450	rBV	1056	971	0.07%	0.010%
12	4.275	452	457	458	rBV2	2068	2943	0.21%	0.030%
13	4.440	484	485	488	rBV	1228	904	0.07%	0.009%
14	4.793	538	545	556	rVB4	14129	39221	2.84%	0.406%
15	4.946	570	571	574	rBV	1332	843	0.06%	0.009%
16	5.081	592	594	596	rVB2	1148	956	0.07%	0.010%
17	5.311	632	633	636	rBV2	1586	1120	0.08%	0.012%
18	5.511	665	667	668	rBV	1258	1075	0.08%	0.011%
19	5.528	668	670	672	rVV	1357	1510	0.11%	0.016%
20	5.658	686	692	695	rVV4	1764	3263	0.24%	0.034%
21	5.840	714	723	730	rBV6	6035	15820	1.15%	0.164%
22	5.958	741	743	746	rBV2	740	972	0.07%	0.010%
23	6.034	752	756	757	rVB	1107	1039	0.08%	0.011%
24	6.152	774	776	777	rBV	1465	955	0.07%	0.010%
25	6.322	803	805	808	rVB2	1186	1227	0.09%	0.013%
26	6.358	808	811	812	rBV	768	833	0.06%	0.009%
27	6.369	812	813	816	rBV2	857	950	0.07%	0.010%
28	6.416	819	821	823	rBV	1181	881	0.06%	0.009%
29	6.499	833	835	838	rVB2	947	857	0.06%	0.009%
30	6.669	861	864	866	rVB	1153	1101	0.08%	0.011%
31	6.710	869	871	874	rBV2	911	974	0.07%	0.010%
32	6.863	895	897	899	rBV	1126	1010	0.07%	0.010%
33	6.981	910	917	924	rBV2	26157	72508	5.26%	0.751%
34	7.205	951	955	957	rBV2	875	1546	0.11%	0.016%
35	7.422	991	992	995	rVV	1028	832	0.06%	0.009%
36	7.563	1006	1016	1031	rBV	171410	438962	31.83%	4.549%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
 Data File : VD076436.D
 Acq On : 15 Jun 2023 13:20
 Operator : KP/SY
 Sample : VIBLK120
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Title : SFAM01.0

37	7.663	1031	1033	1035	rVV3	1112	838	0.06%	0.009%
38	7.816	1056	1059	1062	rBV2	1218	1486	0.11%	0.015%
39	7.881	1065	1070	1071	rVB3	1452	1710	0.12%	0.018%
40	8.128	1110	1112	1114	rBV	862	1065	0.08%	0.011%

41	8.199	1114	1124	1142	rVV3	384395	1145077	83.03%	11.867%
42	8.775	1213	1222	1234	rBV	314245	643731	46.68%	6.671%
43	8.963	1252	1254	1259	rBV3	1052	1886	0.14%	0.020%
44	9.016	1261	1263	1267	rVB3	2237	1967	0.14%	0.020%
45	9.210	1287	1296	1305	rBV	237576	501217	36.34%	5.194%

46	9.581	1356	1359	1360	rBV	1069	886	0.06%	0.009%
47	9.840	1397	1403	1409	rVV3	3314	6748	0.49%	0.070%
48	9.981	1415	1427	1434	rBV	144596	282345	20.47%	2.926%
49	10.163	1454	1458	1461	rBV4	2547	3893	0.28%	0.040%
50	10.269	1468	1476	1486	rBV	524303	949433	68.85%	9.839%

51	10.434	1502	1504	1508	rBV2	819	1125	0.08%	0.012%
52	10.528	1513	1520	1528	rBV	94462	167981	12.18%	1.741%
53	10.663	1537	1543	1550	rBV	45738	77908	5.65%	0.807%
54	10.804	1563	1567	1570	rVB3	3636	4781	0.35%	0.050%
55	10.834	1570	1572	1573	rBV2	1166	866	0.06%	0.009%

56	10.875	1573	1579	1586	rBV	103216	181867	13.19%	1.885%
57	11.028	1600	1605	1615	rVB	21102	36401	2.64%	0.377%
58	11.134	1619	1623	1629	rBV3	3604	6830	0.50%	0.071%
59	11.357	1658	1661	1664	rBV3	3123	5467	0.40%	0.057%
60	11.404	1664	1669	1675	rVB2	19759	31956	2.32%	0.331%

61	11.481	1681	1682	1684	rBV2	1243	1008	0.07%	0.010%
62	11.522	1687	1689	1692	rVB3	1608	1408	0.10%	0.015%
63	11.581	1692	1699	1711	rBV	433346	752704	54.58%	7.800%
64	11.681	1714	1716	1721	rVB4	3519	4561	0.33%	0.047%
65	11.757	1727	1729	1730	rBV	1153	902	0.07%	0.009%

66	11.787	1730	1734	1739	rVB2	3944	6691	0.49%	0.069%
67	12.010	1770	1772	1775	rVB2	921	892	0.06%	0.009%
68	12.040	1775	1777	1778	rBV2	1089	902	0.07%	0.009%
69	12.140	1787	1794	1798	rBV4	5644	11989	0.87%	0.124%
70	12.422	1838	1842	1846	rVB4	5012	7749	0.56%	0.080%

71	12.469	1848	1850	1854	rVB2	1223	1038	0.08%	0.011%
72	12.540	1860	1862	1863	rBV	1098	865	0.06%	0.009%
73	12.581	1863	1869	1874	rVV2	19089	30017	2.18%	0.311%
74	12.651	1874	1881	1889	rVB	168113	276802	20.07%	2.869%
75	12.728	1893	1894	1896	rBV	1763	1033	0.07%	0.011%

76	12.910	1920	1925	1929	rBV4	5251	8207	0.60%	0.085%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
 Data File : VD076436.D
 Acq On : 15 Jun 2023 13:20
 Operator : KP/SY
 Sample : VIBLK120
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Title : SFAM01.0

77	12.993	1938	1939	1941	rBV	2005	1392	0.10%	0.014%
78	13.057	1947	1950	1954	rBV2	1108	1327	0.10%	0.014%
79	13.098	1954	1957	1959	rBV2	886	946	0.07%	0.010%
80	13.216	1975	1977	1981	rVB2	4928	4656	0.34%	0.048%
81	13.269	1983	1986	1990	rVB3	3554	4813	0.35%	0.050%
82	13.440	2011	2015	2016	rBV2	4184	4561	0.33%	0.047%
83	13.457	2016	2018	2022	rVV2	7328	8859	0.64%	0.092%
84	13.522	2022	2029	2036	rVV	428492	720631	52.26%	7.468%
85	13.745	2065	2067	2068	rVV2	1902	962	0.07%	0.010%
86	13.816	2072	2079	2087	rVV	400738	687177	49.83%	7.121%
87	14.051	2114	2119	2126	rBV2	8249	13027	0.94%	0.135%
88	14.128	2130	2132	2133	rBV2	958	831	0.06%	0.009%
89	14.210	2145	2146	2149	rBV2	1475	880	0.06%	0.009%
90	14.592	2206	2211	2217	rBV4	8147	12305	0.89%	0.128%
91	14.663	2222	2223	2226	rBV	1181	1092	0.08%	0.011%
92	14.887	2260	2261	2263	rBV2	1682	1453	0.11%	0.015%
93	15.016	2281	2283	2285	rBV2	1417	921	0.07%	0.010%
94	15.075	2290	2293	2294	rBV2	1818	1675	0.12%	0.017%
95	15.104	2294	2298	2304	rVB4	10865	18744	1.36%	0.194%
96	15.334	2333	2337	2344	rVB	12730	20001	1.45%	0.207%
97	15.416	2346	2351	2355	rVV2	11098	16649	1.21%	0.173%
98	15.481	2360	2362	2365	rVV3	4700	4820	0.35%	0.050%
99	15.522	2365	2369	2375	rVB5	11080	19181	1.39%	0.199%
100	16.216	2485	2487	2488	rBV	1952	1068	0.08%	0.011%


Sum of corrected areas: 9649530

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
Data File : VD076436.D
Acq On : 15 Jun 2023 13:20
Operator : KP/SY
Sample : VIBLK120
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

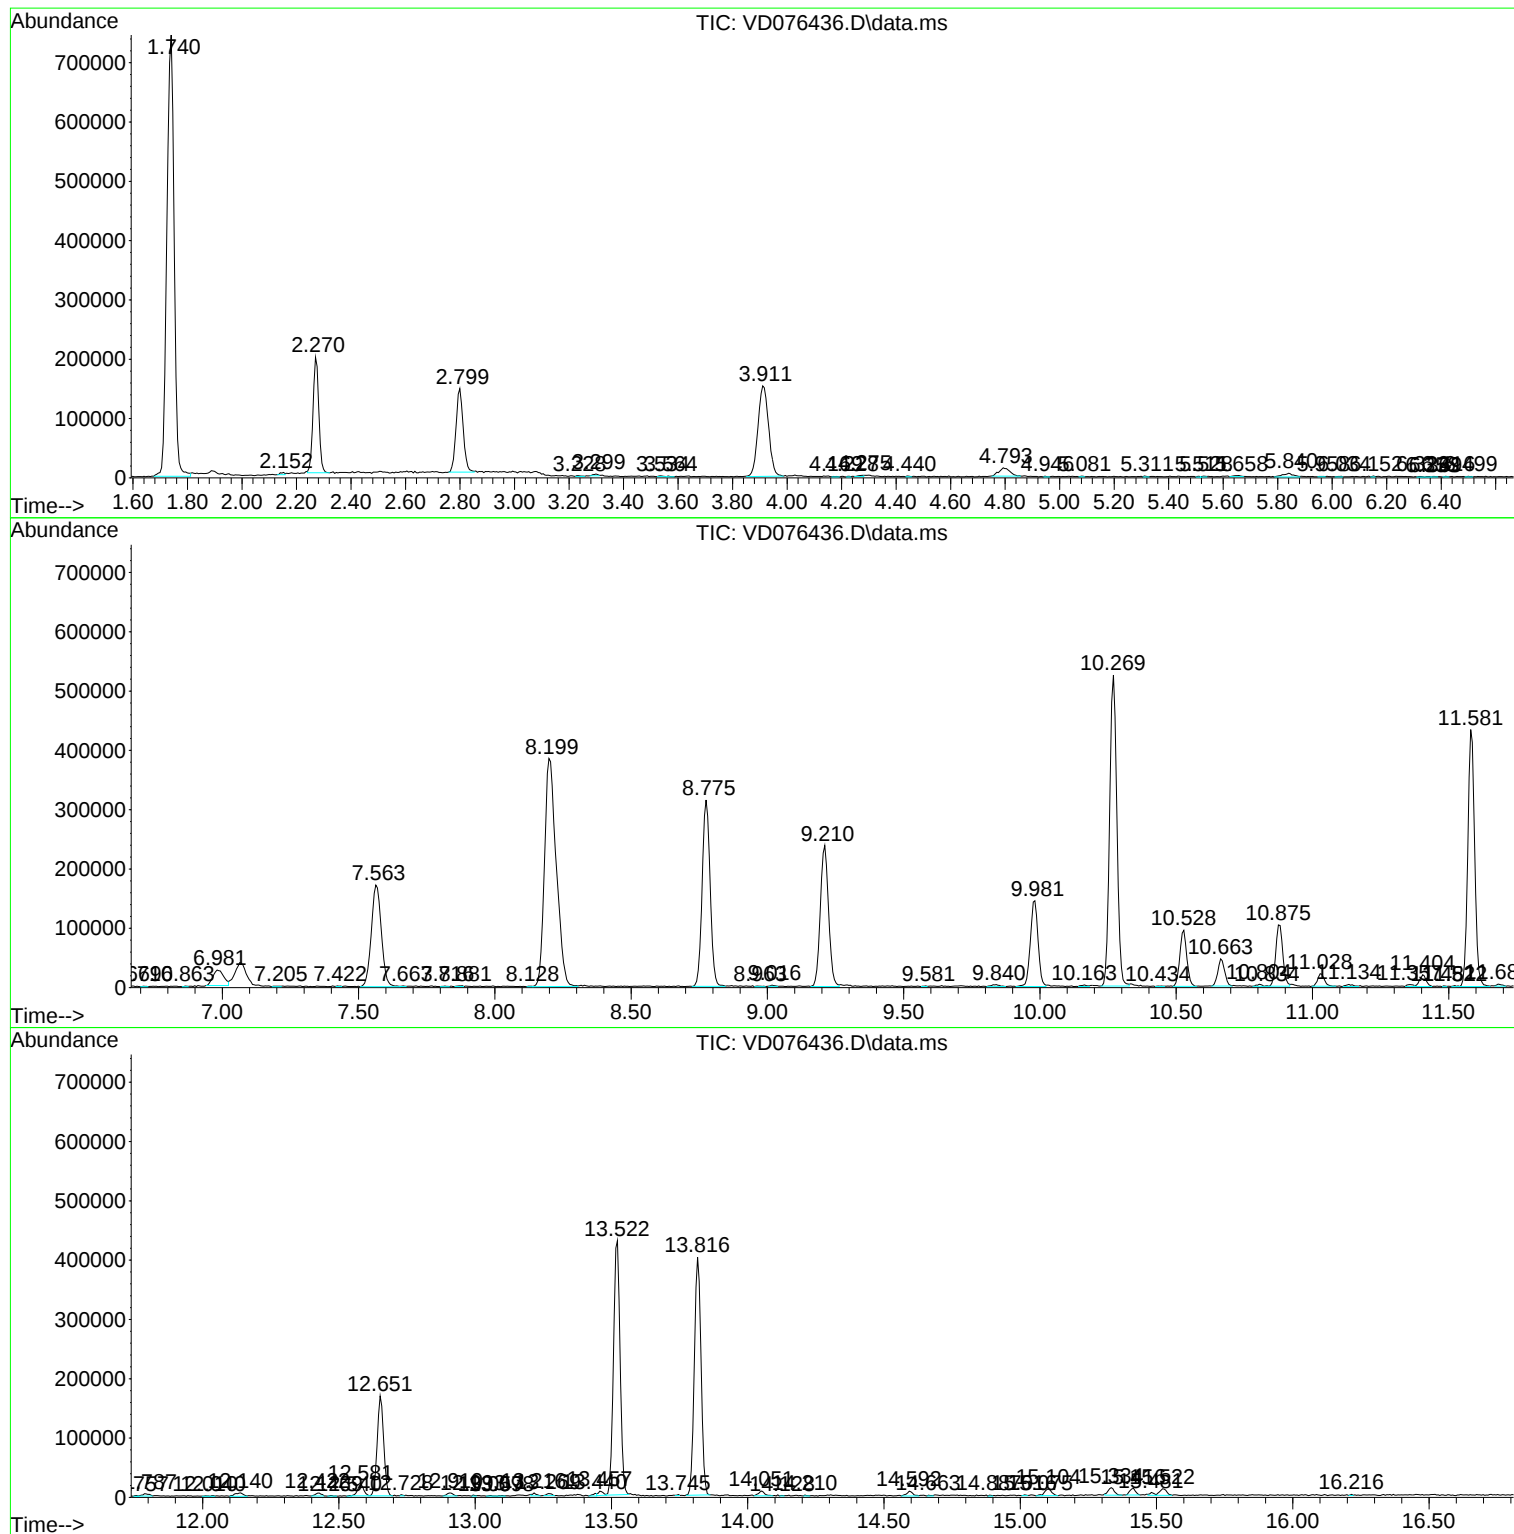

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
Data File : VD076436.D
Acq On : 15 Jun 2023 13:20
Operator : KP/SY
Sample : VIBLK120
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
Data File : VD076436.D
Acq On : 15 Jun 2023 13:20
Operator : KP/SY
Sample : VIBLK120
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------