
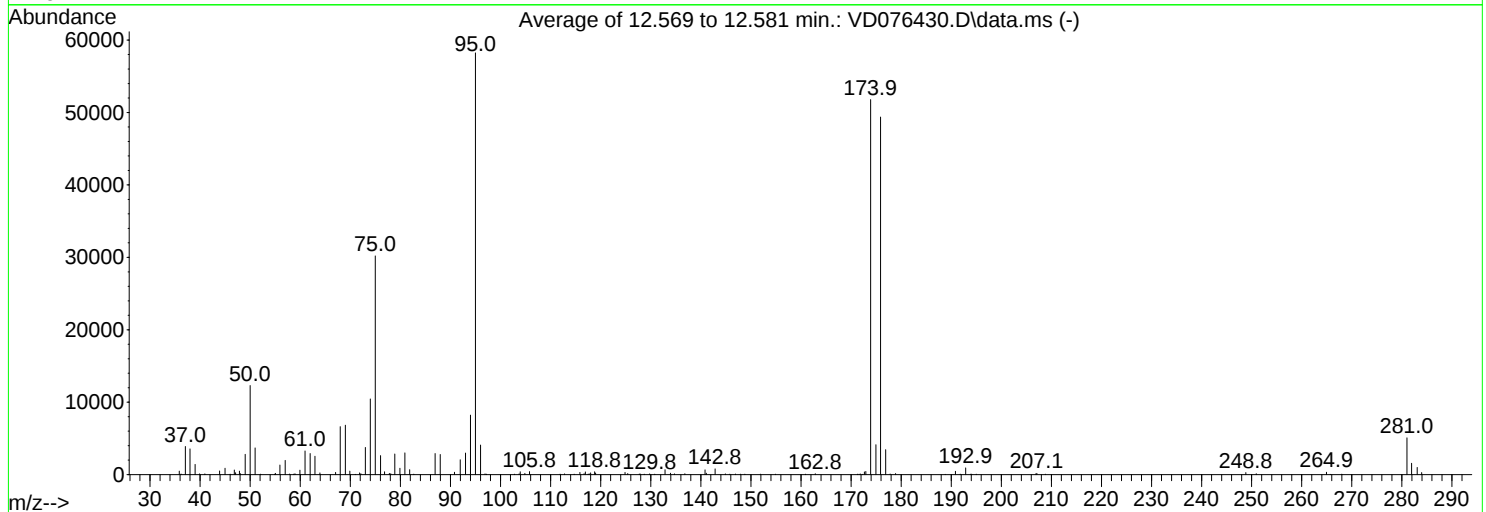


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061523\
 Data File : VD076430.D
 Acq On : 15 Jun 2023 09:25
 Operator : KP/SY
 Sample : BFB145
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB145

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Title : SFAM01.0
 Last Update : Fri Jun 16 01:50:34 2023

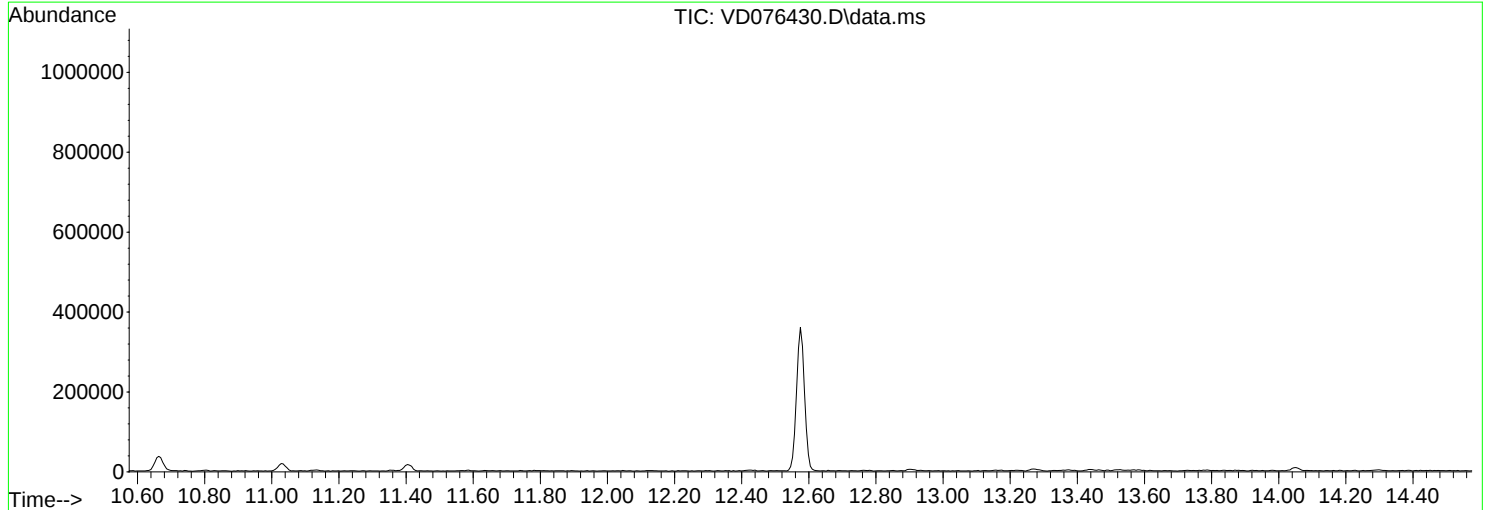

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	12316	PASS
75	95	30	80	51.8	30189	PASS
95	95	100	100	100.0	58235	PASS
96	95	5	9	7.0	4096	PASS
173	174	0.00	2	0.8	437	PASS
174	95	50	120	88.9	51784	PASS
175	174	5	9	8.0	4124	PASS
176	174	95	105	95.3	49371	PASS
177	176	5	10	7.0	3444	PASS

m/z	Abundance
39.90	1234.0
42.20	198.0
43.00	239.0
43.90	952.0
57.00	153.0
207.00	240.0

Instrument :
MSVOA_D
ClientSampleId :
BFB145

m/z	Abundance
35.90	336.0
37.00	3745.0
38.00	3908.0
39.00	1677.0
39.90	1197.0
40.90	164.0
44.00	1571.0
45.00	889.0
47.10	778.0
47.80	375.0
48.10	411.0
49.00	2496.0
50.00	13107.0
51.00	3189.0
54.90	210.0
56.10	1475.0
57.10	1859.0
58.70	185.0
59.90	527.0
60.90	3012.0
62.00	2349.0
62.90	2435.0
64.00	217.0
67.10	282.0
68.00	6090.0
69.00	6684.0
69.90	364.0
72.10	400.0
73.00	3469.0
74.00	10308.0
75.00	30408.0
76.10	2528.0
76.80	326.0
77.80	320.0
78.90	2529.0
79.90	795.0
80.90	2993.0
81.80	796.0
87.00	2709.0
87.90	2831.0
90.80	417.0
92.00	2030.0
93.00	2268.0
94.00	8014.0
95.00	55576.0
96.00	3770.0
97.20	204.0
104.00	330.0
104.90	193.0
105.80	383.0
111.90	220.0
115.90	286.0
117.00	476.0
117.50	213.0
118.00	312.0
118.80	622.0
124.80	205.0
127.70	283.0
128.70	208.0
132.90	796.0
134.80	201.0
140.90	642.0
142.90	671.0
145.00	177.0
147.90	203.0
162.90	201.0
171.60	192.0
172.30	163.0
172.90	690.0
173.90	48656.0
175.00	3717.0
175.90	45560.0
176.90	2989.0
190.80	389.0
192.90	716.0
195.00	179.0
207.00	548.0
208.80	174.0
250.90	200.0
264.90	254.0
281.00	3891.0
282.00	1056.0
283.10	747.0

Instrument :
MSVOA_D
ClientSampleId :
BFB145

m/z	Abundance
35.90	776.0
37.10	4293.0
38.00	3916.0
39.00	1601.0
39.90	1570.0
41.00	205.0
43.10	249.0
43.90	1446.0
45.00	1156.0
46.00	193.0
46.80	722.0
47.90	633.0
49.00	3209.0
50.00	12550.0
51.00	3796.0
52.10	219.0
55.10	247.0
55.90	1440.0
57.00	2637.0
57.90	254.0
59.00	169.0
60.00	653.0
61.00	3953.0
62.00	3729.0
63.00	2923.0
63.90	307.0
67.10	311.0
68.00	7087.0
69.00	7574.0
69.90	598.0
71.80	516.0
73.00	3718.0
74.00	11844.0
75.00	32736.0
76.00	3075.0
76.80	413.0
77.80	244.0
78.90	3267.0
79.80	931.0
80.90	2855.0
81.80	584.0
82.70	212.0
87.00	2962.0
88.00	3227.0
90.90	249.0
91.90	2178.0
93.00	3512.0
94.00	8927.0
95.00	65160.0
96.00	4687.0
96.90	362.0
103.90	568.0
104.80	191.0
105.90	518.0
112.90	181.0
114.70	210.0
115.80	418.0
116.90	657.0
118.00	435.0
118.80	604.0
124.90	337.0
125.40	197.0
129.80	343.0
130.80	195.0
132.90	689.0
134.00	349.0
134.70	161.0
136.80	182.0
140.70	607.0
141.10	587.0
142.80	997.0
145.80	170.0
151.90	184.0
160.90	207.0
162.80	228.0
172.60	490.0
173.00	620.0
173.90	56208.0
174.90	4304.0
175.90	53640.0
176.90	3410.0
177.80	295.0
178.90	224.0
188.80	158.0
190.90	476.0
191.80	178.0
192.80	935.0
193.90	193.0
206.80	598.0
248.80	452.0
250.90	232.0
265.00	393.0

Instrument :
MSVOA_D
ClientSampleId :
BFB145

265.70	153.0
268.00	169.0
281.00	5612.0
282.00	1917.0
283.10	1004.0
284.00	540.0

Instrument :
MSVOA_D
ClientSampleId :
BFB145

m/z	Abundance
35.70	362.0
36.20	252.0
37.00	3626.0
38.00	2884.0
38.90	954.0
40.00	1289.0
44.00	1385.0
45.00	617.0
46.90	1201.0
47.90	440.0
49.00	2721.0
50.00	11292.0
51.00	4110.0
55.00	313.0
55.80	1046.0
57.00	1839.0
58.90	264.0
60.00	663.0
60.90	2873.0
62.00	2668.0
62.90	2248.0
63.90	216.0
67.00	328.0
68.00	6736.0
69.00	6221.0
69.90	510.0
71.00	160.0
71.90	207.0
73.00	4105.0
74.00	9204.0
75.00	27424.0
76.00	2310.0
76.90	443.0
78.10	426.0
78.90	2784.0
80.00	906.0
80.90	3135.0
81.90	686.0
86.90	3098.0
88.00	2274.0
90.70	354.0
92.00	1967.0
93.00	3137.0
94.00	7686.0
95.00	53968.0
96.00	3831.0
102.80	182.0
103.70	330.0
104.00	320.0
104.80	171.0
105.70	385.0
112.70	175.0
115.80	242.0
116.70	417.0
117.70	370.0
119.00	656.0
124.80	381.0
125.40	247.0
127.90	302.0
132.80	583.0
133.90	223.0
136.80	196.0
140.90	755.0
142.90	715.0
144.80	153.0
146.90	282.0
148.80	171.0
154.90	217.0
171.30	181.0
171.90	265.0
172.70	659.0
173.90	50488.0
174.90	4352.0
175.90	48912.0
176.90	3932.0
178.90	231.0
190.80	526.0
193.00	1122.0
194.10	238.0
207.10	543.0
248.90	408.0
264.90	342.0
281.00	5766.0
281.90	1732.0
283.00	1231.0
283.80	306.0

Instrument :
MSVOA_D
ClientSampleId :
BFB145