
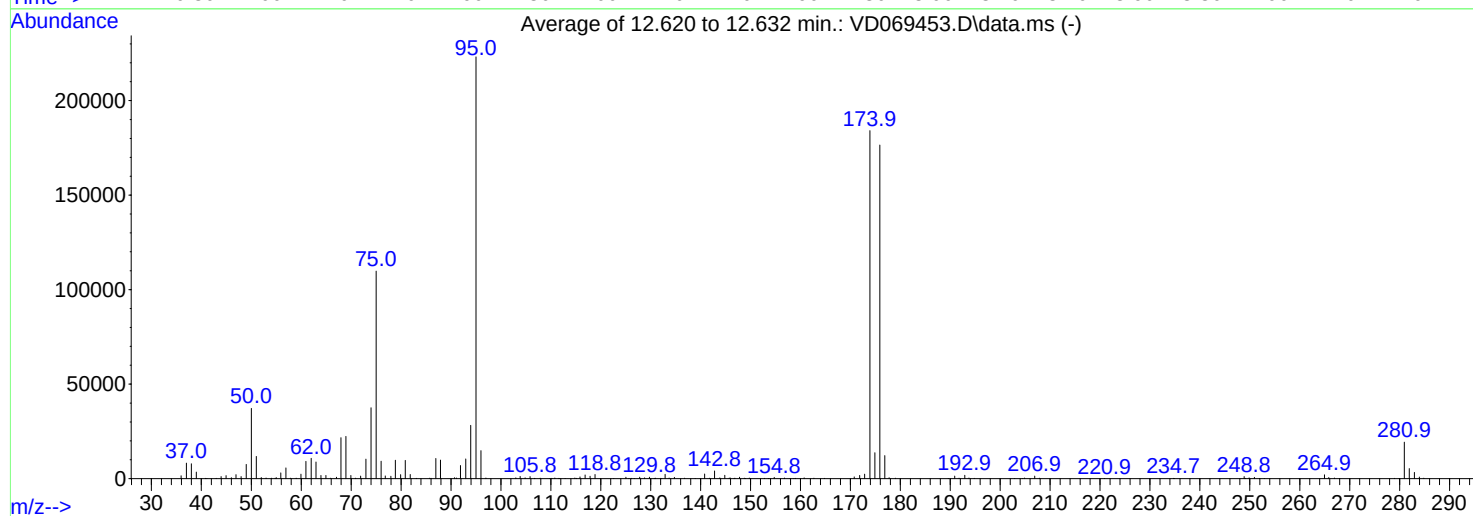


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061621\
Data File : VD069453.D
Acq On : 16 Jun 2021 08:07
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061121S.M
Title : SW846 8260
Last Update : Fri Jun 11 12:50:13 2021

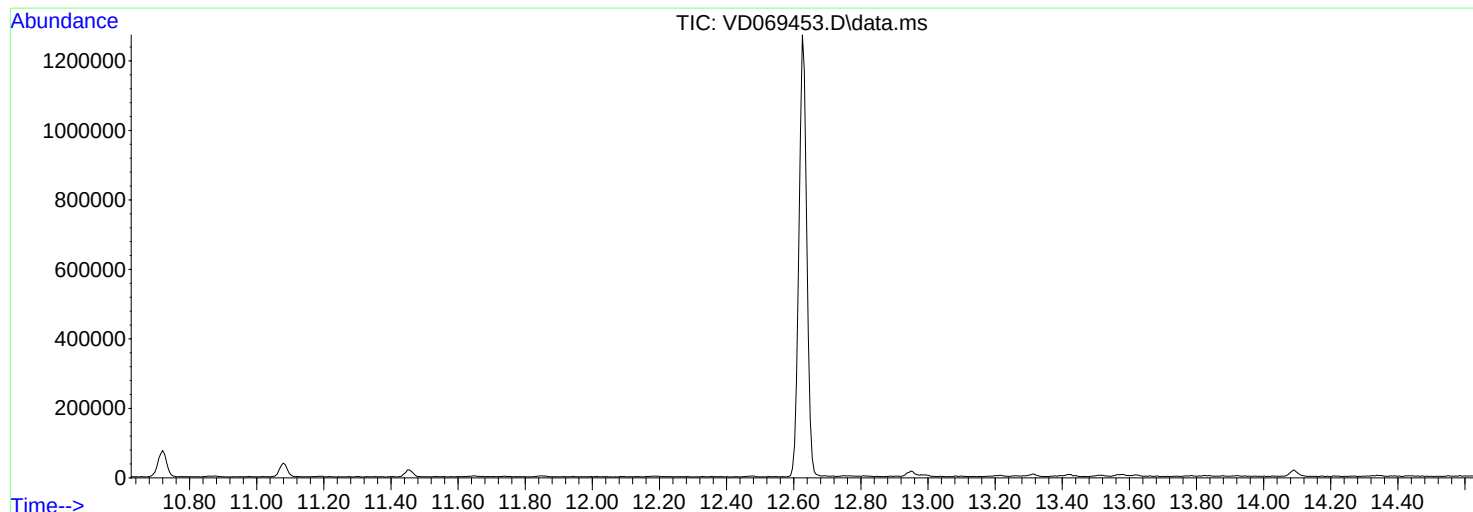

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	37205	PASS
75	95	30	60	49.2	109792	PASS
95	95	100	100	100.0	223168	PASS
96	95	5	9	6.6	14780	PASS
173	174	0.00	2	1.3	2411	PASS
174	95	50	100	82.5	184149	PASS
175	174	5	9	7.4	13694	PASS
176	174	95	101	95.8	176469	PASS
177	176	5	9	6.9	12152	PASS