
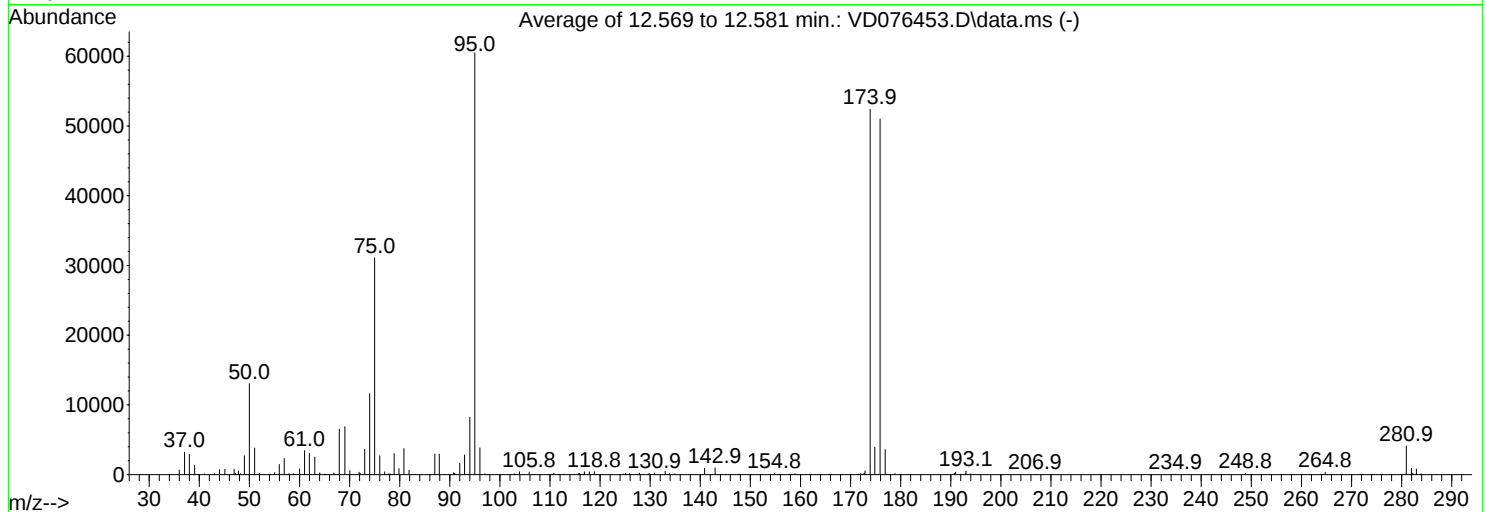


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061623\
Data File : VD076453.D
Acq On : 16 Jun 2023 12:52
Operator : KP/SY
Sample : BFB
Misc : 5.00G/10.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Title : SW846 8260
Last Update : Mon Jun 19 04:51:45 2023

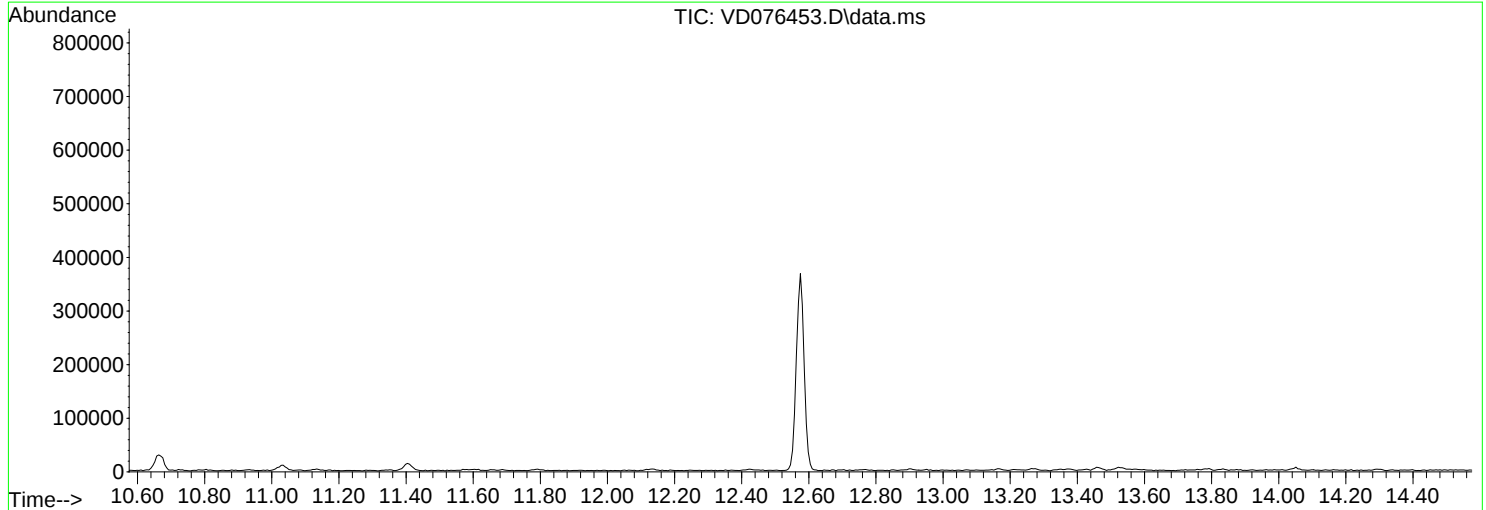

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	13048	PASS
75	95	30	60	51.4	31088	PASS
95	95	100	100	100.0	60491	PASS
96	95	5	9	6.3	3839	PASS
173	174	0.00	2	1.1	560	PASS
174	95	50	100	86.7	52416	PASS
175	174	5	9	7.5	3950	PASS
176	174	95	101	97.3	51005	PASS
177	176	5	9	7.0	3580	PASS