


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD061719\
Data File : VD062717.D
Acq On : 17 Jun 2019 9:47
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
Title : SW846 8260
Last Update : Sat Jun 08 00:02:21 2019

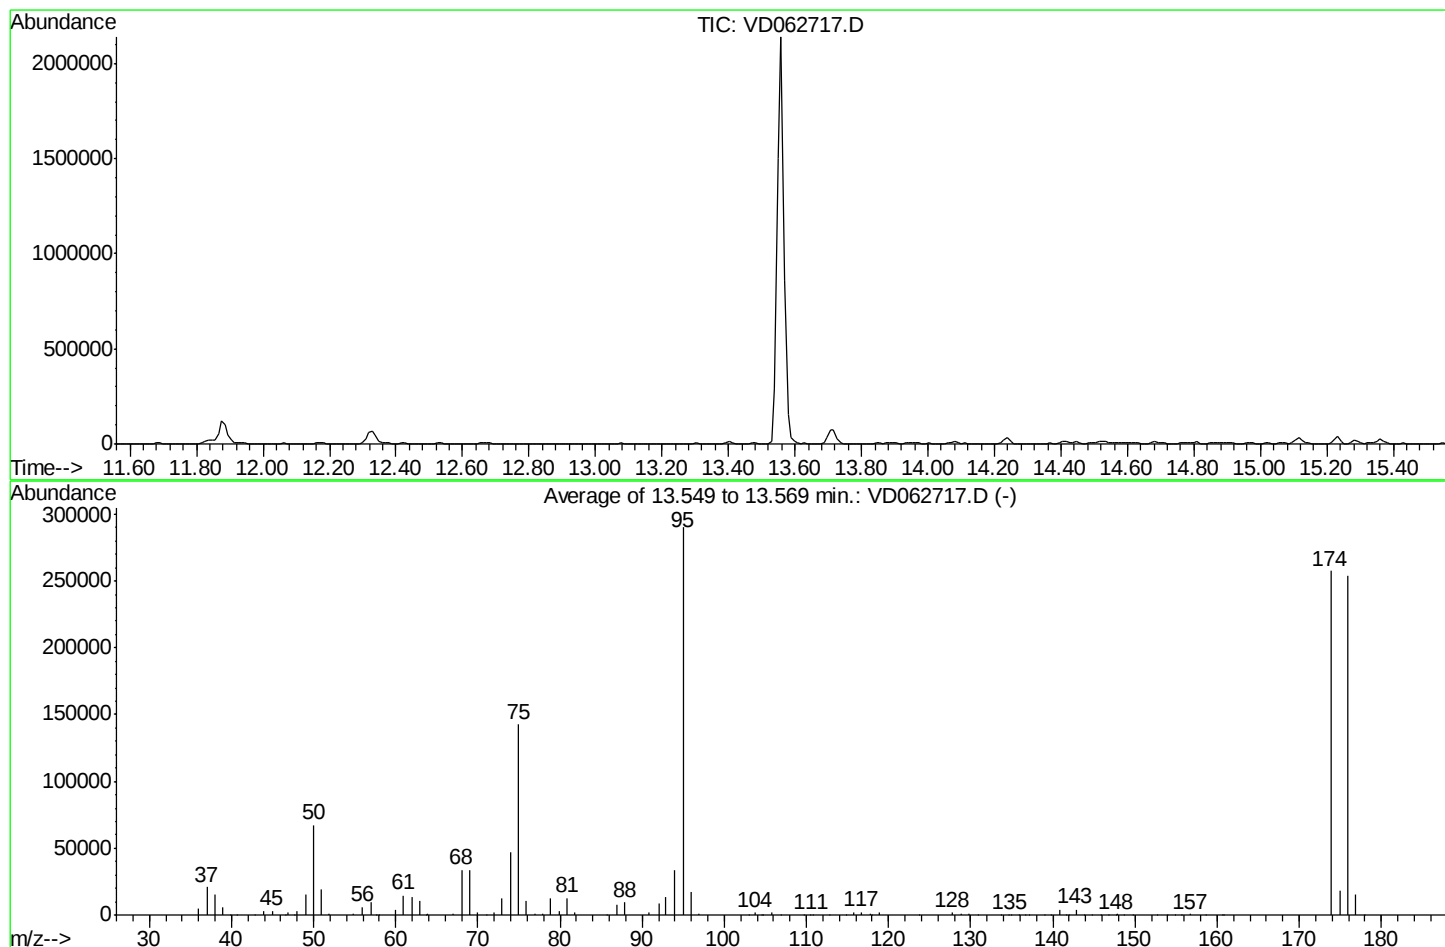

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	67141	PASS
75	95	30	60	49.1	142464	PASS
95	95	100	100	100.0	290154	PASS
96	95	5	9	5.8	16856	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.7	257493	PASS
175	174	5	9	7.0	18071	PASS
176	174	95	101	98.8	254314	PASS
177	176	5	9	6.1	15570	PASS