


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD061819\
 Data File : VD062741.D
 Acq On : 18 Jun 2019 9:38
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060719S.M
 Title : SW846 8260
 Last Update : Sat Jun 08 00:02:21 2019

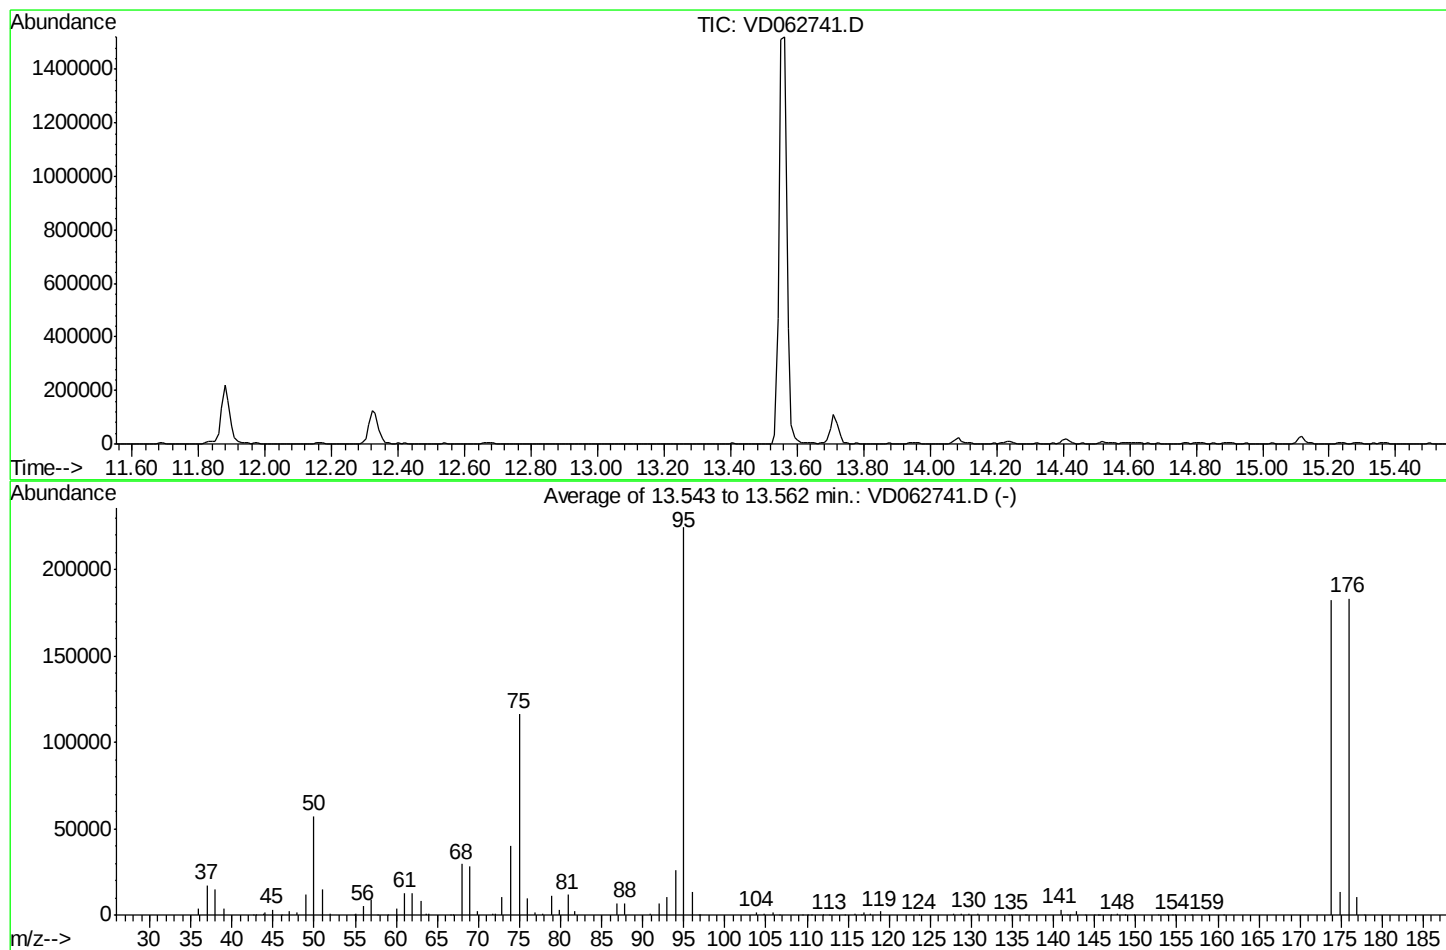

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.6	57490	PASS
75	95	30	60	51.9	116474	PASS
95	95	100	100	100.0	224581	PASS
96	95	5	9	6.0	13444	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.3	182664	PASS
175	174	5	9	7.5	13665	PASS
176	174	95	101	100.3	183248	PASS
177	176	5	9	5.6	10186	PASS