


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD061819\  
Data File : VD062763.D  
Acq On : 18 Jun 2019 22:19  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D060719S.M  
Title : SW846 8260  
Last Update : Sat Jun 08 00:02:21 2019

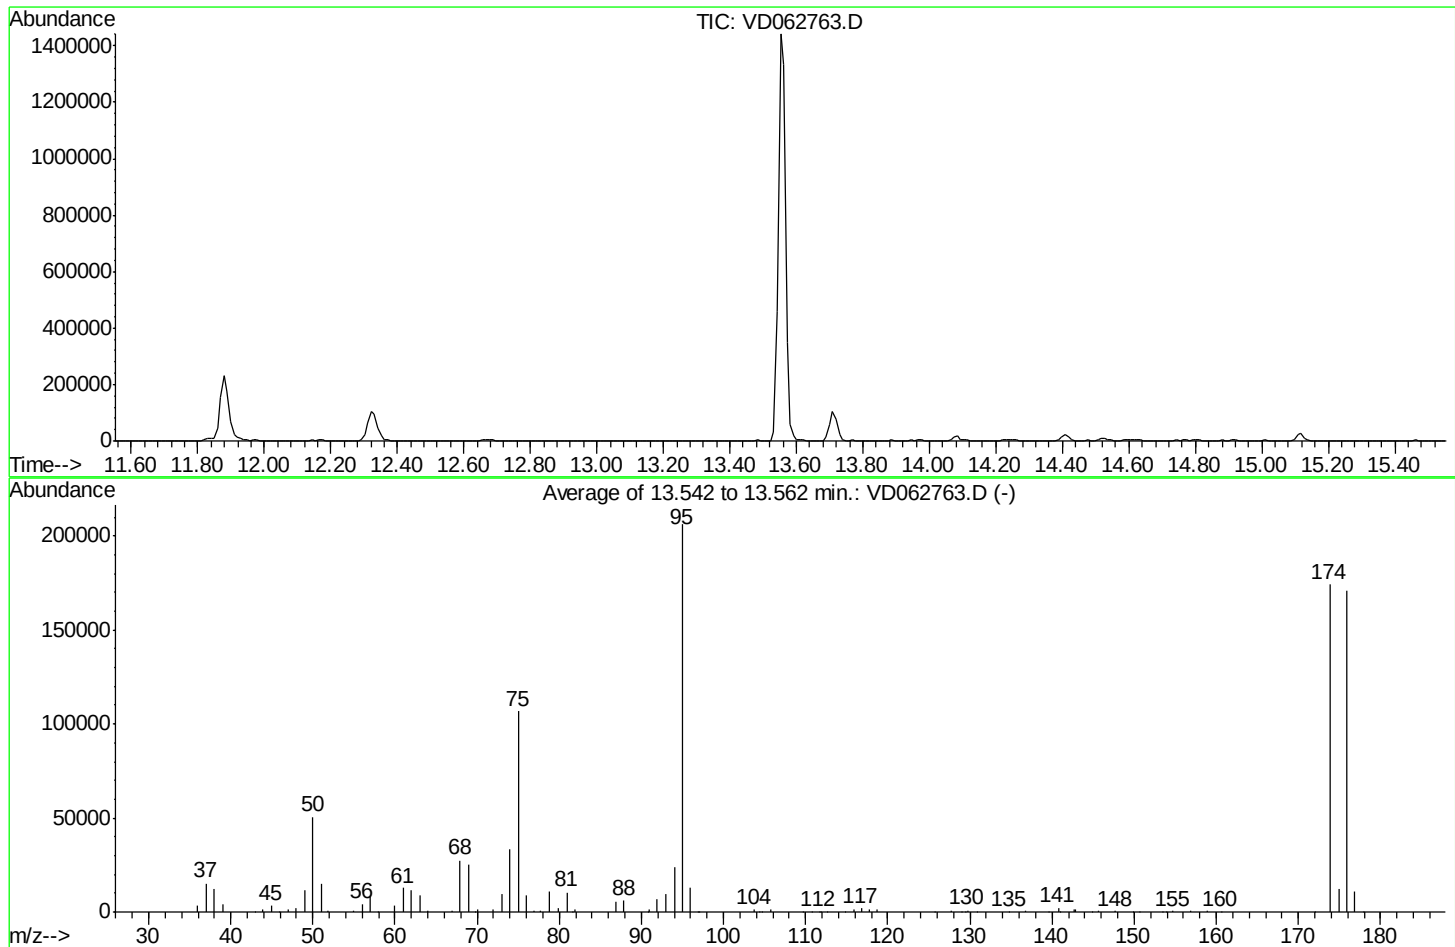

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 24.5      | 50536   | PASS             |
| 75          | 95           | 30           | 60           | 51.7      | 106698  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 206216  | PASS             |
| 96          | 95           | 5            | 9            | 6.2       | 12744   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 84.4      | 174096  | PASS             |
| 175         | 174          | 5            | 9            | 7.0       | 12244   | PASS             |
| 176         | 174          | 95           | 101          | 98.0      | 170650  | PASS             |
| 177         | 176          | 5            | 9            | 6.2       | 10659   | PASS             |