


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062018\
Data File : VD058203.D
Acq On : 20 Jun 2018 10:01
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Title : SW846 8260
Last Update : Wed Jun 20 05:52:56 2018

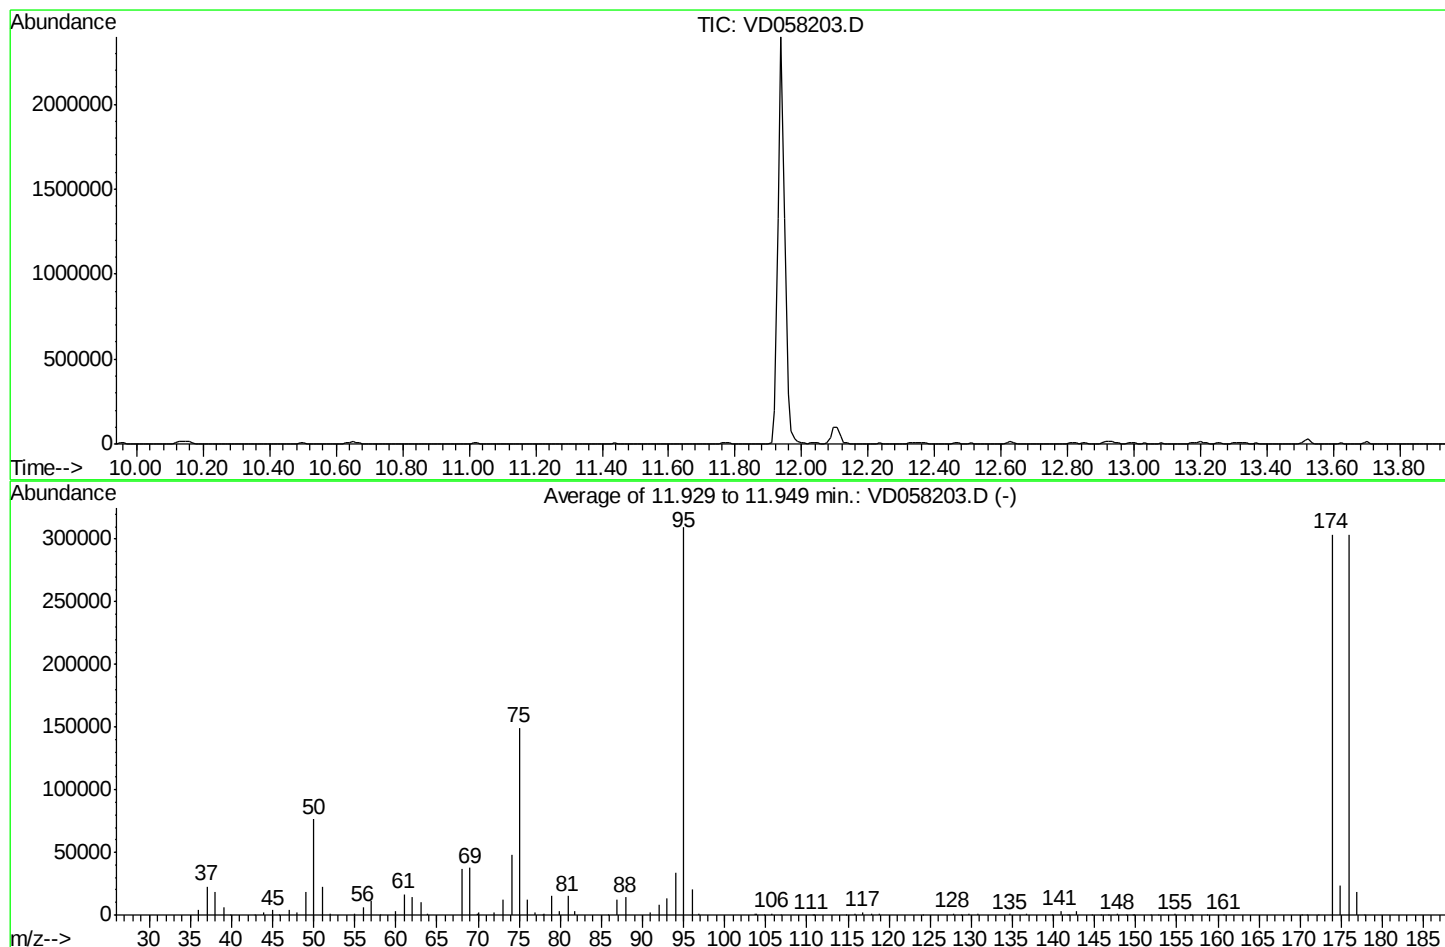

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	76336	PASS
75	95	30	60	48.3	149560	PASS
95	95	100	100	100.0	309482	PASS
96	95	5	9	6.8	20918	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	98.1	303701	PASS
175	174	5	9	7.6	23206	PASS
176	174	95	101	99.8	303210	PASS
177	176	5	9	6.0	18272	PASS