

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062023\
 Data File : VD076488.D
 Acq On : 20 Jun 2023 13:16
 Operator : KP/SY
 Sample : 03289-02
 Misc : 5.04G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-01-4.0-6.0

Quant Time: Jun 21 06:45:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	6235	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	10658	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.587	117	11595	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	5548	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	5735	91.805	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 183.600%#	
35) Dibromofluoromethane	7.804	113	4434	70.030	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 140.060%	
50) Toluene-d8	10.269	98	13109	54.593	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 109.180%	
62) 4-Bromofluorobenzene	12.575	95	5214	66.906	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 133.820%	


Target Compounds				Qvalue		
3) Chloromethane	2.152	50	256	2.598	ug/l #	41
4) Vinyl Chloride	2.264	62	136	1.237	ug/l #	42
5) Bromomethane	2.693	94	300	4.198	ug/l #	1
6) Chloroethane	2.934	64	146	1.938	ug/l #	43
11) Tert butyl alcohol	4.981	59	67	12.422	ug/l #	73
13) Acrolein	3.940	56	54	9.295	ug/l #	15
15) Acrylonitrile	5.175	53	59	3.370	ug/l #	18
16) Acetone	4.022	43	1629	109.584	ug/l #	32
18) Methyl Acetate	4.569	43	151	2.204	ug/l #	42
21) trans-1,2-Dichloroethene	5.310	96	87	1.319	ug/l #	4
25) 2-Butanone	7.087	43	156	6.785	ug/l #	37
26) 2,2-Dichloropropane	7.063	77	835	7.687	ug/l #	49
29) Tetrahydrofuran	7.452	42	79	5.347	ug/l #	23
31) Cyclohexane	7.946	56	59	Below Cal	#	8
37) Ethyl Acetate	7.199	43	76	1.479	ug/l #	62
38) Carbon Tetrachloride	7.869	117	414	5.224	ug/l #	11
41) Methacrylonitrile	7.404	41	151	5.205	ug/l #	31
43) Isopropyl Acetate	8.346	43	131	1.347	ug/l #	43
46) Dibromomethane	9.440	93	54	1.375	ug/l #	2
48) Methyl methacrylate	9.387	41	178	3.993	ug/l #	1
51) 4-Methyl-2-Pentanone	10.410	43	142	2.856	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.910	63	58	1.907	ug/l #	43
59) 2-Hexanone	10.810	43	131	3.788	ug/l	71
76) 1,2,3-Trichloropropane	12.569	75	2672	48.527	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.369	75	96	3.820	ug/l #	17
87) 1,3-Dichlorobenzene	13.545	146	183	1.011	ug/l	91
88) 1,4-Dichlorobenzene	13.545	146	183	1.014	ug/l	91
92) 1,2-Dibromo-3-Chloropr...	14.375	75	55	4.741	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.092	180	149	1.413	ug/l #	72
95) Naphthalene	15.339	128	496	2.353	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062023\
Data File : VD076488.D
Acq On : 20 Jun 2023 13:16
Operator : KP/SY
Sample : 03289-02
Misc : 5.04G/5.0ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Quant Time: Jun 21 06:45:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

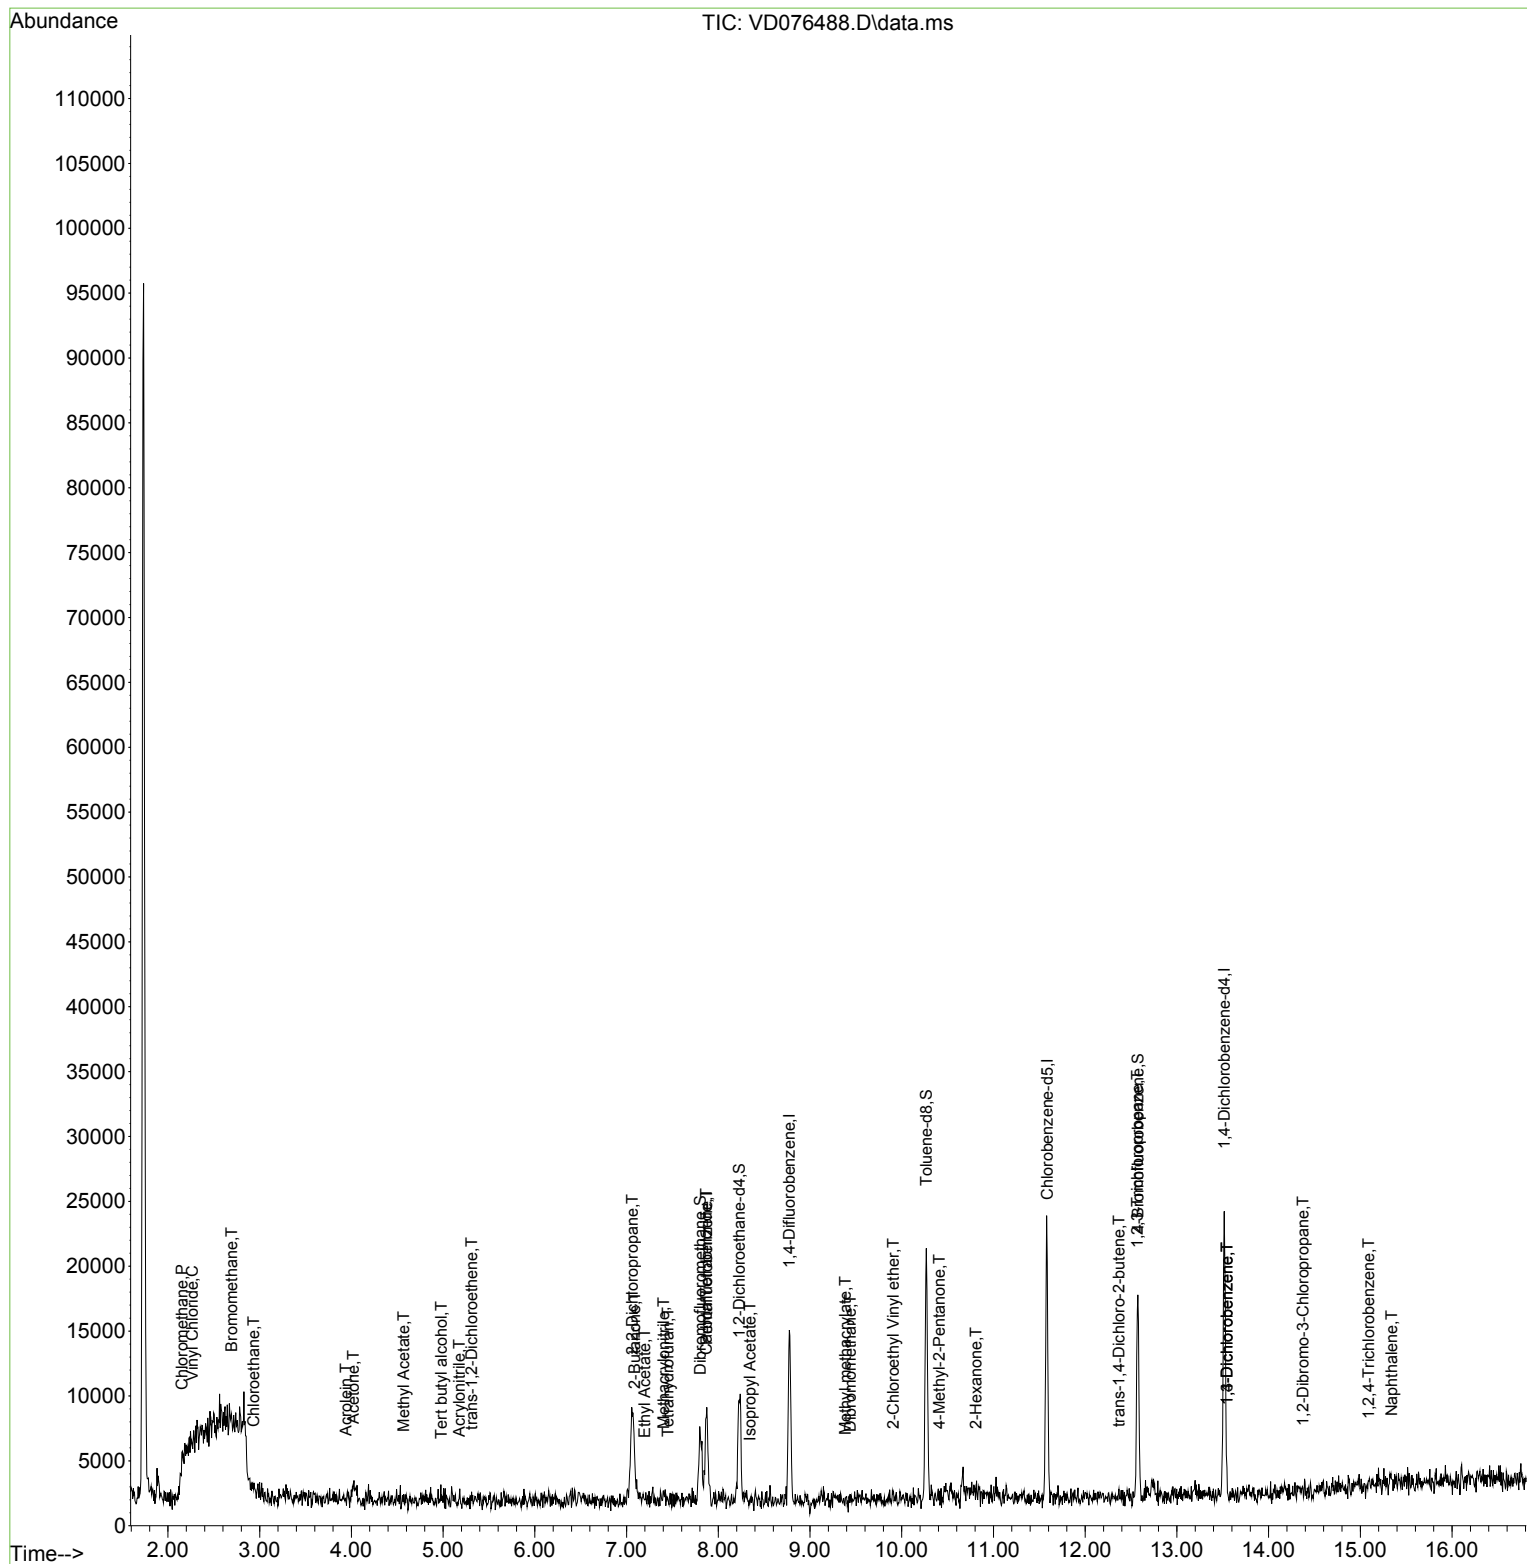






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0



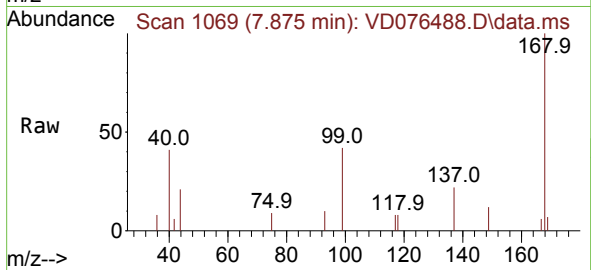



Tgt Ion:168 Resp: 6235
Ion Ratio Lower Upper
168 100
99 42.2 36.7 55.1

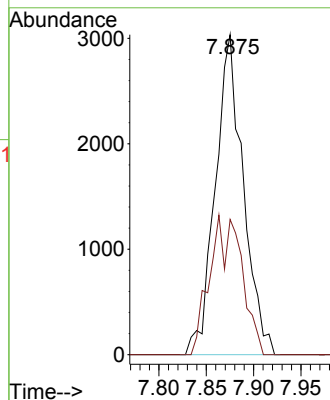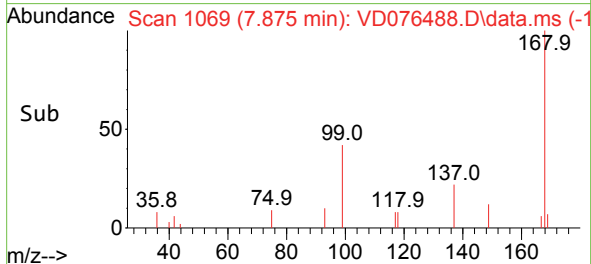

#3
Chloromethane
Concen: 2.598 ug/l
RT: 2.152 min Scan# 96
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 50 Resp: 256
Ion Ratio Lower Upper
50 100
52 0.0 26.6 40.0#


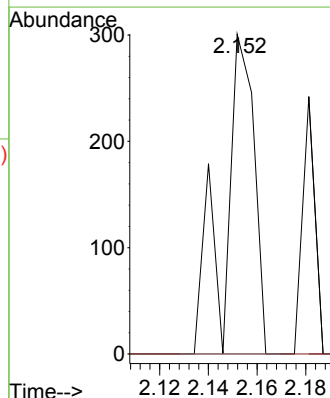




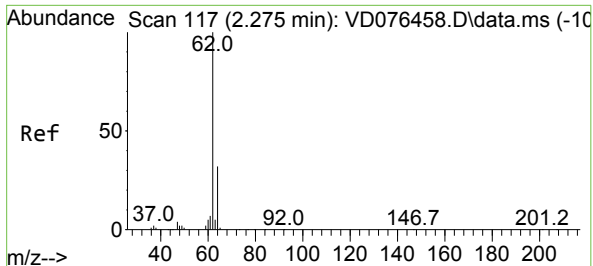

#4
 Vinyl Chloride
 Concen: 1.237 ug/l
 RT: 2.264 min Scan# 115
 Delta R.T. -0.012 min
 Lab File: VD076488.D
 Acq: 20 Jun 2023 13:16




Instrument :
 MSVOA_D
 ClientSampleId :
 SB-01-4.0-6.0


Tgt Ion: 62 Resp: 136
 Ion Ratio Lower Upper
 62 100
 64 0.0 26.0 39.0#

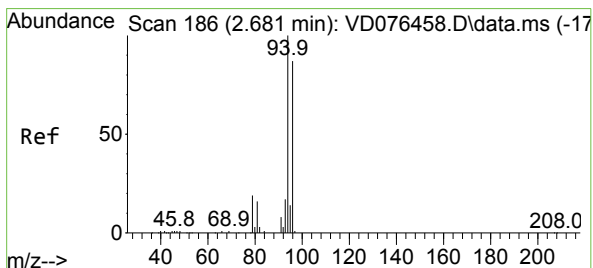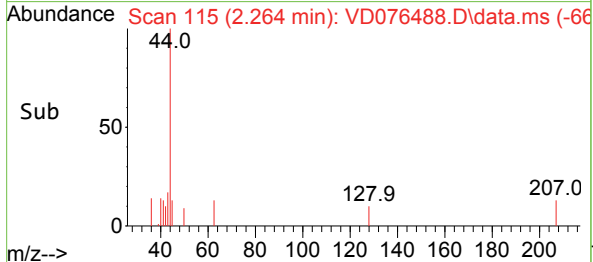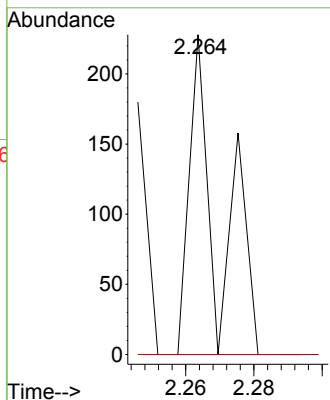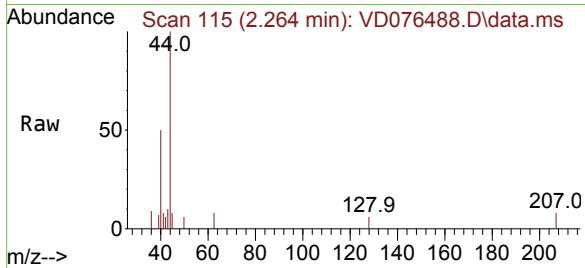

#5
 Bromomethane
 Concen: 4.198 ug/l
 RT: 2.693 min Scan# 188
 Delta R.T. 0.012 min
 Lab File: VD076488.D
 Acq: 20 Jun 2023 13:16

Tgt Ion: 94 Resp: 300
 Ion Ratio Lower Upper
 94 100
 96 236.7 75.8 113.8#


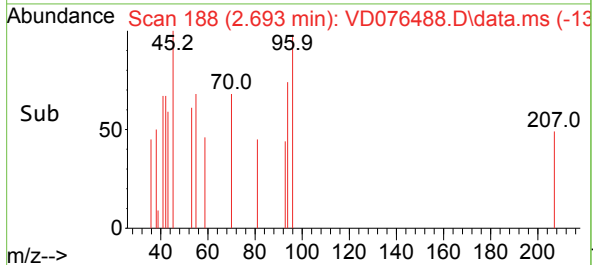
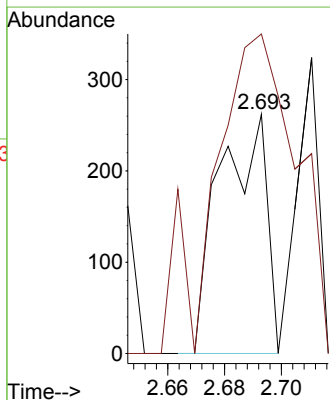
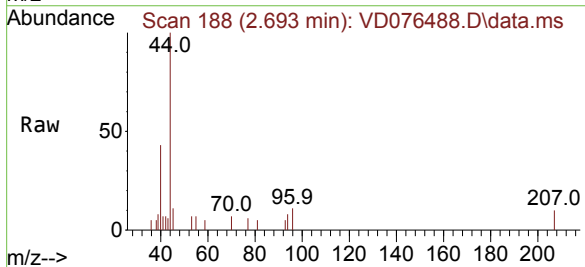




#6
Chloroethane
Concen: 1.938 ug/l
RT: 2.934 min Scan# 211
Delta R.T. 0.106 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 64 Resp: 146
Ion Ratio Lower Upper
64 100
66 0.0 25.5 38.3#

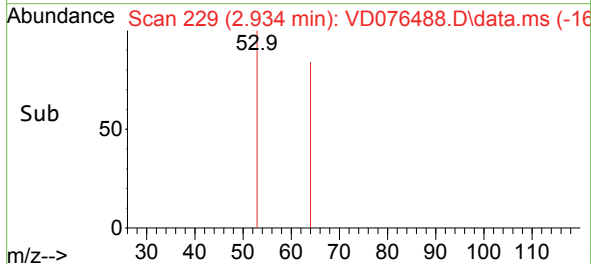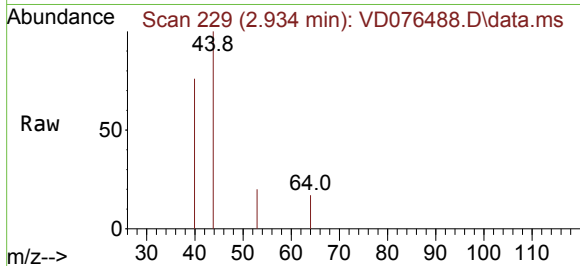

#11
Tert butyl alcohol
Concen: 12.422 ug/l
RT: 4.981 min Scan# 577
Delta R.T. -0.077 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 59 Resp: 67
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




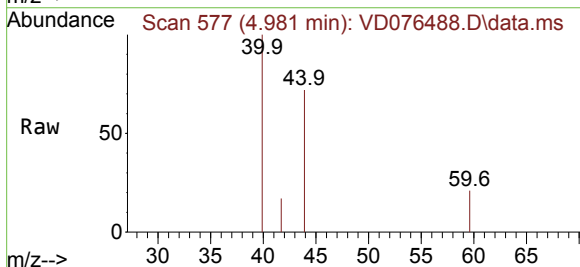




#13
Acrolein
Concen: 9.295 ug/l
RT: 3.940 min Scan# 40
Delta R.T. 0.147 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 56 Resp: 54
Ion Ratio Lower Upper
56 100
55 0.0 55.1 82.7#

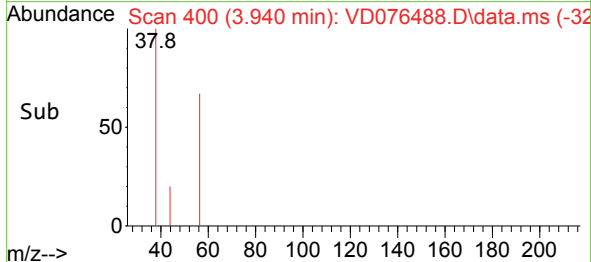

#15
Acrylonitrile
Concen: 3.370 ug/l
RT: 5.175 min Scan# 610
Delta R.T. -0.077 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 53 Resp: 59
Ion Ratio Lower Upper
53 100
52 0.0 65.0 97.4#
51 0.0 28.3 42.5#




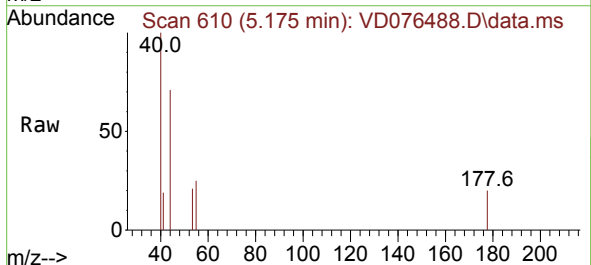


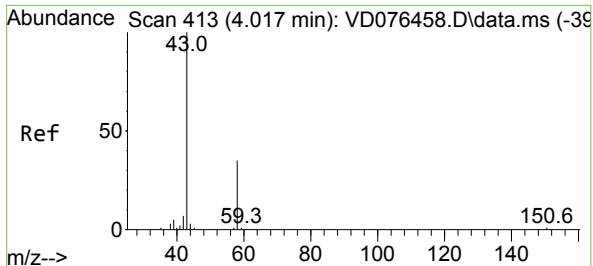

#16
Acetone
Concen: 109.584 ug/l
RT: 4.022 min Scan# 413
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 43 Resp: 1629
Ion Ratio Lower Upper
43 100
58 0.0 34.7 52.1#

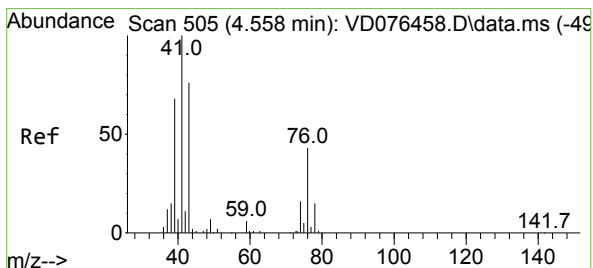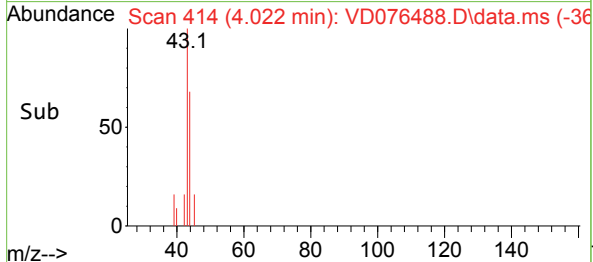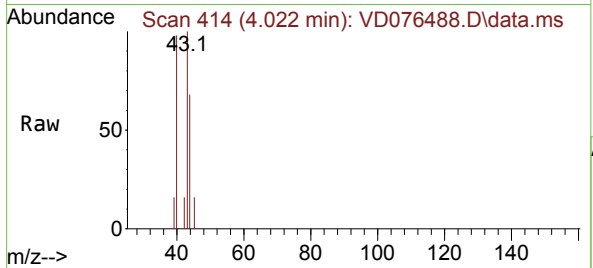

#18
Methyl Acetate
Concen: 2.204 ug/l
RT: 4.569 min Scan# 507
Delta R.T. 0.012 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16


Tgt Ion: 43 Resp: 151
Ion Ratio Lower Upper
43 100
74 0.0 26.4 39.6#

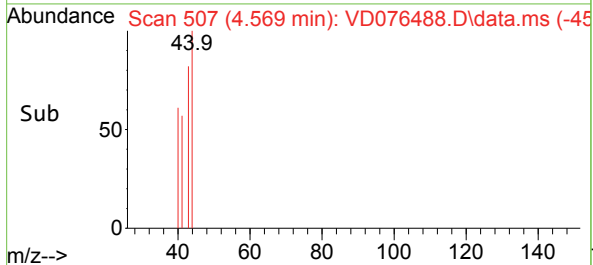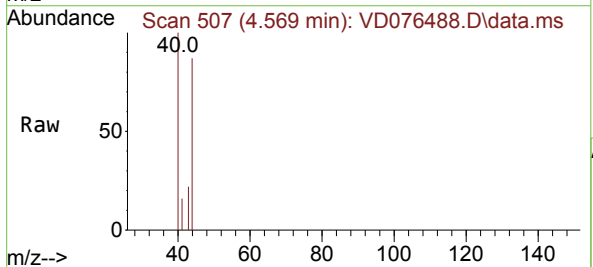



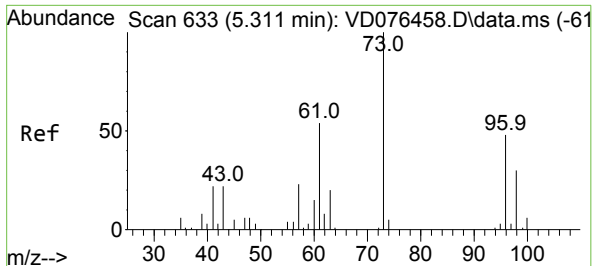


#21
trans-1,2-Dichloroethene
Concen: 1.319 ug/l
RT: 5.310 min Scan# 611
Delta R.T. -0.000 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0



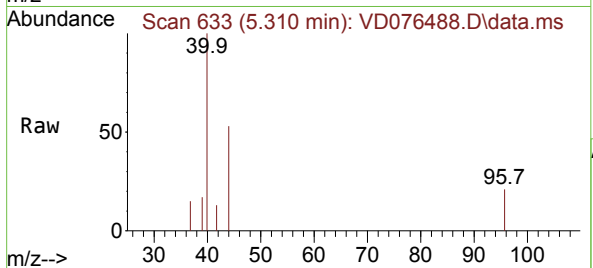



Tgt Ion: 96 Resp: 87
Ion Ratio Lower Upper
96 100
61 0.0 89.3 133.9#
98 0.0 48.6 73.0#

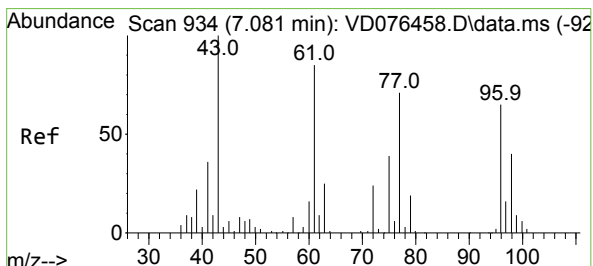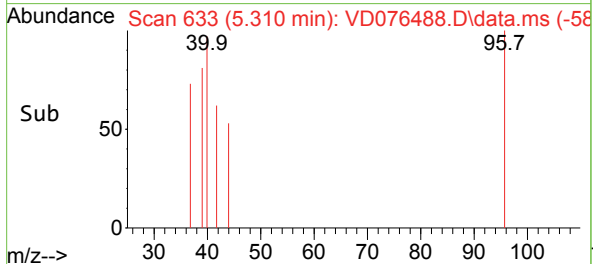

#25
2-Butanone
Concen: 6.785 ug/l
RT: 7.087 min Scan# 935
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 43 Resp: 156
Ion Ratio Lower Upper
43 100
72 0.0 30.7 46.1#


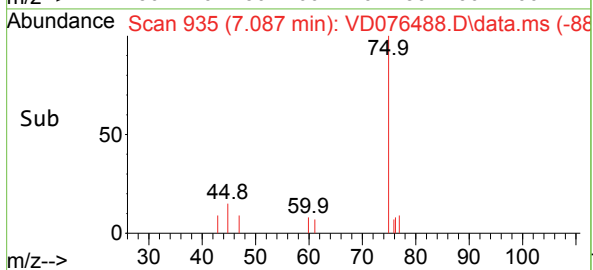

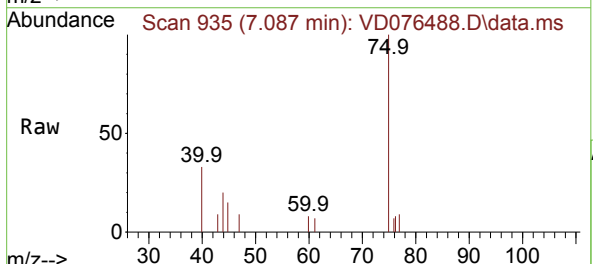




#26
2,2-Dichloropropane
Concen: 7.687 ug/l
RT: 7.063 min Scan# 91
Delta R.T. -0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 77 Resp: 835
Ion Ratio Lower Upper
77 100
97 0.0 13.2 39.6#



#29
Tetrahydrofuran
Concen: 5.347 ug/l
RT: 7.452 min Scan# 997
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 42 Resp: 79
Ion Ratio Lower Upper
42 100
72 0.0 46.5 69.7#
71 0.0 44.5 66.7#

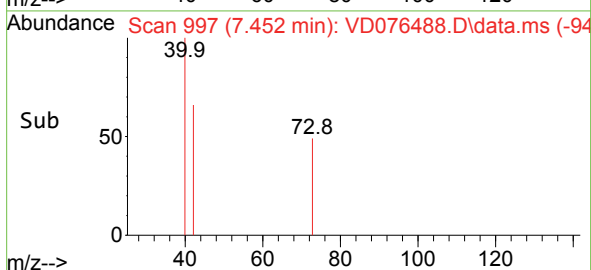



#33

1,2-Dichloroethane-d4

Concen: 91.805 ug/l

RT: 8.228 min Scan# 1129

Delta R.T. -0.000 min

Lab File: VD076488.D

Acq: 20 Jun 2023 13:16

Instrument :

MSVOA_D

ClientSampleId :





SB-01-4.0-6.0

Tgt Ion: 65 Resp: 5735

Ion Ratio Lower Upper

65 100

67 57.2 0.0 115.0

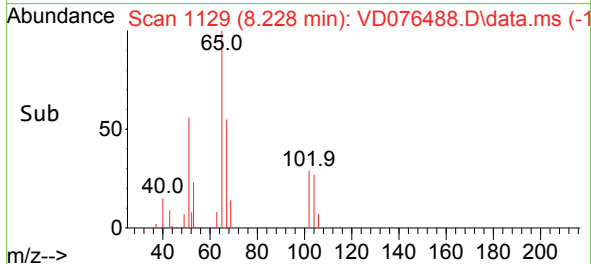

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1222

Delta R.T. -0.000 min

Lab File: VD076488.D

Acq: 20 Jun 2023 13:16




Tgt Ion: 114 Resp: 10658


Ion Ratio Lower Upper

114 100

63 15.2 0.0 33.4

88 15.8 0.0 26.2


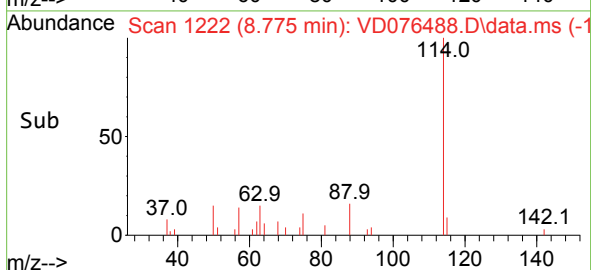






#35
 Dibromofluoromethane
 Concen: 70.030 ug/l
 RT: 7.804 min Scan# 1057
 Delta R.T. -0.000 min
 Lab File: VD076488.D
 Acq: 20 Jun 2023 13:16




Instrument :
 MSVOA_D
 ClientSampleId :
 SB-01-4.0-6.0


Tgt Ion:	113	Resp:	4434
Ion	Ratio	Lower	Upper
113	100		
111	93.3	84.7	127.1
192	19.0	16.8	25.2

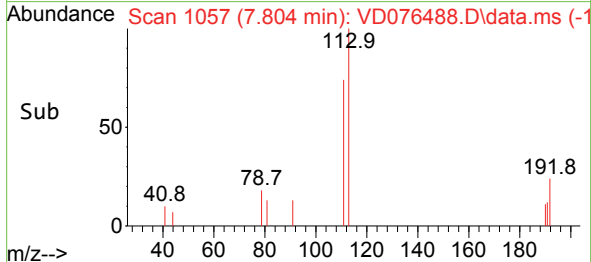

#37
 Ethyl Acetate
 Concen: 1.479 ug/l
 RT: 7.199 min Scan# 954
 Delta R.T. 0.029 min
 Lab File: VD076488.D
 Acq: 20 Jun 2023 13:16

Tgt Ion:	43	Resp:	76
Ion	Ratio	Lower	Upper
43	100		
61	0.0	14.9	22.3#
70	0.0	10.0	15.0#

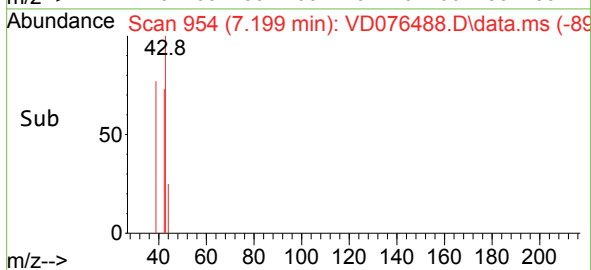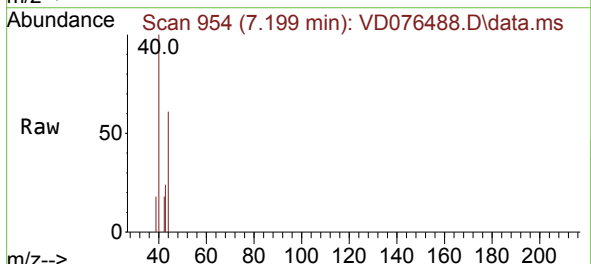



#38

Carbon Tetrachloride

Concen: 5.224 ug/l

RT: 7.869 min Scan# 1068

Delta R.T. -0.118 min

Lab File: VD076488.D


Acq: 20 Jun 2023 13:16

Instrument :

MSVOA_D

ClientSampleId :

SB-01-4.0-6.0






Tgt Ion:117 Resp: 414

Ion Ratio Lower Upper

117 100

119 0.0 78.0 117.0#

121 0.0 24.2 36.2#

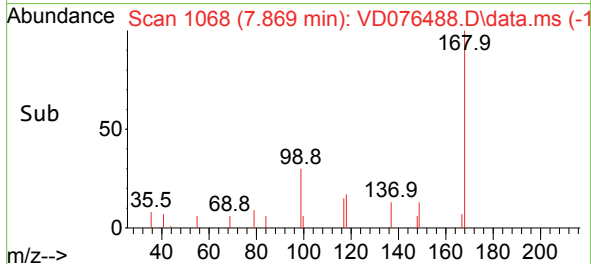

#41

Methacrylonitrile

Concen: 5.205 ug/l

RT: 7.404 min Scan# 989

Delta R.T. 0.006 min

Lab File: VD076488.D

Acq: 20 Jun 2023 13:16

Tgt Ion: 41 Resp: 151




Ion Ratio Lower Upper


41 100

39 47.7 34.0 51.0

67 0.0 77.0 115.4#


52 0.0 27.9 41.9#








#43
Isopropyl Acetate
Concen: 1.347 ug/l
RT: 8.346 min Scan# 1149
Delta R.T. -0.012 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0







Tgt Ion: 43 Resp: 131
Ion Ratio Lower Upper
43 100
61 0.0 31.4 47.0#
87 0.0 14.9 22.3#

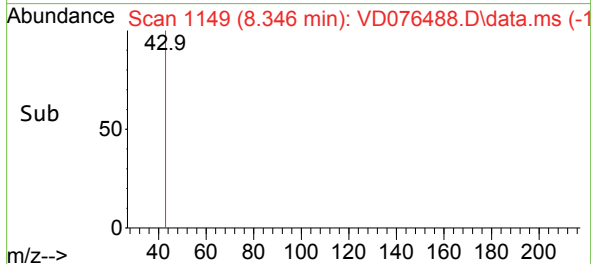

#46
Dibromomethane
Concen: 1.375 ug/l
RT: 9.440 min Scan# 1335
Delta R.T. 0.047 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 93 Resp: 54
Ion Ratio Lower Upper
93 100
95 0.0 67.7 101.5#
174 0.0 85.4 128.2#









#48
Methyl methacrylate
Concen: 3.993 ug/l
RT: 9.387 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 41 Resp: 178
Ion Ratio Lower Upper
41 100
69 0.0 102.2 153.2#
39 0.0 41.4 62.2#

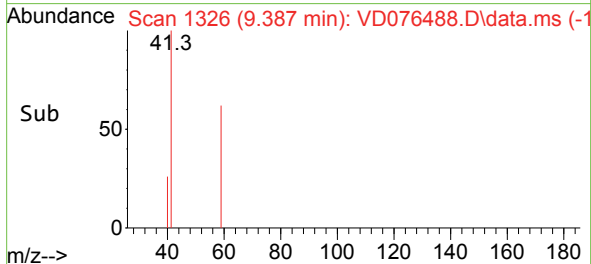

#50
Toluene-d8
Concen: 54.593 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 98 Resp: 13109
Ion Ratio Lower Upper
98 100
100 66.6 50.3 75.5


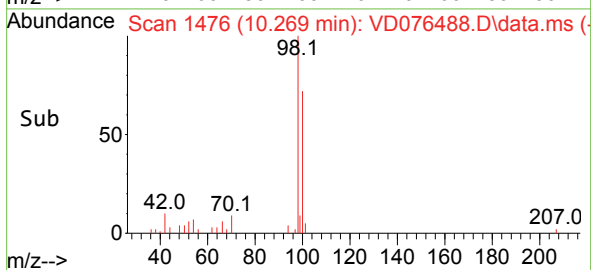

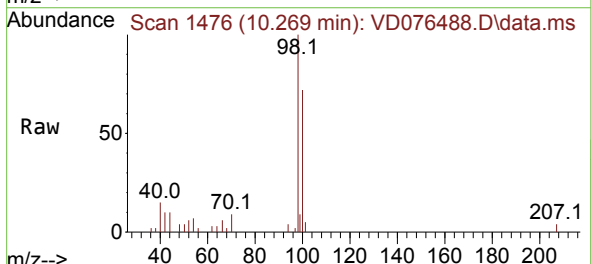




#51
4-Methyl-2-Pentanone
Concen: 2.856 ug/l
RT: 10.410 min Scan# 1457
Delta R.T. 0.253 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 43 Resp: 142
Ion Ratio Lower Upper
43 100
58 47.9 38.9 58.3

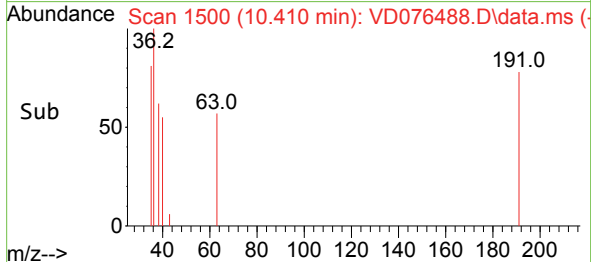

#58
2-Chloroethyl Vinyl ether
Concen: 1.907 ug/l
RT: 9.910 min Scan# 1415
Delta R.T. 0.041 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 63 Resp: 58
Ion Ratio Lower Upper
63 100
106 0.0 25.3 37.9#


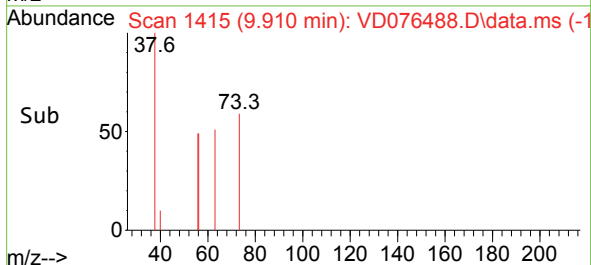




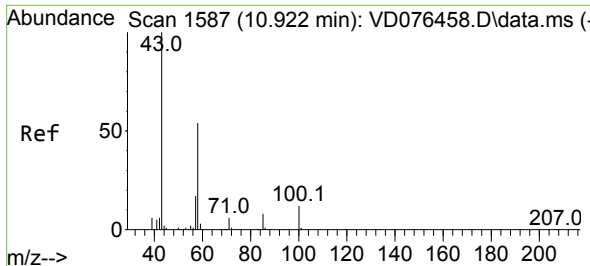

#59
2-Hexanone
Concen: 3.788 ug/l
RT: 10.810 min Scan# 1568
Delta R.T. -0.112 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 43 Resp: 131
Ion Ratio Lower Upper
43 100
58 44.3 34.1 102.2

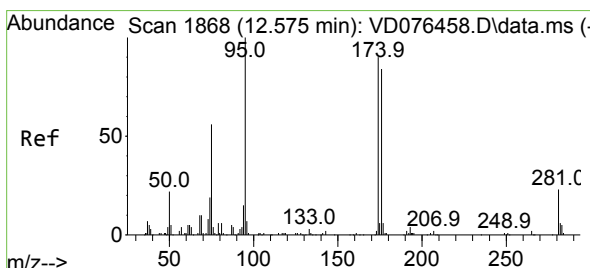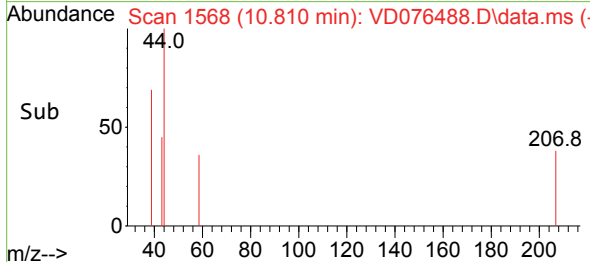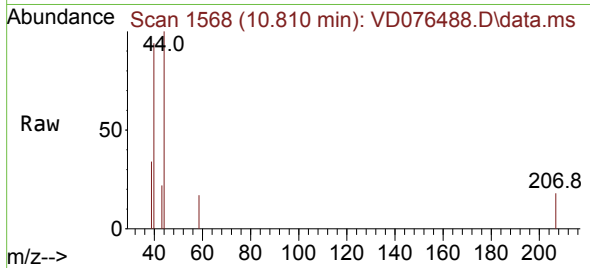

#62
4-Bromofluorobenzene
Concen: 66.906 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 95 Resp: 5214
Ion Ratio Lower Upper
95 100
174 82.4 0.0 201.8
176 72.7 0.0 191.8


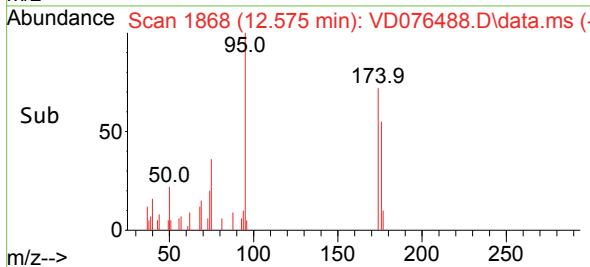

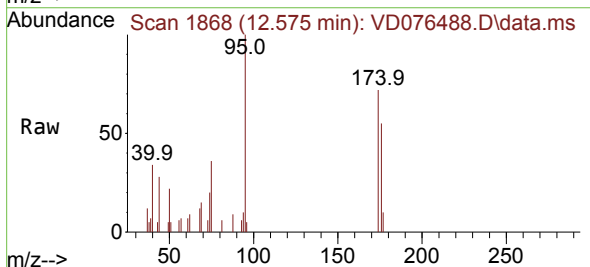




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.587 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion:117	Resp:	11595
Ion Ratio	Lower	Upper
117	100	
82	46.5	38.3 57.5
119	27.7	25.0 37.4

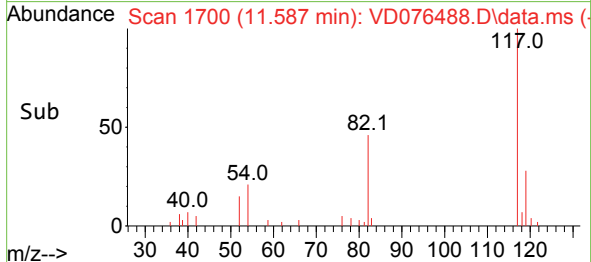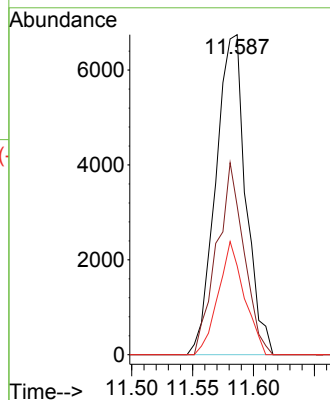

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion:152	Resp:	5548
Ion Ratio	Lower	Upper
152	100	
115	57.4	27.1 81.3
150	153.6	0.0 353.6



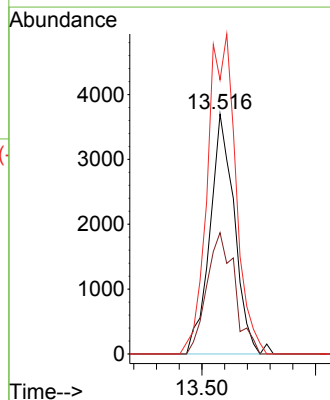
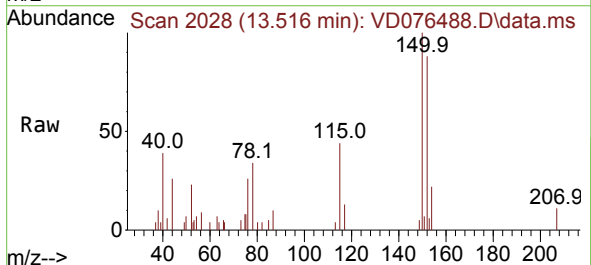




#76
1,2,3-Trichloropropane
Concen: 48.527 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.153 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 75 Resp: 2672
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

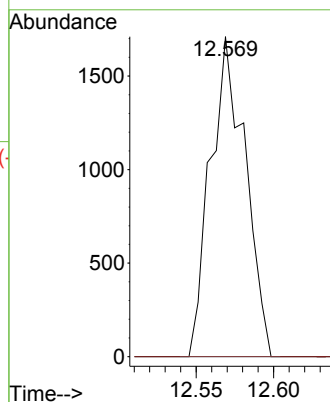

#81
trans-1,4-Dichloro-2-butene
Concen: 3.820 ug/l
RT: 12.369 min Scan# 1833
Delta R.T. -0.100 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion: 75 Resp: 96
Ion Ratio Lower Upper
75 100
53 0.0 63.0 94.4#
89 0.0 37.9 56.9#


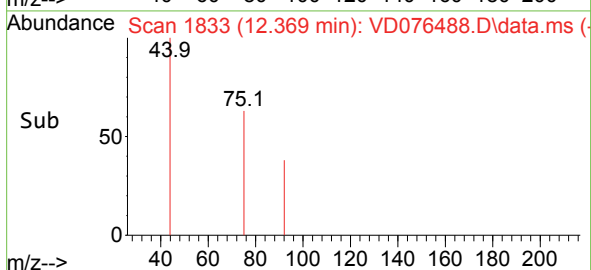
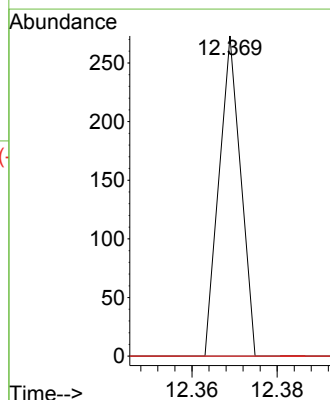



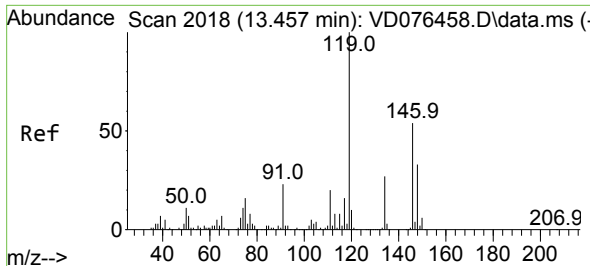

#87
1,3-Dichlorobenzene
Concen: 1.011 ug/l
RT: 13.545 min Scan# 2018
Delta R.T. 0.088 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion:146 Resp: 183
Ion Ratio Lower Upper
146 100
111 45.9 17.9 53.8
148 61.2 32.3 96.8

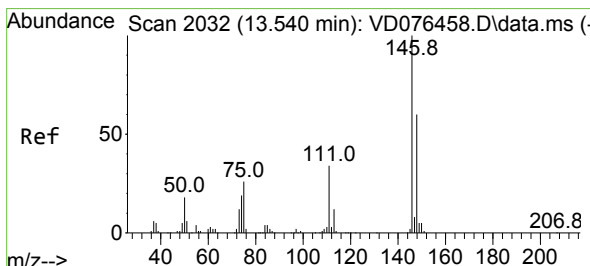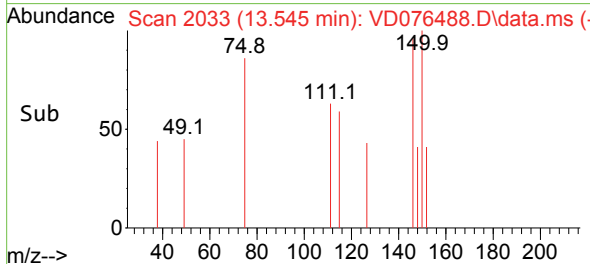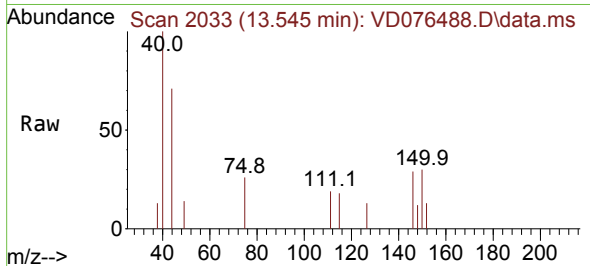

#88
1,4-Dichlorobenzene
Concen: 1.014 ug/l
RT: 13.545 min Scan# 2033
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Tgt Ion:146 Resp: 183
Ion Ratio Lower Upper
146 100
111 45.9 17.4 52.3
148 61.2 31.7 95.1


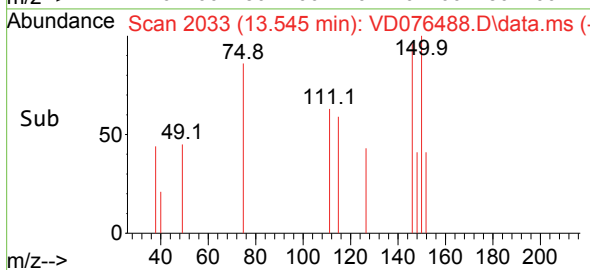

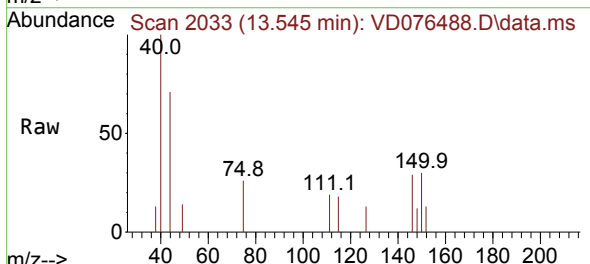




#92
1,2-Dibromo-3-Chloropropane
Concen: 4.741 ug/l
RT: 14.375 min Scan# 2186
Delta R.T. -0.071 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16




Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0


Tgt Ion: 75 Resp: 55
Ion Ratio Lower Upper
75 100
155 0.0 47.9 143.8#
157 0.0 59.9 179.7#

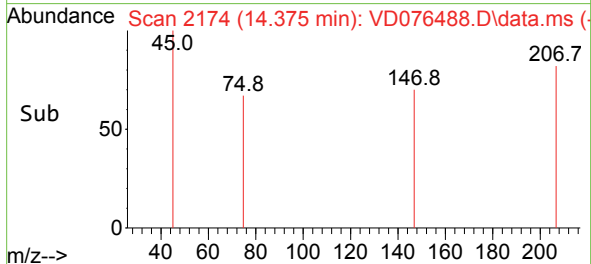

#93
1,2,4-Trichlorobenzene
Concen: 1.413 ug/l
RT: 15.092 min Scan# 2296
Delta R.T. -0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16


Tgt Ion: 180 Resp: 149
Ion Ratio Lower Upper
180 100
182 77.2 48.5 145.6
145 0.0 14.2 42.6#

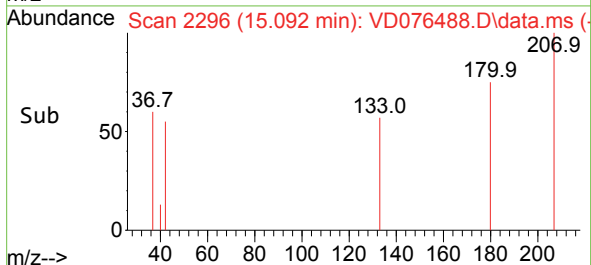

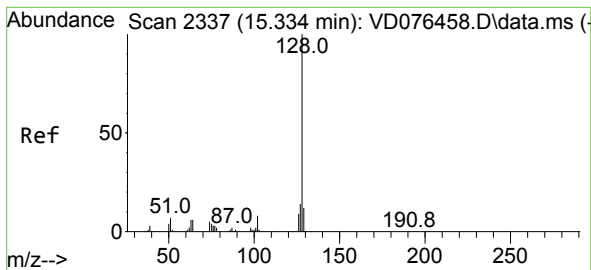

#95
Naphthalene
Concen: 2.353 ug/l
RT: 15.339 min Scan# 21
Delta R.T. 0.006 min
Lab File: VD076488.D
Acq: 20 Jun 2023 13:16

Instrument :
MSVOA_D
ClientSampleId :
SB-01-4.0-6.0

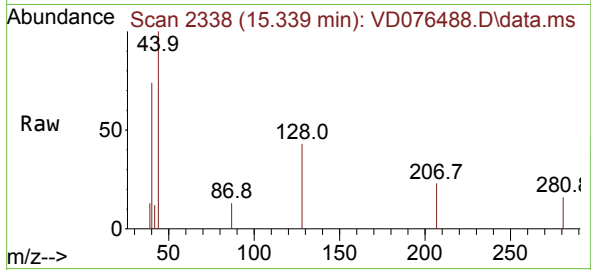

Tgt Ion:128 Resp: 496
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.7 13.1#

