


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062118\
 Data File : VD058268.D
 Acq On : 21 Jun 2018 23:37
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
 Title : SW846 8260
 Last Update : Wed Jun 20 05:52:56 2018

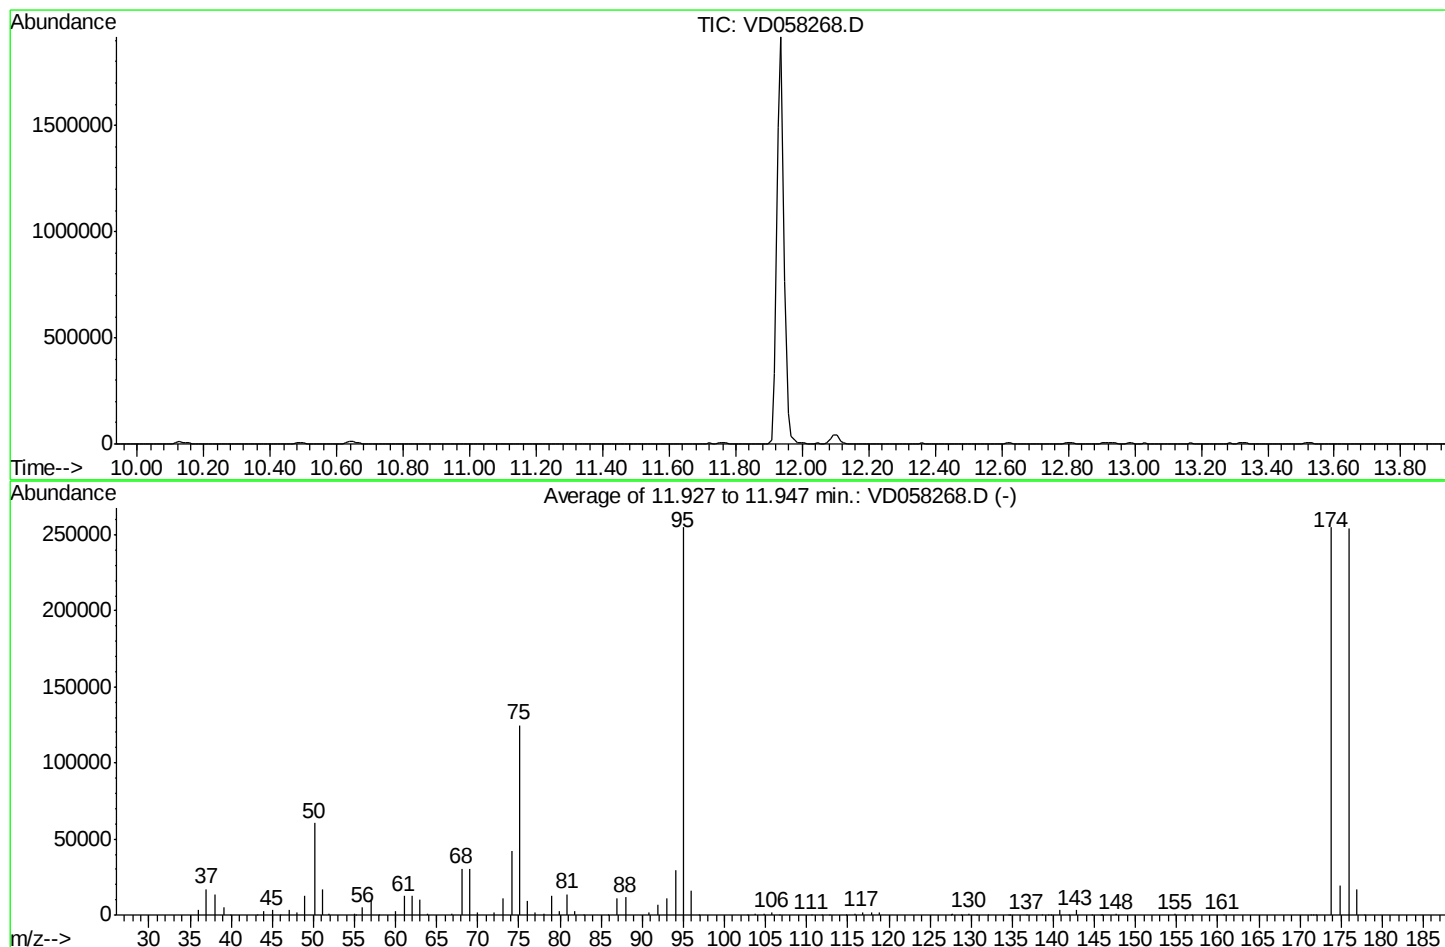

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	60517	PASS
75	95	30	60	49.0	124816	PASS
95	95	100	100	100.0	254965	PASS
96	95	5	9	6.3	16131	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	99.9	254762	PASS
175	174	5	9	7.6	19395	PASS
176	174	95	101	100.0	254656	PASS
177	176	5	9	6.7	16955	PASS