

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062123\
 Data File : VD076525.D
 Acq On : 21 Jun 2023 21:22
 Operator : KP/SY
 Sample : 03355-13
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-07-6.5-7.0

Quant Time: Jun 22 02:04:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.869	168	113963	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	201722	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	175685	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	70067	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	69593	60.950	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	121.900%
35) Dibromofluoromethane	7.804	113	67788	56.567	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	113.140%
50) Toluene-d8	10.269	98	222053	48.859	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.720%
62) 4-Bromofluorobenzene	12.575	95	63136	42.805	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	85.620%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062123\
Data File : VD076525.D
Acq On : 21 Jun 2023 21:22
Operator : KP/SY
Sample : 03355-13
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-07-6.5-7.0


Quant Time: Jun 22 02:04:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

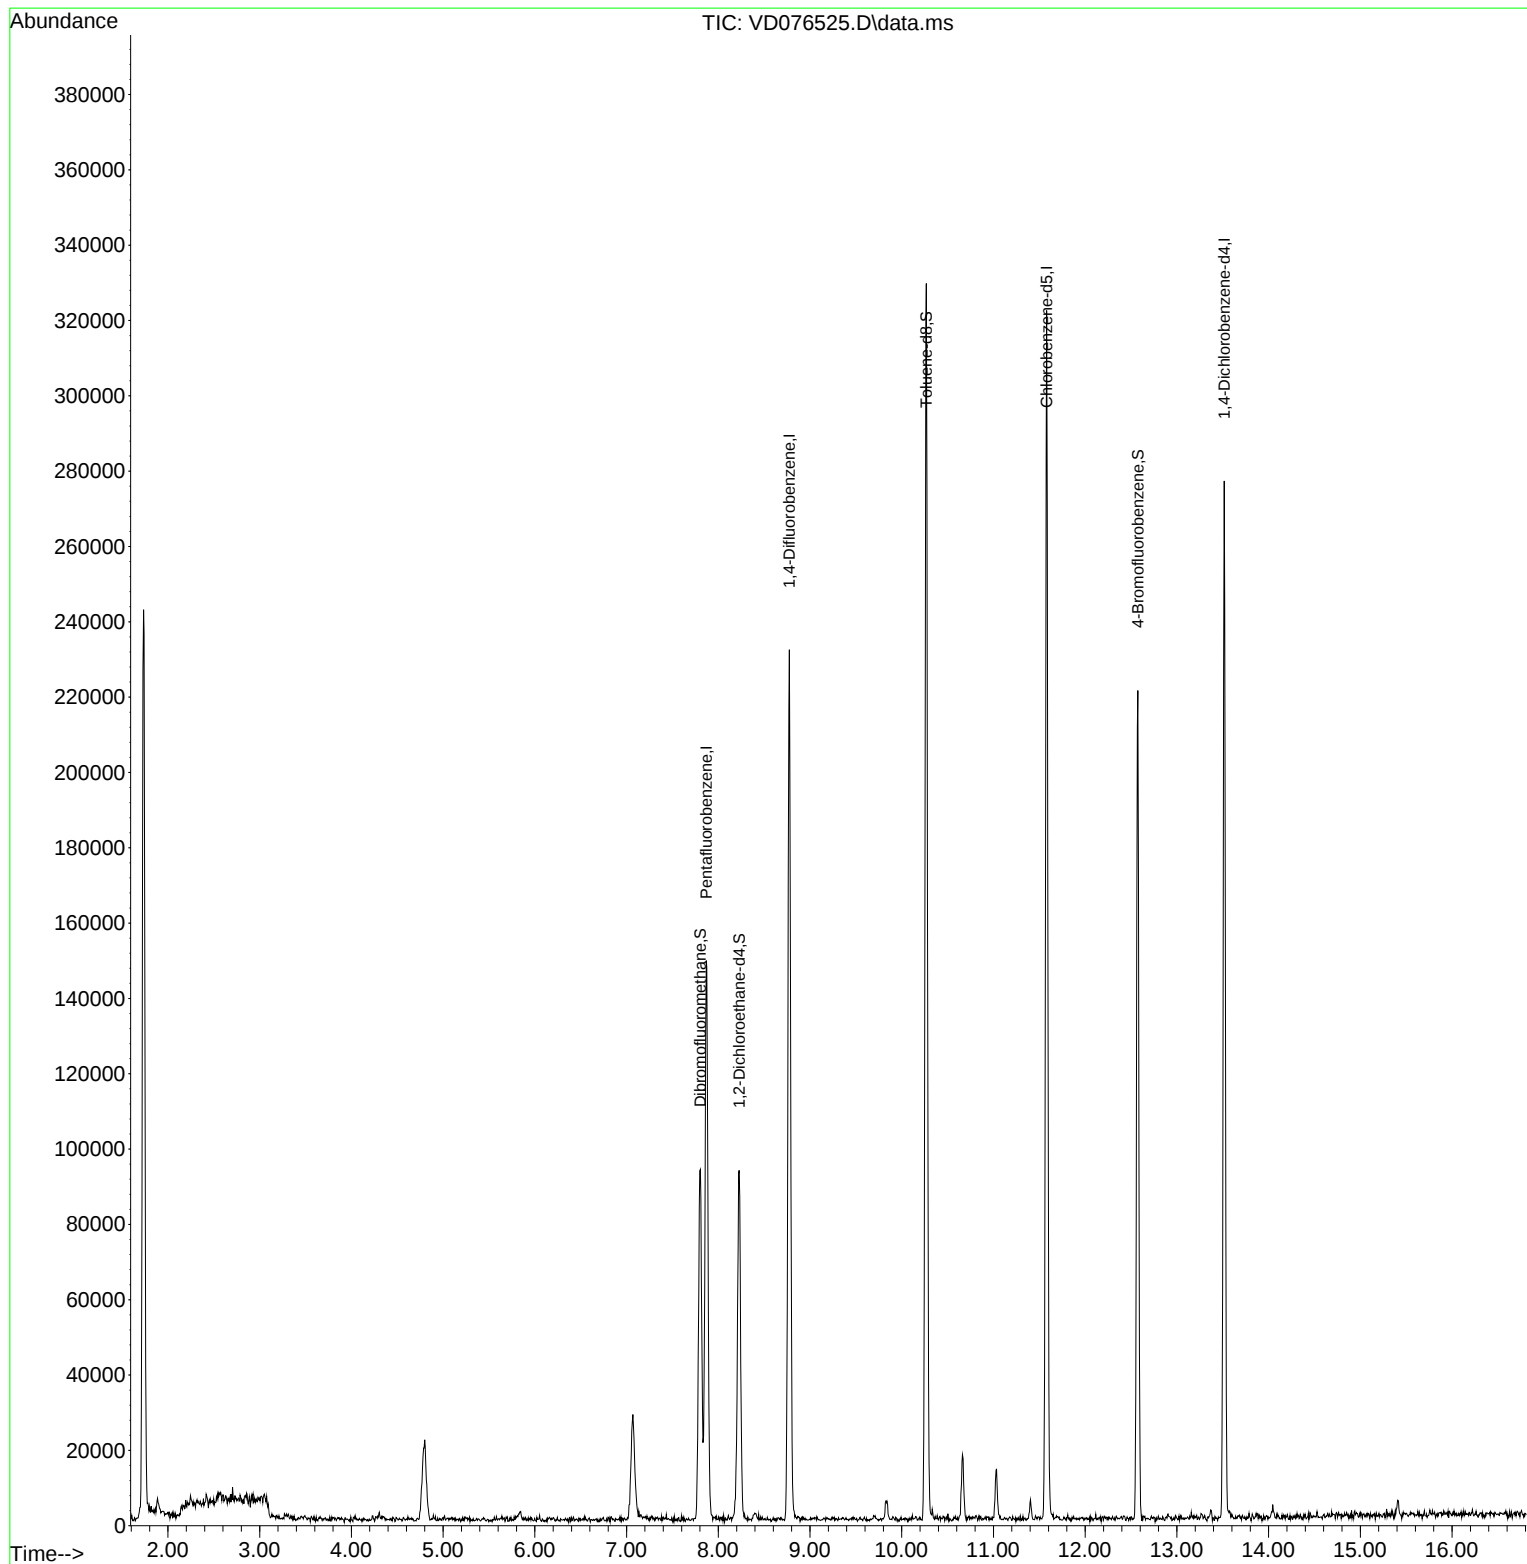



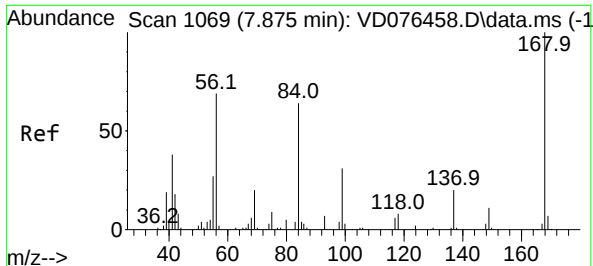


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.869 min Scan# 1106
Delta R.T. -0.006 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22

Instrument :
MSVOA_D
ClientSampleId :
SB-07-6.5-7.0



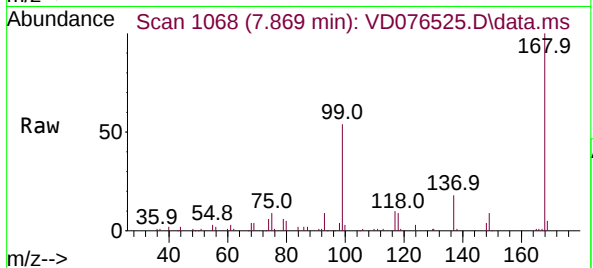



Tgt Ion:168 Resp: 113963
Ion Ratio Lower Upper
168 100
99 54.2 36.7 55.1

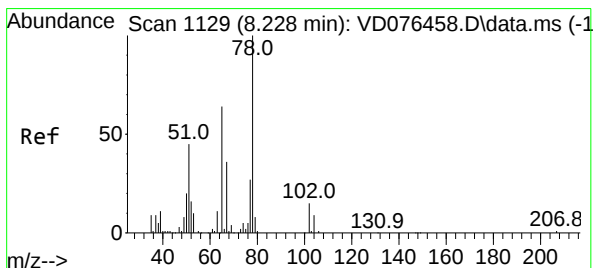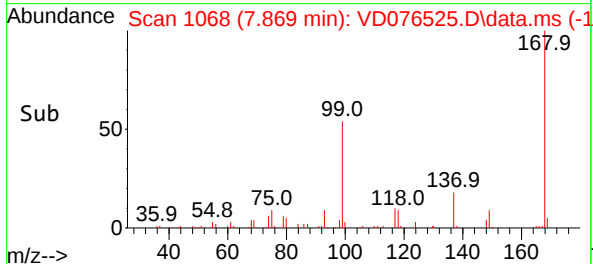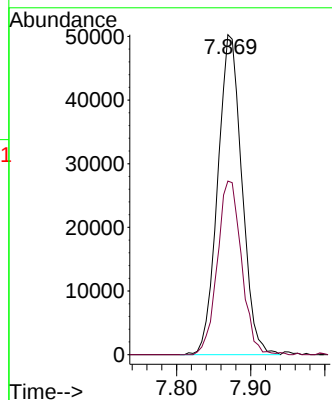

#33
1,2-Dichloroethane-d4
Concen: 60.950 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22

Tgt Ion: 65 Resp: 69593
Ion Ratio Lower Upper
65 100
67 55.9 0.0 115.0

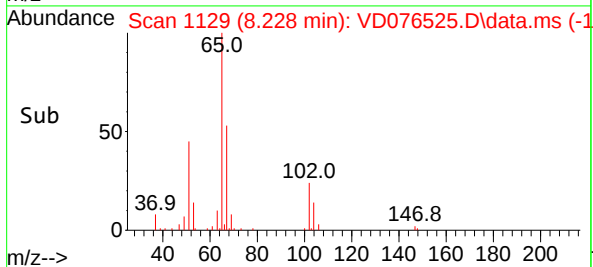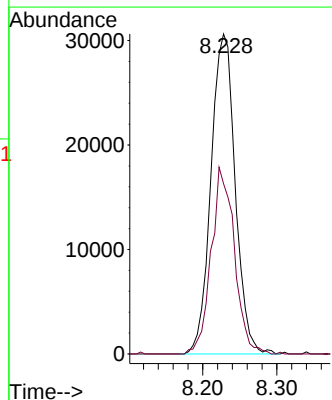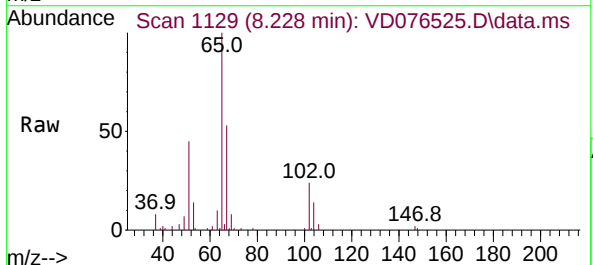

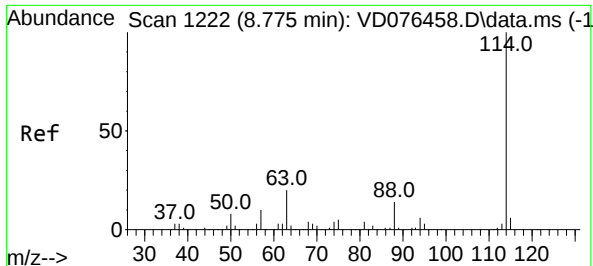

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076525.D

Acq: 21 Jun 2023 21:22

Instrument :

MSVOA_D

ClientSampleId :

SB-07-6.5-7.0





Tgt Ion:114 Resp: 201722

Ion Ratio Lower Upper

114 100

63 20.2 0.0 33.4

88 15.1 0.0 26.2

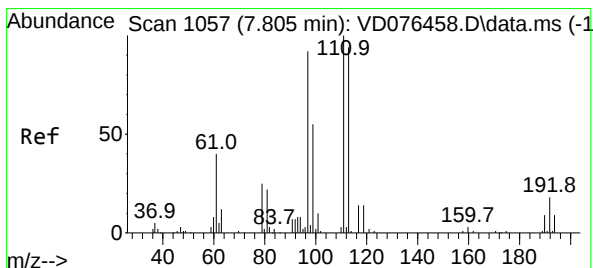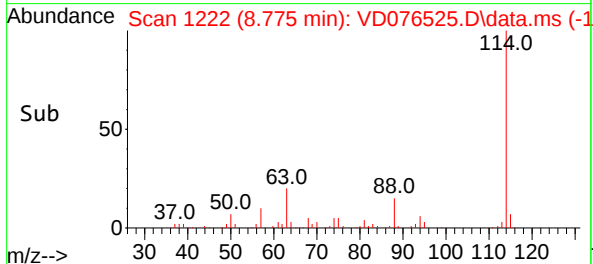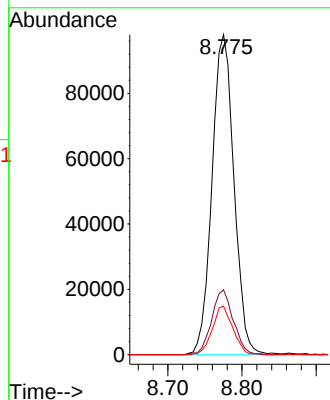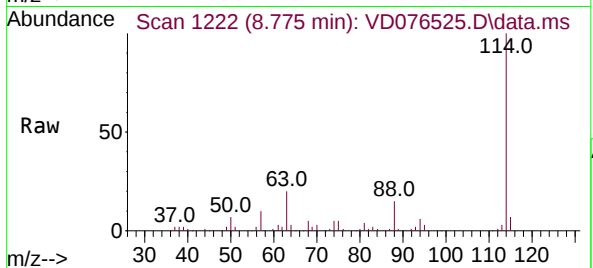

#35

Dibromofluoromethane

Concen: 56.567 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076525.D

Acq: 21 Jun 2023 21:22




Tgt Ion:113 Resp: 67788


Ion Ratio Lower Upper

113 100

111 104.6 84.7 127.1

192 19.3 16.8 25.2

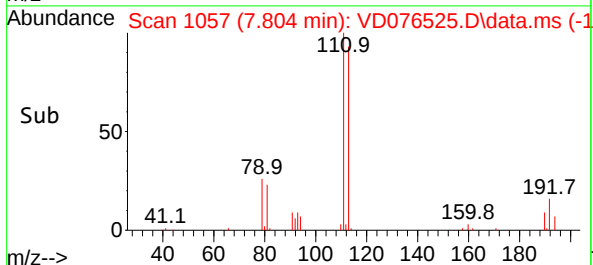
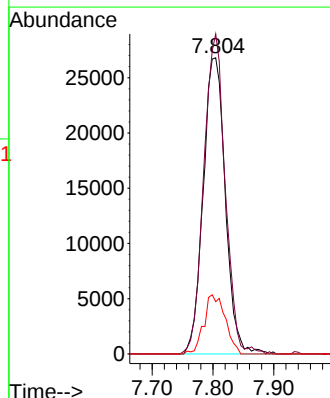
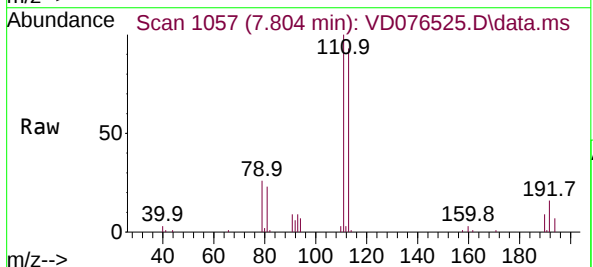


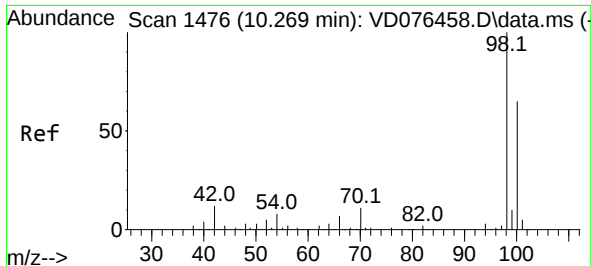

#50
Toluene-d8
Concen: 48.859 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22




Instrument :
MSVOA_D
ClientSampleId :
SB-07-6.5-7.0


Tgt Ion: 98 Resp: 222053
Ion Ratio Lower Upper
98 100
100 64.7 50.3 75.5

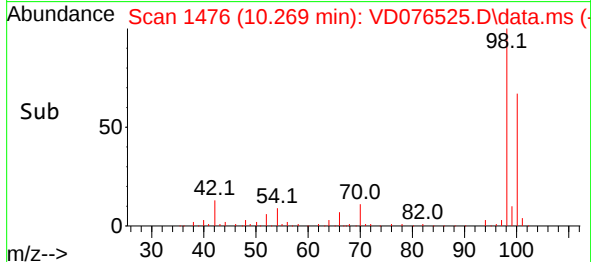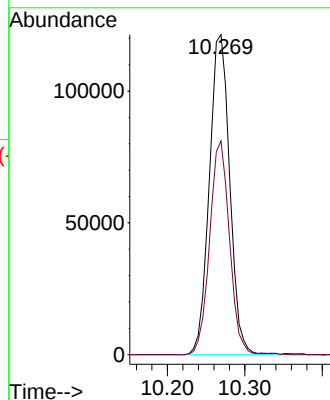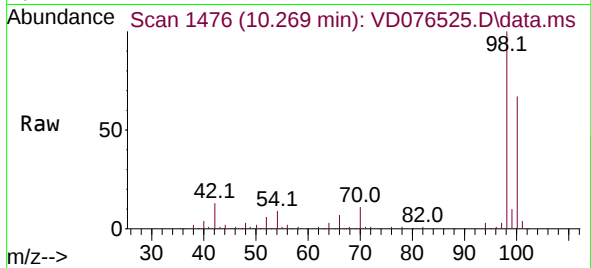

#62
4-Bromofluorobenzene
Concen: 42.805 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22

Tgt Ion: 95 Resp: 63136
Ion Ratio Lower Upper
95 100
174 93.2 0.0 201.8
176 89.4 0.0 191.8


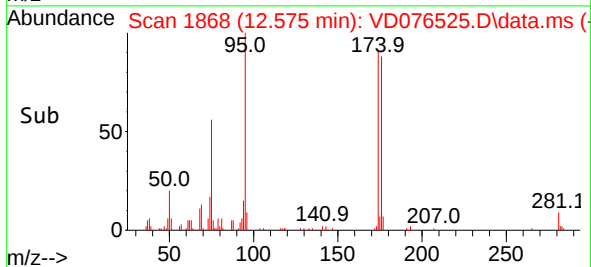
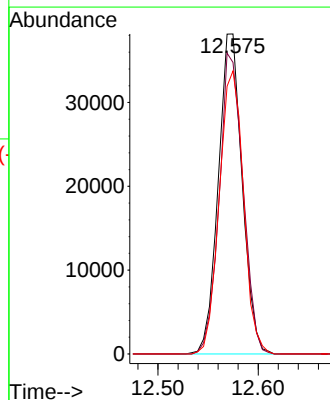
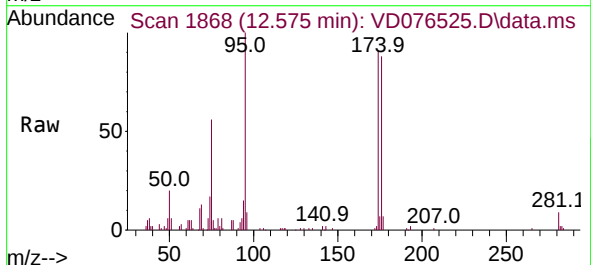


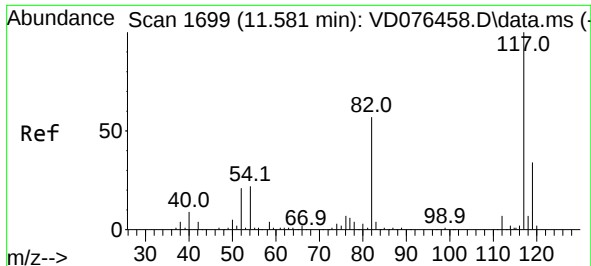

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22

Instrument :
MSVOA_D
ClientSampleId :
SB-07-6.5-7.0

Tgt Ion:117 Resp: 175685
Ion Ratio Lower Upper
117 100
82 52.8 38.3 57.5
119 31.9 25.0 37.4

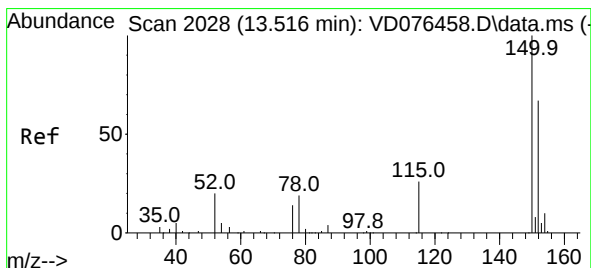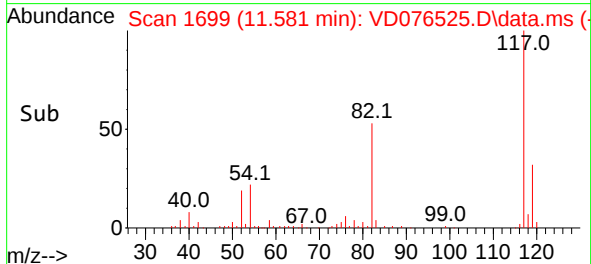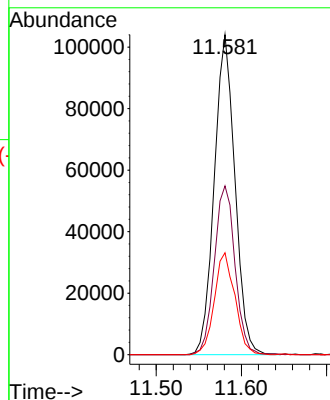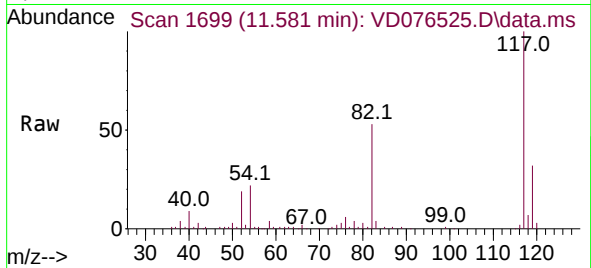

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076525.D
Acq: 21 Jun 2023 21:22

Tgt Ion:152 Resp: 70067
Ion Ratio Lower Upper
152 100
115 57.2 27.1 81.3
150 159.3 0.0 353.6

